
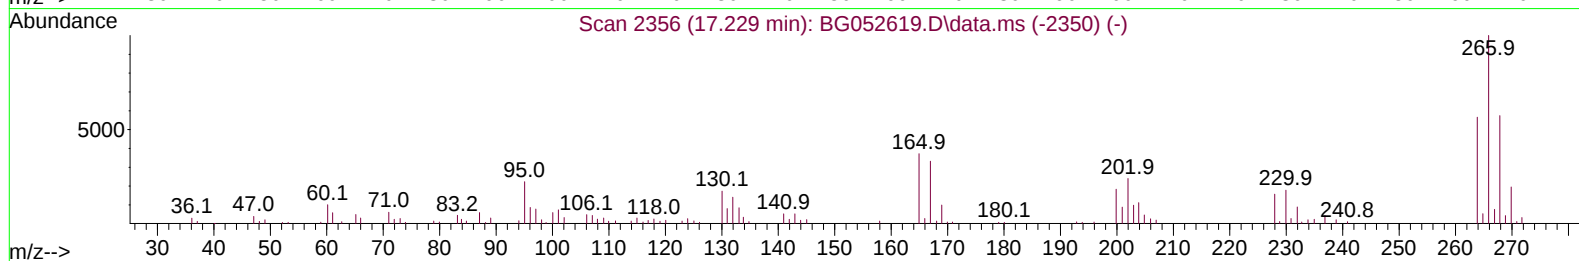
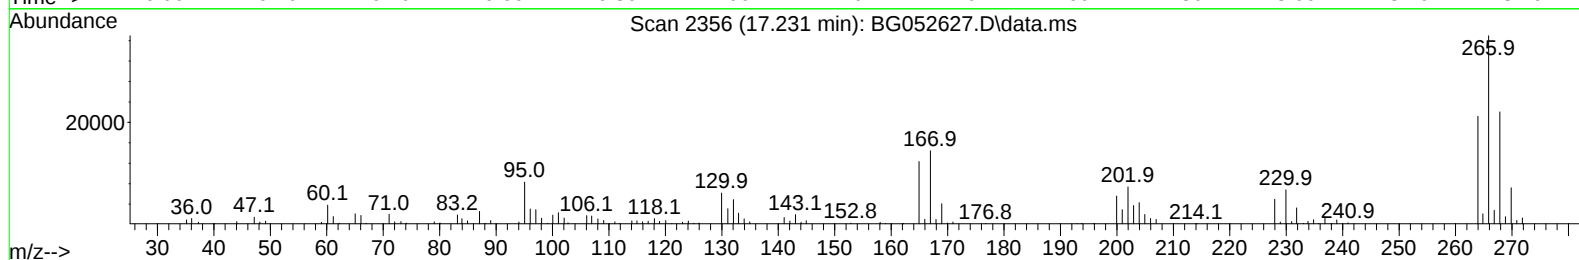


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
Data File : BG052627.D
Acq On : 10 Mar 2022 10:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 10 13:13:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 10 06:37:54 2022
Response via : Initial Calibration

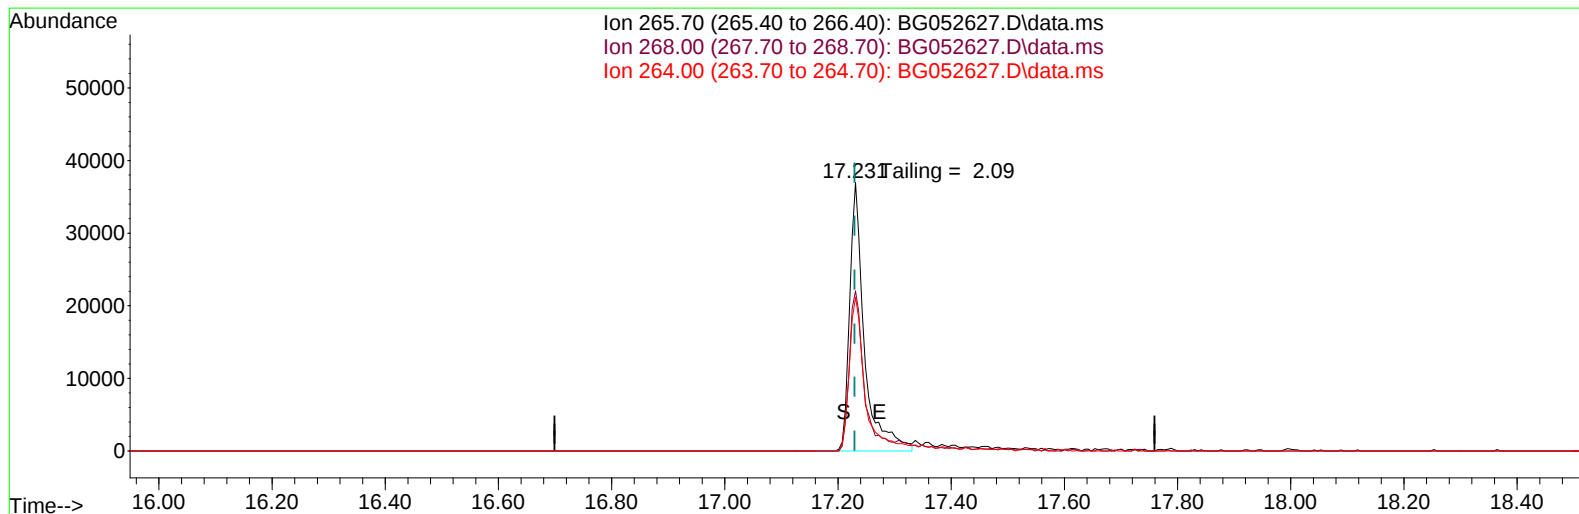

TIC: BG052627.D\data.ms

(70) Pentachlorophenol (C)




17.231min (+ 0.002) 34429.96 ng

response 67147

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	59.68
264.00	56.60	57.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
Data File : BG052627.D
Acq On : 10 Mar 2022 10:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 10 13:13:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 10 06:37:54 2022
Response via : Initial Calibration

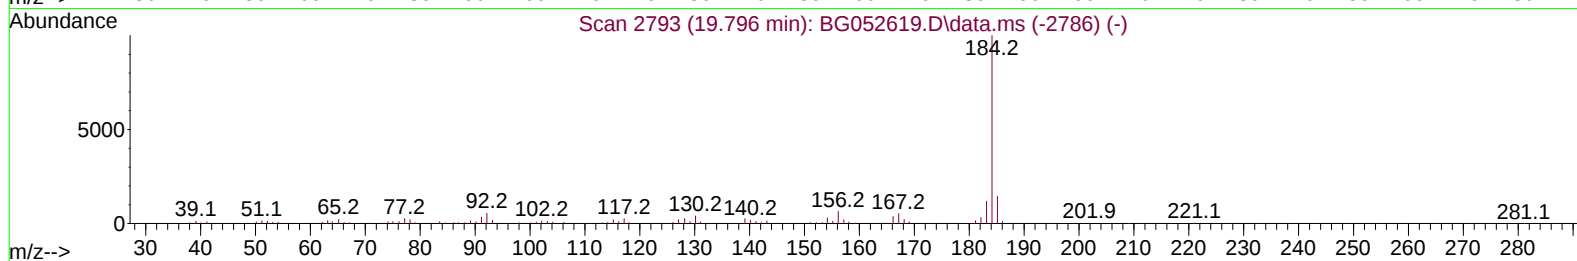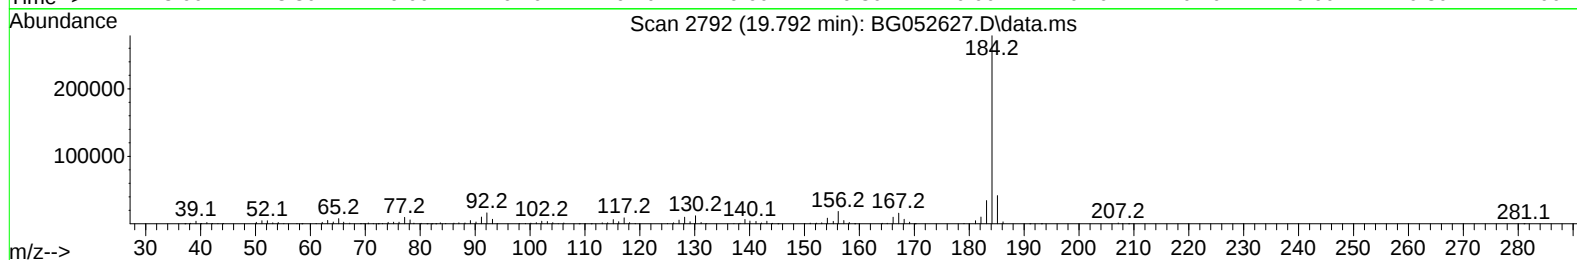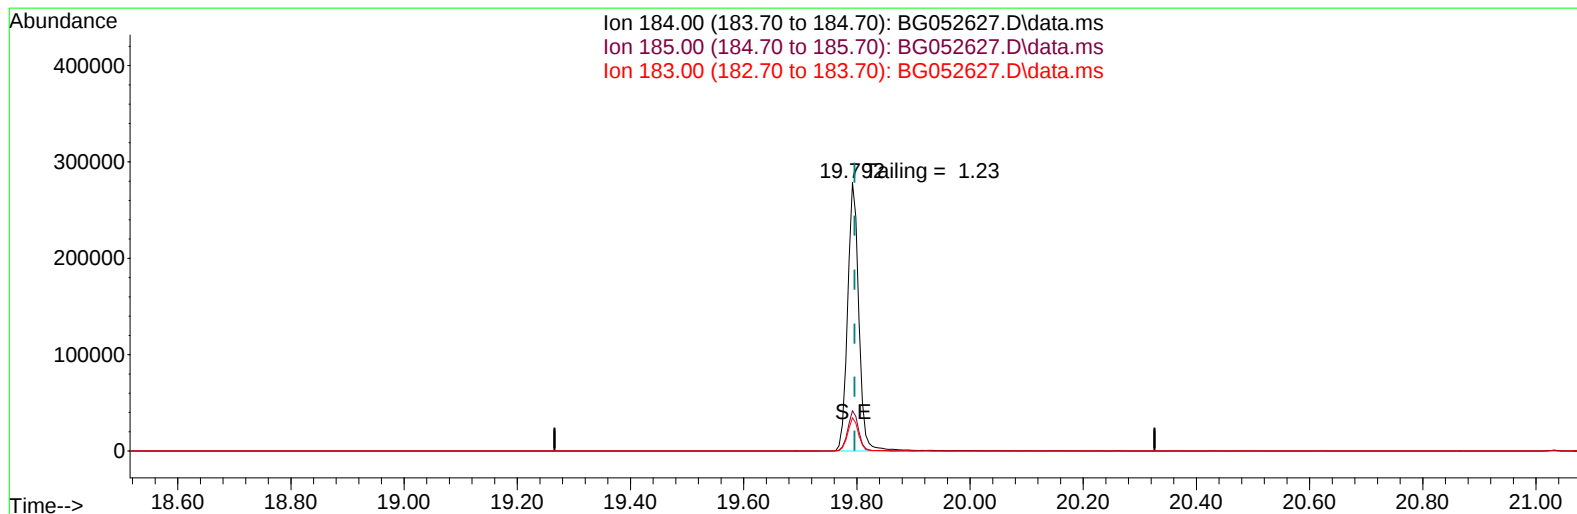

TIC: BG052627.D\data.ms

(77) Benzidine**19.792min (-0.004) 204882.35 ng****response 382517**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	15.04
183.00	11.80	12.43
0.00	0.00	0.00