

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
 Data File : BG052635.D
 Acq On : 10 Mar 2022 15:41
 Operator : CG/JU
 Sample : N1845-10 2X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SAMPLE-10

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG052635.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.214	306	311	319	rBV3	6229	11168	1.42%	0.210%
2	5.708	388	395	408	rBV	194382	332179	42.33%	6.235%
3	7.329	663	671	685	rBV	230454	428757	54.64%	8.048%
4	8.175	807	815	822	rBV	150379	249552	31.80%	4.684%
5	9.350	1006	1015	1023	rBV	159948	281245	35.84%	5.279%
6	10.765	1251	1256	1264	rBV	12845	22589	2.88%	0.424%
7	11.012	1291	1298	1305	rVB	194160	345732	44.06%	6.489%
8	13.450	1706	1713	1720	rVB	434660	650857	82.94%	12.217%
9	13.638	1740	1745	1748	rBV3	6240	10509	1.34%	0.197%
10	14.825	1940	1947	1955	rVV	299133	469986	59.89%	8.822%
11	15.647	2084	2087	2091	rVB5	6789	9529	1.21%	0.179%
12	15.870	2121	2125	2128	rBV5	5222	8389	1.07%	0.157%
13	16.058	2151	2157	2161	rBV6	4468	8092	1.03%	0.152%
14	16.317	2195	2201	2207	rBV	195378	306710	39.09%	5.757%
15	16.540	2237	2239	2246	rVB7	10480	13849	1.76%	0.260%
16	17.227	2352	2356	2362	rBV7	6461	13646	1.74%	0.256%
17	17.304	2365	2369	2375	rVV7	8927	16946	2.16%	0.318%
18	17.362	2375	2379	2382	rBV3	9558	14582	1.86%	0.274%
19	17.462	2392	2396	2400	rBV7	7850	10739	1.37%	0.202%
20	17.580	2409	2416	2420	rBV	349044	531238	67.70%	9.971%
21	17.621	2420	2423	2429	rVB	41795	61704	7.86%	1.158%
22	17.715	2436	2439	2442	rBV3	6527	8732	1.11%	0.164%
23	17.979	2481	2484	2490	rBV7	7204	9782	1.25%	0.184%
24	18.220	2522	2525	2529	rVB2	21172	25140	3.20%	0.472%
25	18.496	2570	2572	2579	rVB3	13983	20142	2.57%	0.378%
26	18.643	2594	2597	2602	rVB7	12174	15969	2.04%	0.300%
27	19.624	2760	2764	2769	rBV	67357	100318	12.78%	1.883%
28	19.988	2823	2826	2833	rVB	73768	108487	13.83%	2.036%
29	20.170	2852	2857	2864	rBV	593432	784708	100.00%	14.729%
30	21.886	3144	3149	3155	rVB	264730	456297	58.15%	8.565%




Sum of corrected areas: 5327573

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
Data File : BG052635.D
Acq On : 10 Mar 2022 15:41
Operator : CG/JU
Sample : N1845-10 2X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SAMPLE-10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

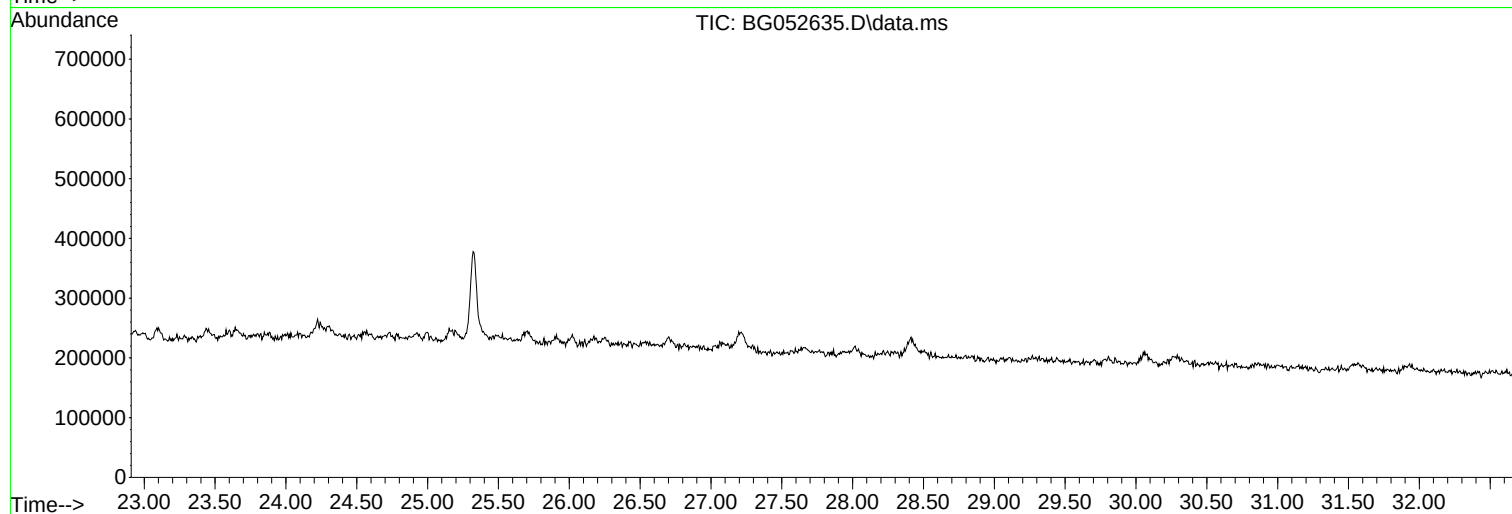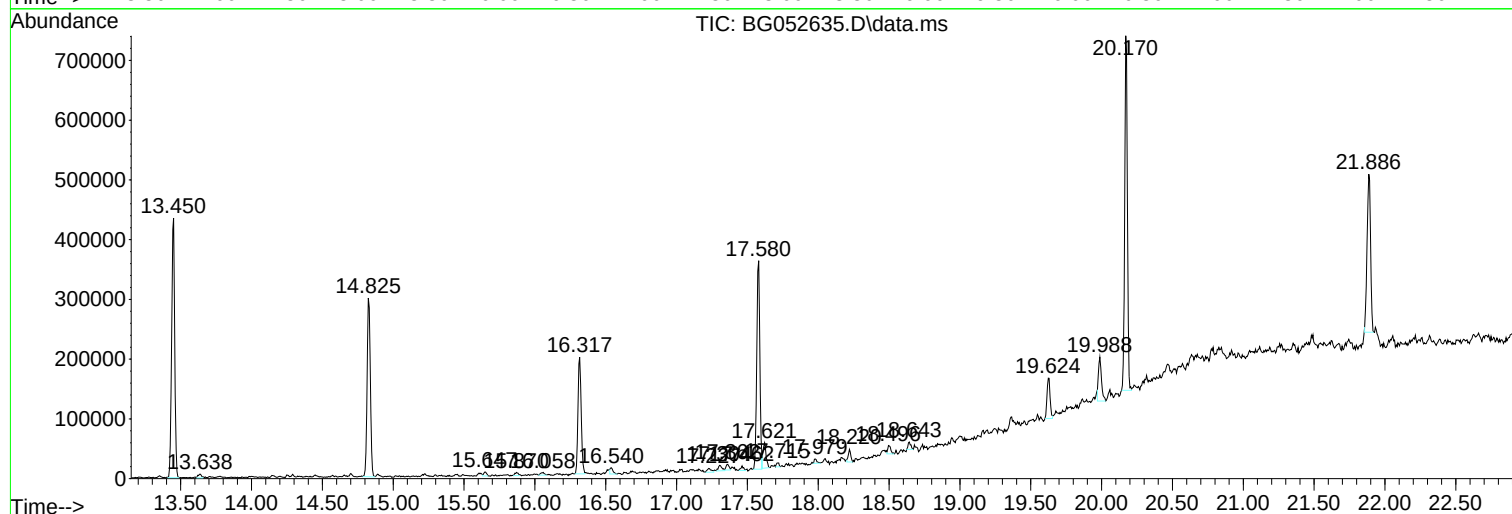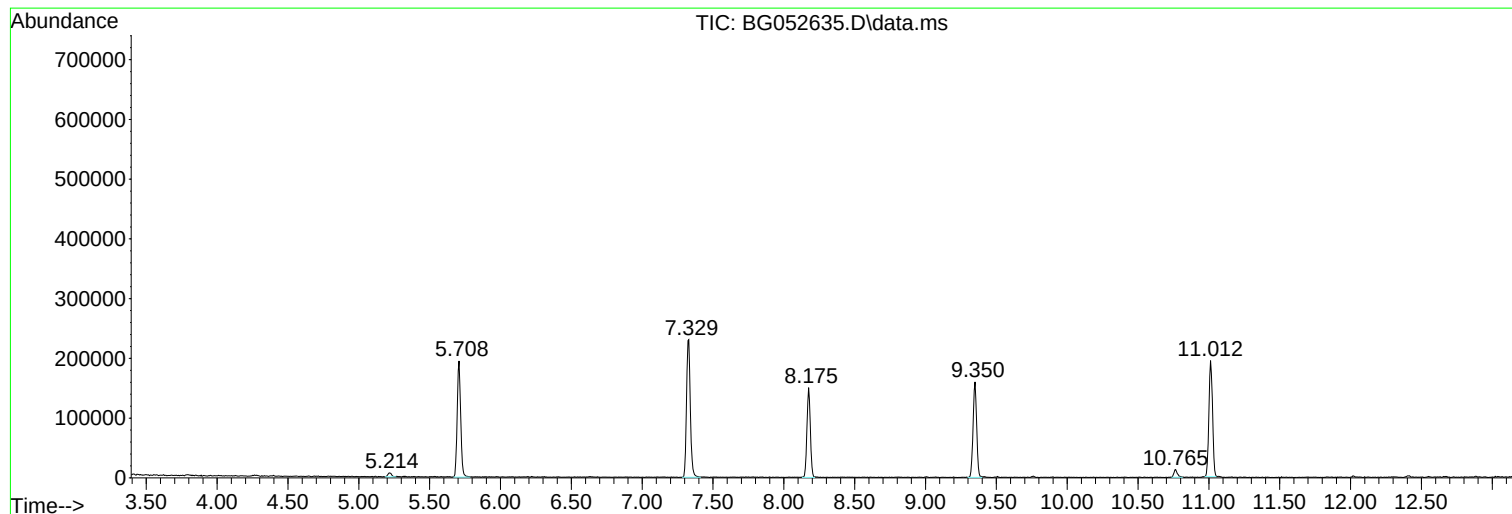

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
Data File : BG052635.D
Acq On : 10 Mar 2022 15:41
Operator : CG/JU
Sample : N1845-10 2X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SAMPLE-10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
Data File : BG052635.D
Acq On : 10 Mar 2022 15:41
Operator : CG/JU
Sample : N1845-10 2X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SAMPLE-10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------