

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
 Data File : BG052637.D
 Acq On : 10 Mar 2022 16:58
 Operator : CG/JU
 Sample : N1845-07 2X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SAMPLE-7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG052637.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.217	306	311	319	rVB2	17566	30397	3.67%	0.507%
2	5.704	388	394	407	rBV	205047	357825	43.18%	5.968%
3	7.325	662	670	683	rBV	263078	479036	57.81%	7.989%
4	8.177	807	815	822	rBV	167432	279348	33.71%	4.659%
5	9.346	1007	1014	1023	rBV	174969	318075	38.39%	5.305%
6	10.768	1250	1256	1262	rBV2	11547	20154	2.43%	0.336%
7	11.015	1285	1298	1305	rBV	234093	404777	48.85%	6.751%
8	13.447	1705	1712	1719	rBV	499843	753839	90.97%	12.573%
9	13.640	1740	1745	1751	rVB5	8235	14149	1.71%	0.236%
10	14.698	1922	1925	1930	rVB4	8189	11740	1.42%	0.196%
11	14.827	1941	1947	1954	rVB	332128	535788	64.66%	8.936%
12	14.892	1954	1958	1965	rVB3	7012	10208	1.23%	0.170%
13	15.221	2008	2014	2018	rBV6	5459	10853	1.31%	0.181%
14	15.444	2046	2052	2056	rBV6	5939	11074	1.34%	0.185%
15	15.614	2075	2081	2084	rBV6	5301	10821	1.31%	0.180%
16	15.650	2084	2087	2093	rVB3	10566	14505	1.75%	0.242%
17	15.873	2119	2125	2132	rBV4	8821	16197	1.95%	0.270%
18	16.061	2151	2157	2161	rVB9	4770	10407	1.26%	0.174%
19	16.319	2195	2201	2208	rBV	156605	247489	29.87%	4.128%
20	16.513	2229	2234	2236	rBV3	9684	13203	1.59%	0.220%
21	16.537	2236	2238	2244	rVB5	12389	18520	2.24%	0.309%
22	17.224	2352	2355	2360	rVB7	7284	11515	1.39%	0.192%
23	17.306	2366	2369	2374	rVB6	13401	17345	2.09%	0.289%
24	17.365	2374	2379	2385	rBV6	13296	23476	2.83%	0.392%
25	17.465	2393	2396	2401	rVB7	8858	12243	1.48%	0.204%
26	17.582	2409	2416	2420	rBV	373790	587459	70.89%	9.798%
27	17.623	2420	2423	2431	rVV	59610	87791	10.59%	1.464%
28	17.711	2435	2438	2443	rVB2	10705	14417	1.74%	0.240%
29	17.976	2481	2483	2487	rVB5	10801	9137	1.10%	0.152%
30	18.052	2493	2496	2502	rVB5	11442	16003	1.93%	0.267%
31	18.222	2522	2525	2528	rVB2	13812	16284	1.97%	0.272%
32	19.362	2716	2719	2724	rBV4	25571	35801	4.32%	0.597%
33	19.626	2760	2764	2770	rBV	101812	141392	17.06%	2.358%
34	19.991	2822	2826	2833	rVB	88110	135741	16.38%	2.264%
35	20.173	2852	2857	2862	rBV	626782	828633	100.00%	13.820%
36	21.888	3144	3149	3155	rVB2	278151	490232	59.16%	8.176%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
Data File : BG052637.D
Acq On : 10 Mar 2022 16:58
Operator : CG/JU
Sample : N1845-07 2X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SAMPLE-7

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 5995874

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
Data File : BG052637.D
Acq On : 10 Mar 2022 16:58
Operator : CG/JU
Sample : N1845-07 2X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SAMPLE-7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

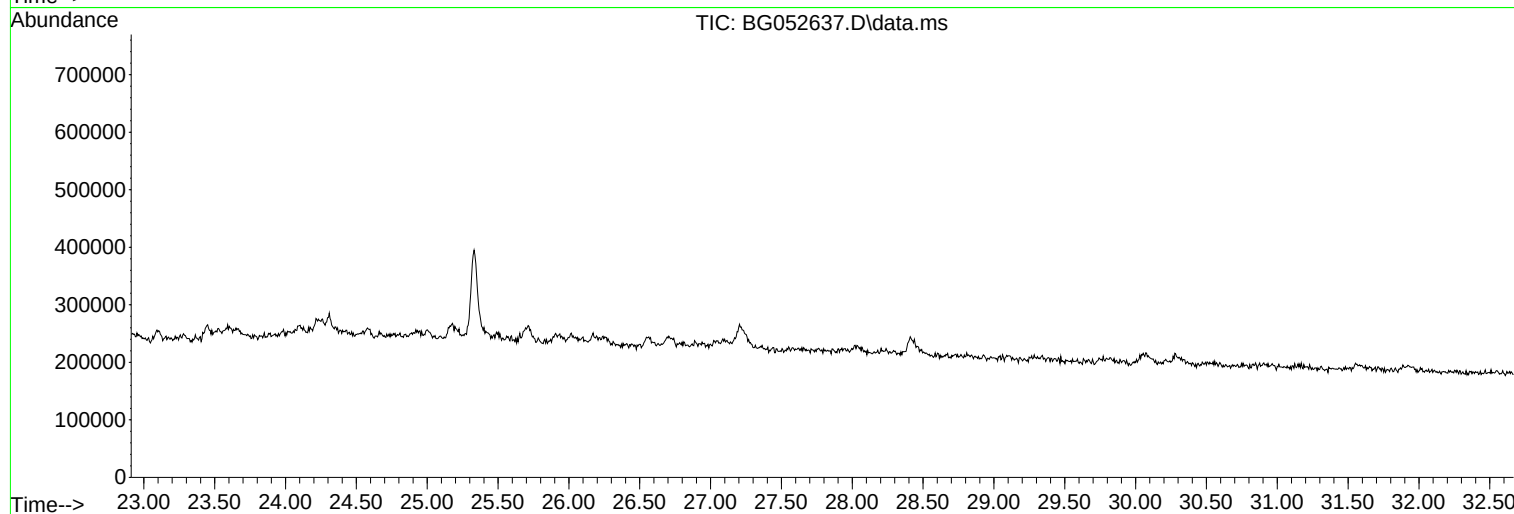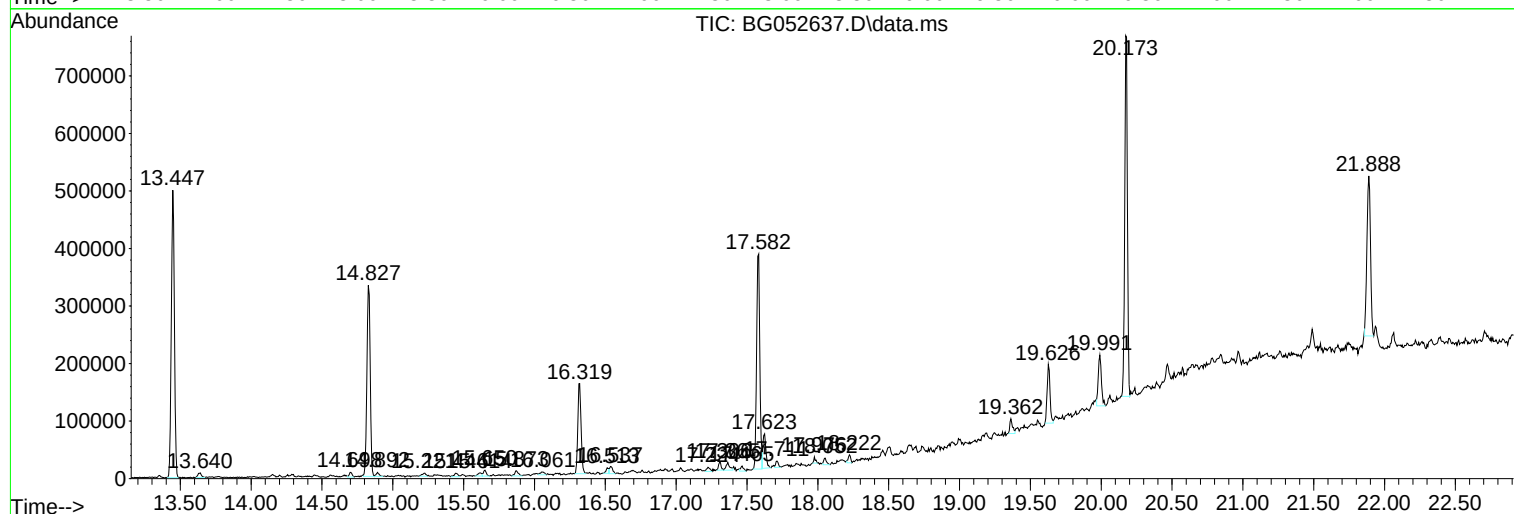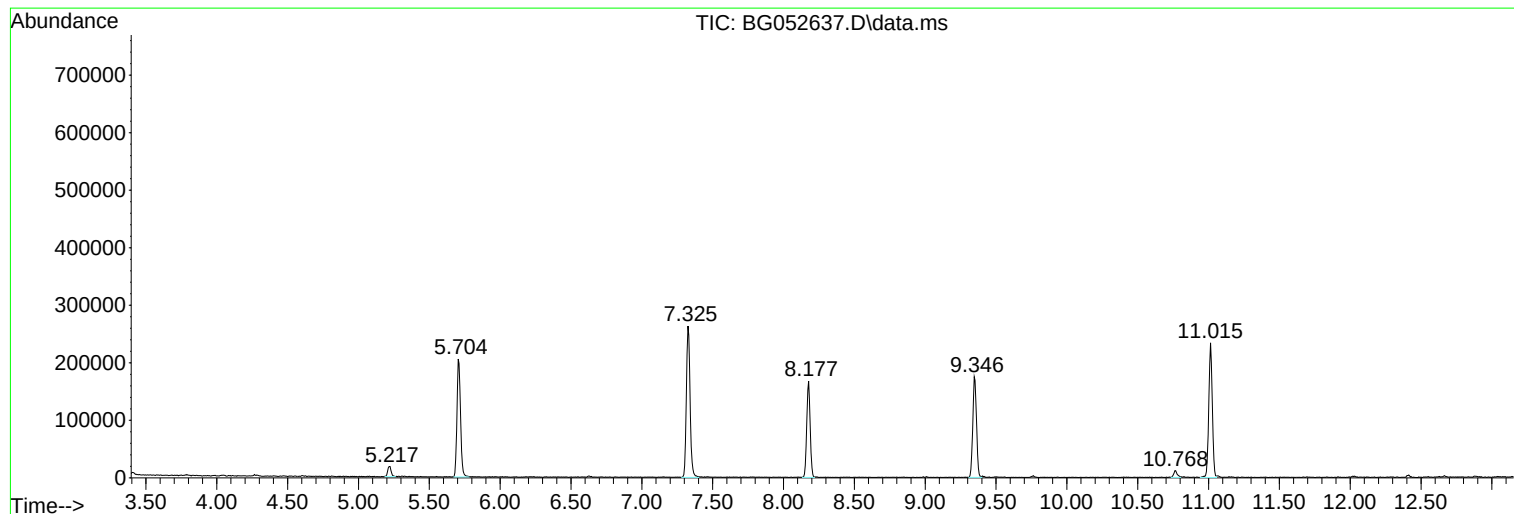

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
Data File : BG052637.D
Acq On : 10 Mar 2022 16:58
Operator : CG/JU
Sample : N1845-07 2X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SAMPLE-7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.217	2.18 ng	30397	1,4-Dichlorobenzene-d4	8.177

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50
2			2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	33
3			3-Octanol	130	C8H18O	000589-98-0	33
4			5-Hexen-2-one	98	C6H10O	000109-49-9	9
5			N-(n-Propyl)acetamide	101	C5H11NO	005331-48-6	9

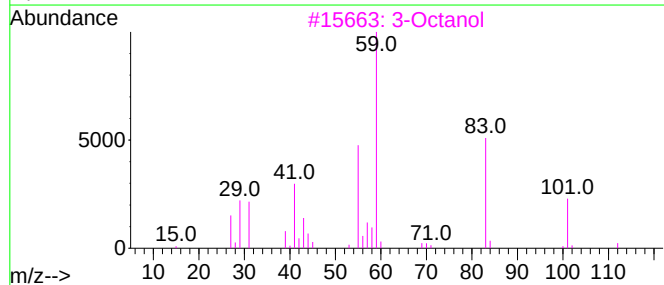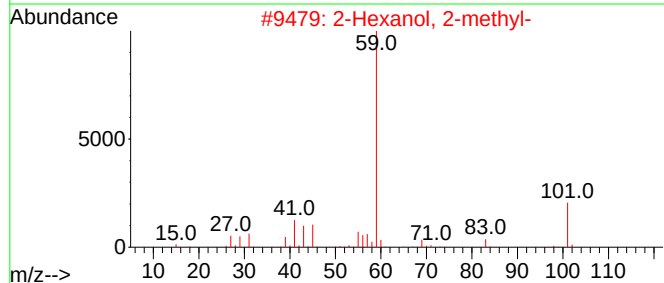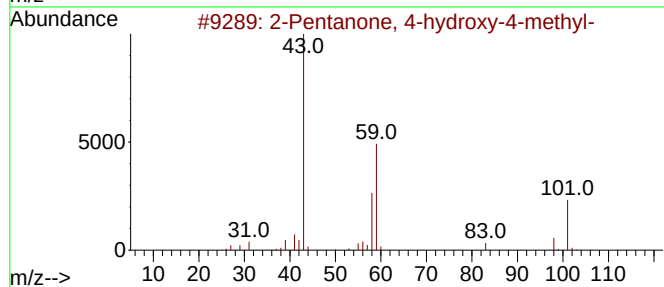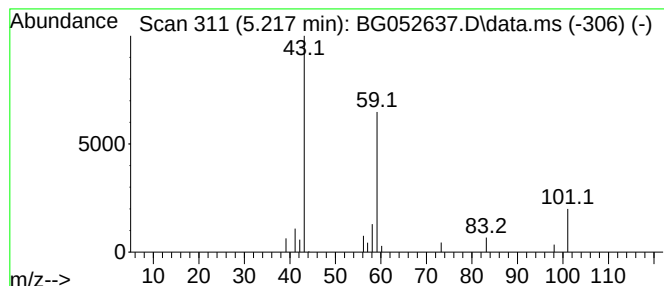

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
Data File : BG052637.D
Acq On : 10 Mar 2022 16:58
Operator : CG/JU
Sample : N1845-07 2X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SAMPLE-7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.217	2.2	ng	30397	1	8.177	279348	20.0