

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
 Data File : BG052638.D
 Acq On : 10 Mar 2022 17:37
 Operator : CG/JU
 Sample : N1845-12RE 2X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SAMPLE-12RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG052638.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.604	201	207	217	rVB	30915	53492	1.79%	0.223%
2	5.214	306	311	322	rVB	98536	161181	5.40%	0.671%
3	5.708	389	395	405	rVB	79656	136176	4.56%	0.567%
4	7.329	664	671	688	rBV	249004	456950	15.30%	1.902%
5	8.175	806	815	822	rBV	153181	259175	8.68%	1.079%
6	9.350	1007	1015	1022	rBV	185257	338158	11.33%	1.408%
7	11.013	1292	1298	1304	rBV	208117	380169	12.73%	1.583%
8	11.065	1304	1307	1315	rVB	48095	77767	2.60%	0.324%
9	12.663	1567	1579	1586	rBV	66205	110791	3.71%	0.461%
10	12.881	1609	1616	1625	rVB	64122	114645	3.84%	0.477%
11	13.450	1704	1713	1723	rVB	527487	819481	27.45%	3.411%
12	13.662	1739	1749	1754	rBV2	48147	92333	3.09%	0.384%
13	13.997	1798	1806	1816	rBV3	53645	152393	5.10%	0.634%
14	14.149	1823	1832	1837	rBV2	96320	170532	5.71%	0.710%
15	14.202	1837	1841	1847	rVB	62840	97292	3.26%	0.405%
16	14.384	1868	1872	1875	rBV	40413	59068	1.98%	0.246%
17	14.555	1896	1901	1907	rVB	21490	36122	1.21%	0.150%
18	14.796	1936	1942	1943	rBV	39108	56286	1.89%	0.234%
19	14.831	1943	1948	1953	rVV	322678	509655	17.07%	2.122%
20	14.895	1953	1959	1965	rVB	225311	360689	12.08%	1.501%
21	15.031	1976	1982	1991	rBV5	19404	50462	1.69%	0.210%
22	15.136	1991	2000	2004	rBV3	13428	32957	1.10%	0.137%
23	15.224	2009	2015	2022	rVB	233097	362700	12.15%	1.510%
24	15.295	2022	2027	2032	rBV	35629	53829	1.80%	0.224%
25	15.436	2045	2051	2056	rBV	33472	61433	2.06%	0.256%
26	15.495	2056	2061	2065	rVB	33349	48692	1.63%	0.203%
27	15.612	2073	2081	2084	rBV4	31988	66549	2.23%	0.277%
28	15.647	2084	2087	2092	rVB3	35117	46177	1.55%	0.192%
29	15.877	2118	2126	2134	rBV2	291147	467641	15.66%	1.947%
30	15.971	2136	2142	2144	rBV5	22401	37994	1.27%	0.158%
31	16.000	2144	2147	2150	rVV2	30568	39418	1.32%	0.164%
32	16.041	2150	2154	2158	rVB	42232	61266	2.05%	0.255%
33	16.164	2171	2175	2183	rVB	95436	154237	5.17%	0.642%
34	16.317	2195	2201	2209	rVV	116820	241684	8.09%	1.006%
35	16.405	2209	2216	2221	rVB2	22794	46217	1.55%	0.192%
36	16.540	2236	2239	2246	rVB5	32199	54331	1.82%	0.226%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
 Data File : BG052638.D
 Acq On : 10 Mar 2022 17:37
 Operator : CG/JU
 Sample : N1845-12RE 2X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SAMPLE-12RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	16.881	2289	2297	2301	rBV2	58880	112537	3.77%	0.468%
38	16.928	2301	2305	2310	rVB3	20832	33175	1.11%	0.138%
39	17.028	2319	2322	2326	rVB3	29864	44118	1.48%	0.184%
40	17.104	2327	2335	2339	rBV5	46206	104871	3.51%	0.437%
41	17.151	2339	2343	2346	rVB2	31313	41640	1.39%	0.173%
42	17.233	2352	2357	2363	rVB	101703	159695	5.35%	0.665%
43	17.304	2364	2369	2376	rVV2	61473	114324	3.83%	0.476%
44	17.398	2380	2385	2392	rVB	134275	220075	7.37%	0.916%
45	17.580	2410	2416	2419	rBV	357319	555409	18.60%	2.312%
46	17.627	2419	2424	2430	rVV	1968848	2985877	100.00%	12.430%
47	17.715	2430	2439	2444	rVV	572046	880821	29.50%	3.667%
48	17.856	2459	2463	2467	rBV2	23485	40713	1.36%	0.169%
49	17.980	2477	2484	2488	rBV2	102442	189527	6.35%	0.789%
50	18.097	2500	2504	2507	rBV	41445	58443	1.96%	0.243%
51	18.162	2511	2515	2523	rVV5	37621	67267	2.25%	0.280%
52	18.455	2560	2565	2569	rBV	176211	254793	8.53%	1.061%
53	18.508	2569	2574	2579	rVB	252286	389352	13.04%	1.621%
54	18.585	2582	2587	2592	rBV	129063	181097	6.07%	0.754%
55	18.655	2593	2599	2602	rBV3	251259	450826	15.10%	1.877%
56	18.684	2602	2604	2609	rVB	114956	145557	4.87%	0.606%
57	18.749	2611	2615	2620	rVB5	24485	39642	1.33%	0.165%
58	18.949	2644	2649	2653	rBV	153708	211731	7.09%	0.881%
59	18.990	2653	2656	2662	rVB	79602	119646	4.01%	0.498%
60	19.196	2687	2691	2695	rVB3	37775	52550	1.76%	0.219%
61	19.243	2696	2699	2703	rVV	34867	43985	1.47%	0.183%
62	19.284	2703	2706	2709	rVB	34041	39218	1.31%	0.163%
63	19.366	2715	2720	2724	rBV2	76510	127200	4.26%	0.530%
64	19.507	2740	2744	2753	rBV2	64726	128769	4.31%	0.536%
65	19.636	2759	2766	2771	rBV	1789762	2508276	84.00%	10.442%
66	19.724	2778	2781	2785	rVB2	46089	60178	2.02%	0.251%
67	19.959	2816	2821	2823	rBV2	288733	449836	15.07%	1.873%
68	19.994	2823	2827	2834	rVV	1331605	1950609	65.33%	8.120%
69	20.059	2834	2838	2843	rVB2	74470	116803	3.91%	0.486%
70	20.177	2852	2858	2862	rBV2	761395	1010168	33.83%	4.205%
71	20.306	2876	2880	2881	rBV	74518	96715	3.24%	0.403%
72	20.576	2924	2926	2930	rVB	69735	74413	2.49%	0.310%
73	21.257	3039	3042	3049	rVB	98584	147310	4.93%	0.613%
74	21.492	3079	3082	3087	rVB	103494	147193	4.93%	0.613%
75	21.551	3089	3092	3097	rVB2	97916	144313	4.83%	0.601%
76	21.880	3142	3148	3155	rBV3	646002	1548844	51.87%	6.448%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
Data File : BG052638.D
Acq On : 10 Mar 2022 17:37
Operator : CG/JU
Sample : N1845-12RE 2X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SAMPLE-12RE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	21.945	3155	3159	3171	rVB	476574	870155	29.14%	3.622%
78	22.103	3183	3186	3192	rVB	92096	153243	5.13%	0.638%
79	24.242	3543	3550	3557	rBV	202787	683311	22.88%	2.845%




Sum of corrected areas: 24022167

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
Data File : BG052638.D
Acq On : 10 Mar 2022 17:37
Operator : CG/JU
Sample : N1845-12RE 2X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SAMPLE-12RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

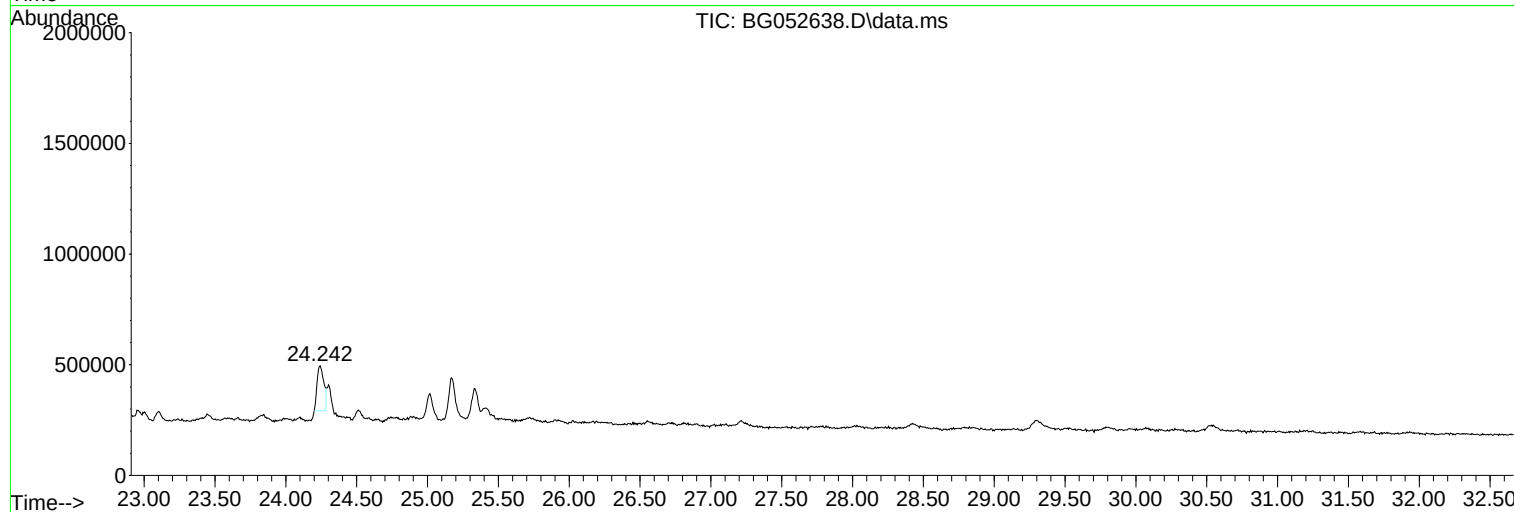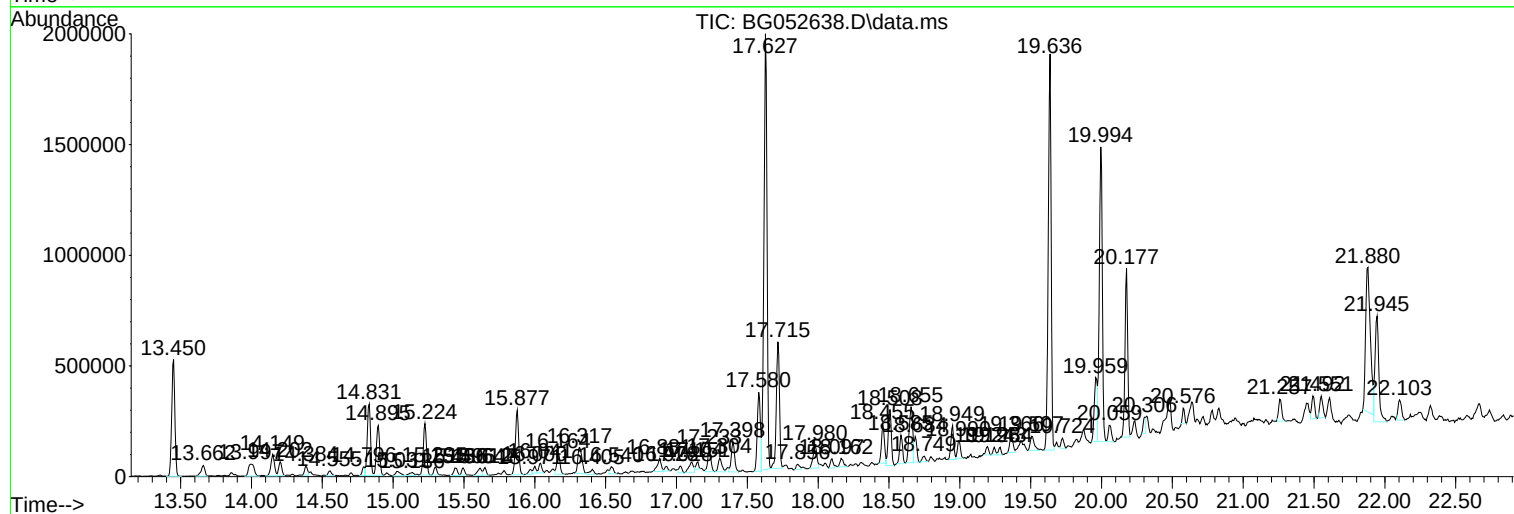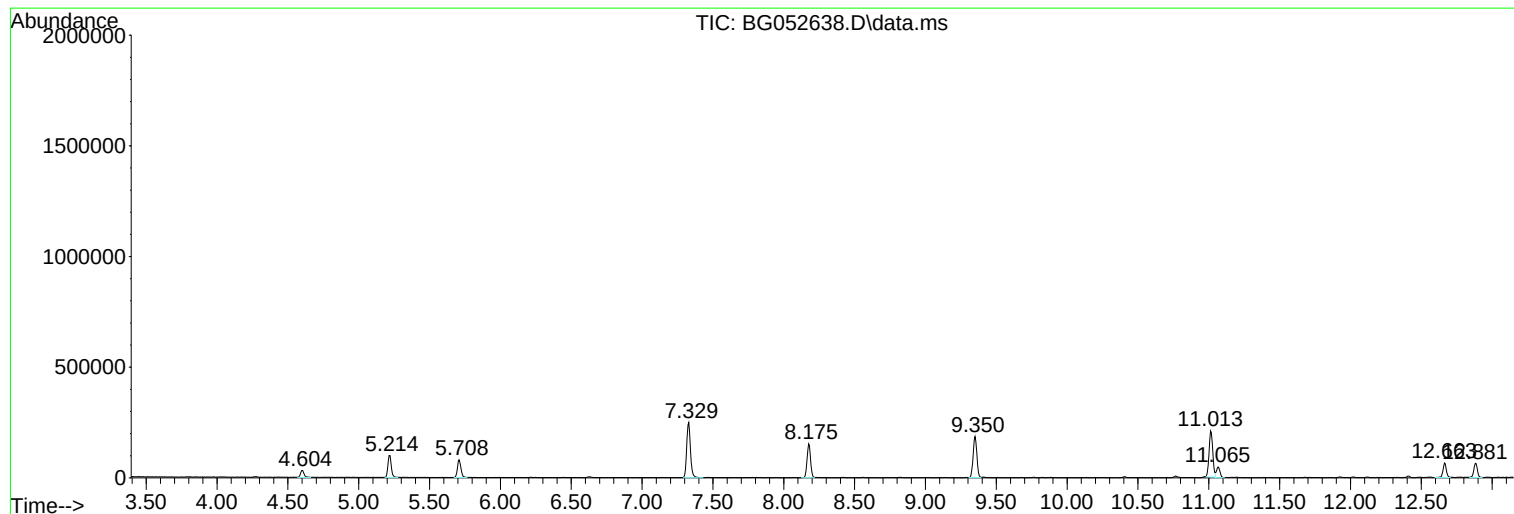

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
Data File : BG052638.D
Acq On : 10 Mar 2022 17:37
Operator : CG/JU
Sample : N1845-12RE 2X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SAMPLE-12RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
Data File : BG052638.D
Acq On : 10 Mar 2022 17:37
Operator : CG/JU
Sample : N1845-12RE 2X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SAMPLE-12RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------