

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
 Data File : BG052639.D
 Acq On : 10 Mar 2022 18:15
 Operator : CG/JU
 Sample : N1845-05 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SAMPLE-5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG052639.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.217	305	311	320	rVB2	12135	18974	3.32%	0.512%
2	5.705	388	394	405	rBV	87925	148280	25.91%	4.002%
3	7.326	663	670	681	rBV	109619	201210	35.16%	5.431%
4	8.178	807	815	823	rBV	148405	253614	44.31%	6.845%
5	9.347	1008	1014	1024	rBV	75688	134922	23.57%	3.642%
6	11.015	1291	1298	1305	rVB	203214	365629	63.88%	9.869%
7	13.447	1704	1712	1719	rBV	223538	332578	58.11%	8.976%
8	13.635	1739	1744	1749	rBV4	4179	5926	1.04%	0.160%
9	14.705	1922	1926	1929	rBV3	4989	6206	1.08%	0.168%
10	14.828	1940	1947	1955	rBV	319205	508515	88.85%	13.725%
11	15.615	2072	2081	2083	rBV5	2991	6686	1.17%	0.180%
12	15.650	2083	2087	2092	rVB2	4863	7696	1.34%	0.208%
13	15.868	2119	2124	2129	rBV7	4173	7063	1.23%	0.191%
14	16.320	2196	2201	2208	rBV2	51661	84929	14.84%	2.292%
15	16.543	2236	2239	2246	rVB7	9078	12624	2.21%	0.341%
16	16.643	2250	2256	2260	rBV2	5492	10103	1.77%	0.273%
17	16.972	2306	2312	2315	rBV7	4127	7708	1.35%	0.208%
18	17.025	2318	2321	2327	rBV2	6814	11736	2.05%	0.317%
19	17.230	2352	2356	2360	rBV5	5615	11003	1.92%	0.297%
20	17.307	2366	2369	2374	rBV6	7191	10408	1.82%	0.281%
21	17.360	2374	2378	2382	rBV5	8023	12671	2.21%	0.342%
22	17.583	2409	2416	2421	rBV	350777	572335	100.00%	15.448%
23	17.618	2421	2422	2430	rVB	26283	31454	5.50%	0.849%
24	17.712	2435	2438	2442	rVB2	4916	6074	1.06%	0.164%
25	17.859	2458	2463	2464	rBV5	4940	6973	1.22%	0.188%
26	18.053	2492	2496	2499	rVB6	7941	9407	1.64%	0.254%
27	18.165	2512	2515	2520	rVB6	4909	7219	1.26%	0.195%
28	18.681	2601	2603	2607	rBV5	8248	9557	1.67%	0.258%
29	18.734	2610	2612	2614	rBV3	7644	8696	1.52%	0.235%
30	19.627	2761	2764	2769	rVB	41459	54718	9.56%	1.477%
31	20.174	2853	2857	2863	rVB	297696	374142	65.37%	10.098%
32	21.889	3144	3149	3155	rVB	291904	465950	81.41%	12.576%




Sum of corrected areas: 3705006

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
Data File : BG052639.D
Acq On : 10 Mar 2022 18:15
Operator : CG/JU
Sample : N1845-05 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SAMPLE-5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

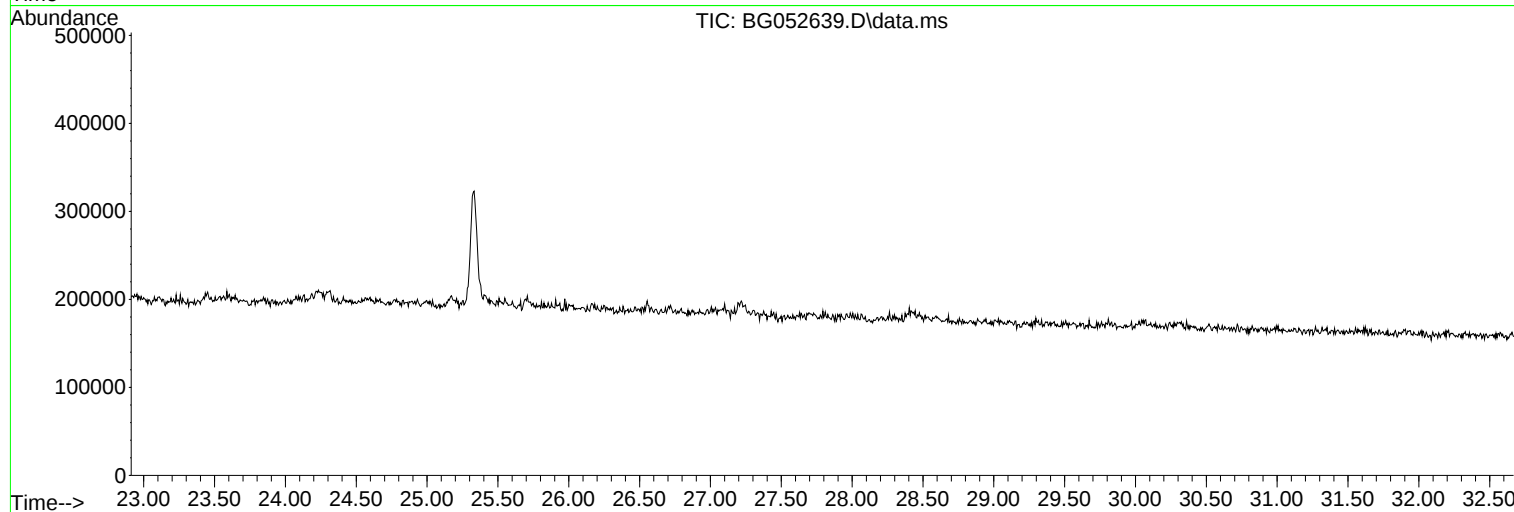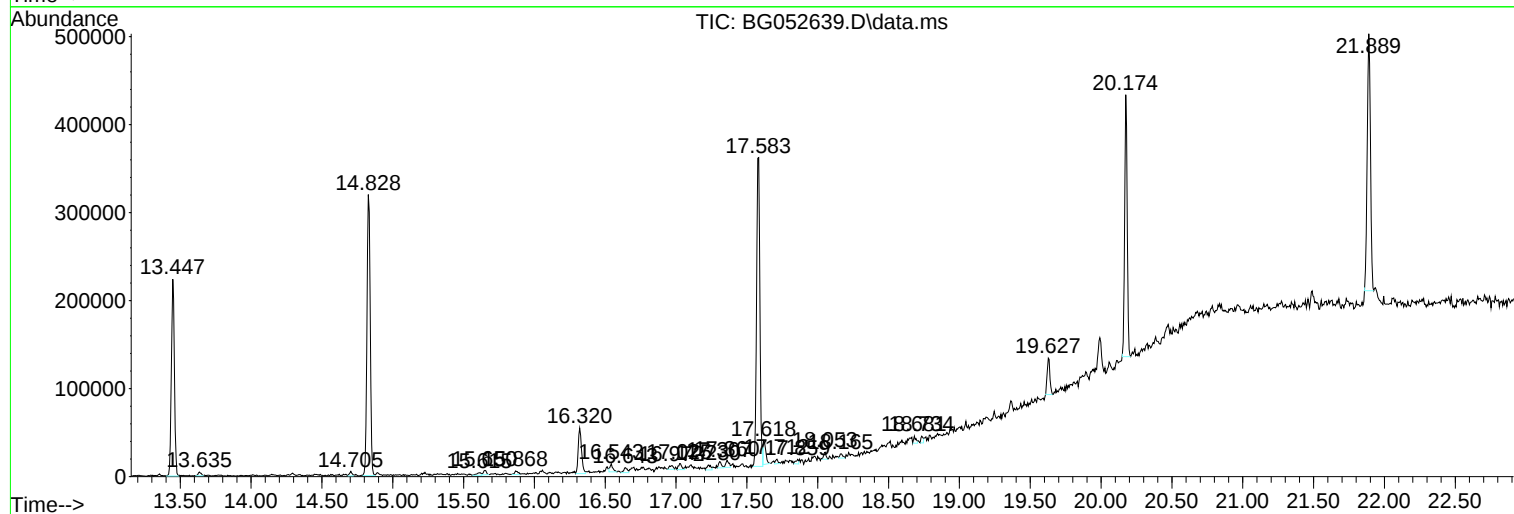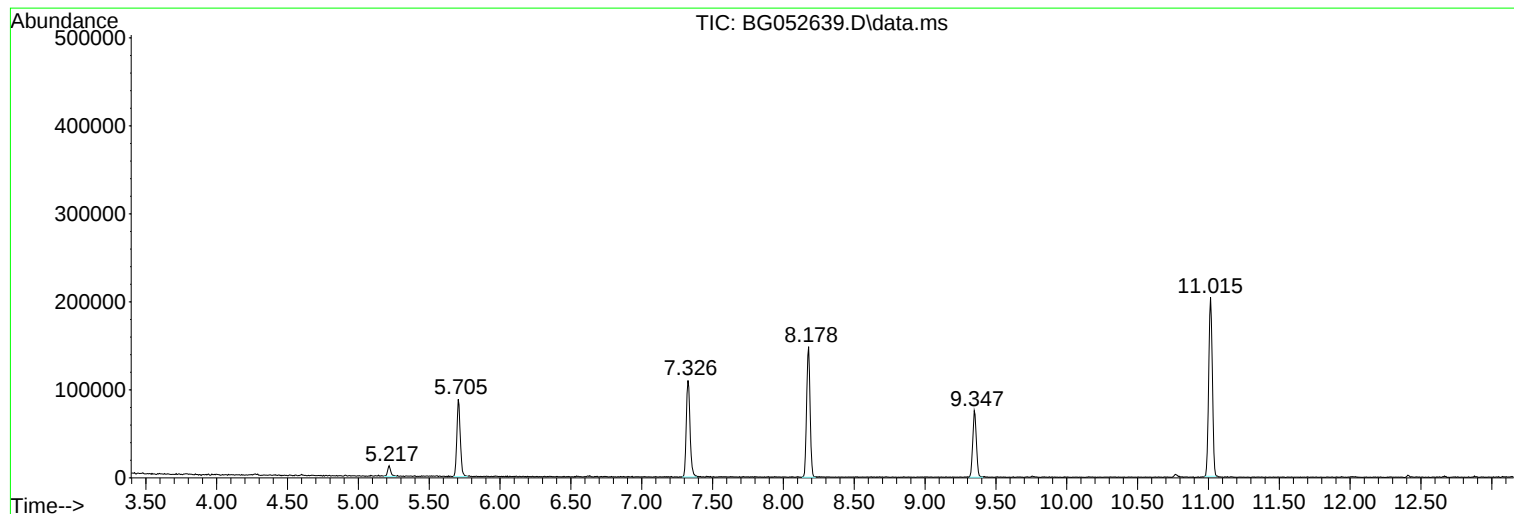

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
Data File : BG052639.D
Acq On : 10 Mar 2022 18:15
Operator : CG/JU
Sample : N1845-05 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SAMPLE-5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
Data File : BG052639.D
Acq On : 10 Mar 2022 18:15
Operator : CG/JU
Sample : N1845-05 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SAMPLE-5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------