

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
 Data File : BG052640.D
 Acq On : 10 Mar 2022 18:54
 Operator : CG/JU
 Sample : N1845-15 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SAMPLE-15

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG052640.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.598	202	206	212	rVB4	4122	7366	1.26%	0.155%
2	5.220	307	312	318	rBV2	14731	24683	4.24%	0.521%
3	5.708	389	395	406	rVB	64683	114424	19.64%	2.415%
4	7.329	663	671	680	rBV	91815	169263	29.05%	3.572%
5	8.175	808	815	824	rBV	154578	261227	44.83%	5.513%
6	9.350	1008	1015	1023	rBV	63385	113077	19.41%	2.386%
7	11.013	1287	1298	1305	rBV	204832	385237	66.12%	8.129%
8	11.065	1305	1307	1314	rVB	12164	16863	2.89%	0.356%
9	12.669	1574	1580	1585	rVB	5993	10263	1.76%	0.217%
10	12.887	1609	1617	1621	rBV3	4417	7566	1.30%	0.160%
11	13.356	1694	1697	1704	rVB4	3463	5836	1.00%	0.123%
12	13.450	1707	1713	1720	rVB	182895	284212	48.78%	5.998%
13	13.638	1738	1745	1755	rBV3	14205	27738	4.76%	0.585%
14	14.155	1827	1833	1838	rVB5	5566	11616	1.99%	0.245%
15	14.208	1838	1842	1845	rBV3	4356	6575	1.13%	0.139%
16	14.291	1847	1856	1860	rBV3	7338	16337	2.80%	0.345%
17	14.702	1922	1926	1931	rVB2	22204	29035	4.98%	0.613%
18	14.784	1933	1940	1942	rVV5	3386	6196	1.06%	0.131%
19	14.831	1942	1948	1954	rVV	327629	524787	90.07%	11.074%
20	14.890	1954	1958	1964	rVB	24859	36663	6.29%	0.774%
21	15.225	2007	2015	2019	rBV	15246	27390	4.70%	0.578%
22	15.319	2024	2031	2036	rBV5	3444	9559	1.64%	0.202%
23	15.653	2084	2088	2093	rVB	15960	19723	3.38%	0.416%
24	15.871	2121	2125	2133	rVB2	25775	42581	7.31%	0.899%
25	16.170	2171	2176	2180	rBV5	4033	6568	1.13%	0.139%
26	16.317	2197	2201	2211	rBV3	31735	55611	9.54%	1.174%
27	16.517	2230	2235	2237	rBV4	9721	14954	2.57%	0.316%
28	16.540	2237	2239	2244	rVB5	9249	12808	2.20%	0.270%
29	17.028	2318	2322	2328	rVB5	6183	8878	1.52%	0.187%
30	17.304	2366	2369	2375	rBV5	11205	18000	3.09%	0.380%
31	17.363	2375	2379	2382	rBV3	8708	14058	2.41%	0.297%
32	17.404	2382	2386	2391	rVB2	11201	19931	3.42%	0.421%
33	17.580	2409	2416	2420	rBV	377574	582675	100.00%	12.296%
34	17.621	2420	2423	2429	rVB	173805	251631	43.19%	5.310%
35	17.715	2434	2439	2443	rVB	45260	68328	11.73%	1.442%
36	17.980	2478	2484	2489	rBV2	21810	37856	6.50%	0.799%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
 Data File : BG052640.D
 Acq On : 10 Mar 2022 18:54
 Operator : CG/JU
 Sample : N1845-15 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SAMPLE-15

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	18.050	2493	2496	2499	rVB5	9922	12120	2.08%	0.256%
38	18.450	2561	2564	2569	rBV	13362	22560	3.87%	0.476%
39	18.508	2570	2574	2579	rVB2	25057	39933	6.85%	0.843%
40	18.655	2593	2599	2602	rBV2	30073	56543	9.70%	1.193%
41	18.743	2610	2614	2616	rBV5	9668	12667	2.17%	0.267%
42	19.630	2760	2765	2770	rBV	181338	260632	44.73%	5.500%
43	19.989	2823	2826	2832	rVB	124134	178103	30.57%	3.758%
44	20.177	2853	2858	2862	rBV	252455	331028	56.81%	6.986%
45	21.892	3143	3150	3156	rBV2	291954	575659	98.80%	12.148%




Sum of corrected areas: 4738760

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
Data File : BG052640.D
Acq On : 10 Mar 2022 18:54
Operator : CG/JU
Sample : N1845-15 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SAMPLE-15

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

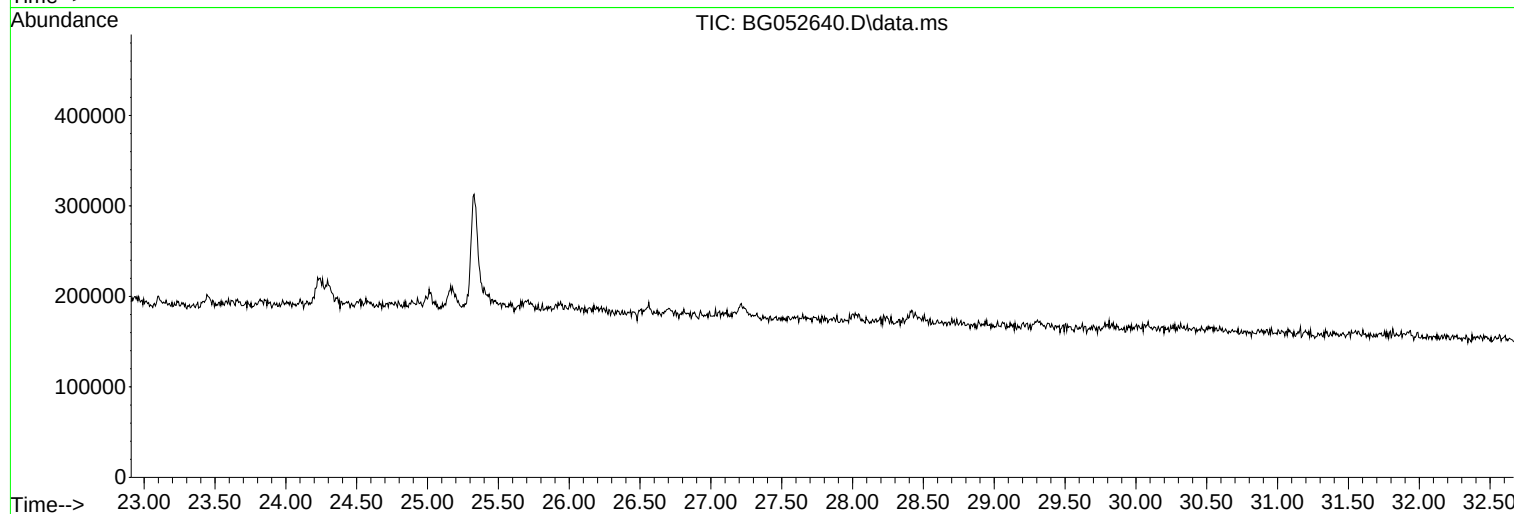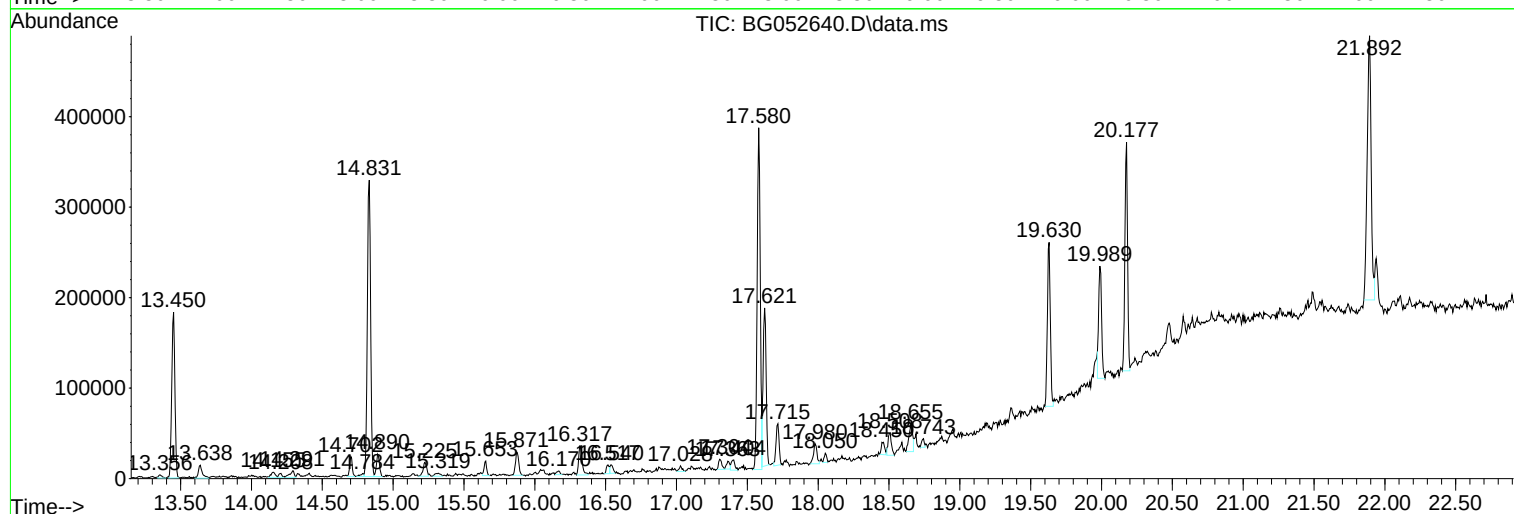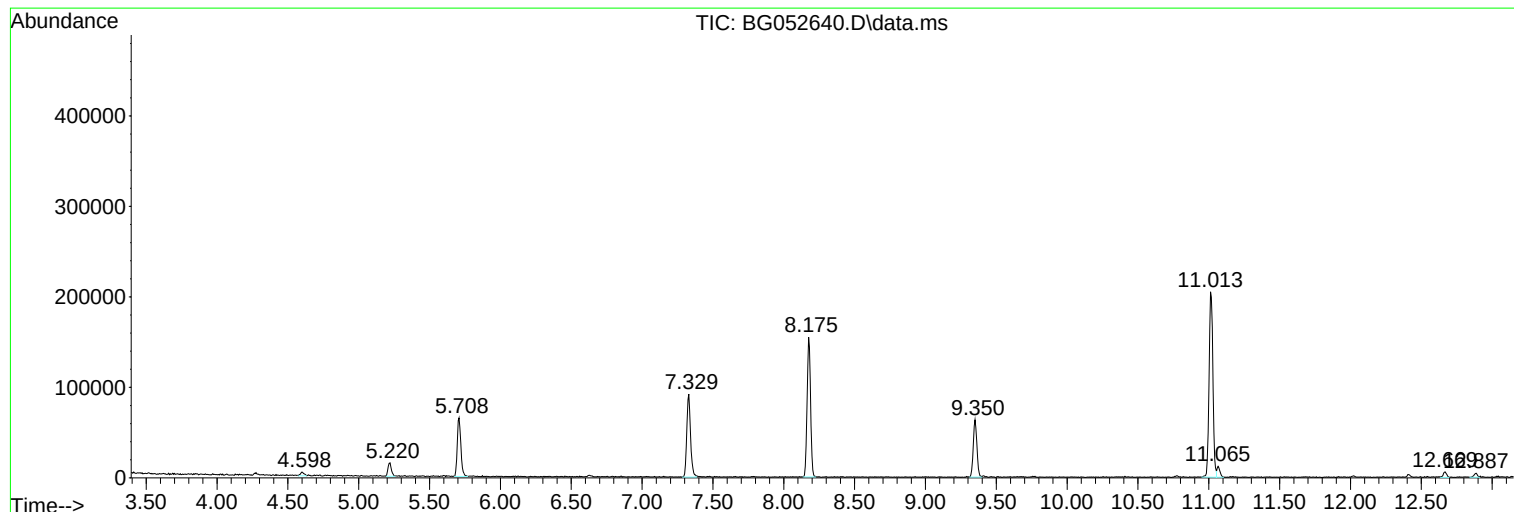

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
Data File : BG052640.D
Acq On : 10 Mar 2022 18:54
Operator : CG/JU
Sample : N1845-15 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SAMPLE-15

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
Data File : BG052640.D
Acq On : 10 Mar 2022 18:54
Operator : CG/JU
Sample : N1845-15 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SAMPLE-15

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------