

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
 Data File : BG052641.D
 Acq On : 10 Mar 2022 19:33
 Operator : CG/JU
 Sample : N1845-02 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SAMPLE-2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG052641.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.222	306	312	316	rBV3	5665	9923	1.76%	0.291%
2	5.704	388	394	406	rBV2	74540	133295	23.62%	3.910%
3	7.325	664	670	681	rBV	87142	165731	29.37%	4.862%
4	8.177	808	815	823	rBV	149867	258461	45.80%	7.582%
5	9.346	1006	1014	1024	rBV	57724	109431	19.39%	3.210%
6	11.014	1291	1298	1309	rBV	208754	371575	65.84%	10.900%
7	13.446	1706	1712	1720	rBV	170742	270751	47.98%	7.943%
8	14.833	1941	1948	1955	rVB	318051	506700	89.79%	14.864%
9	16.319	2196	2201	2207	rBV2	67392	110465	19.57%	3.241%
10	16.542	2229	2239	2245	rBV8	4848	11909	2.11%	0.349%
11	17.312	2365	2370	2374	rBV7	3684	5900	1.05%	0.173%
12	17.370	2374	2380	2384	rVV7	3941	7592	1.35%	0.223%
13	17.582	2409	2416	2421	rBV	376335	564322	100.00%	16.555%
14	17.623	2421	2423	2428	rVB2	18399	23256	4.12%	0.682%
15	17.717	2435	2439	2442	rVB5	3509	5695	1.01%	0.167%
16	18.052	2492	2496	2501	rBV7	5306	7625	1.35%	0.224%
17	18.222	2520	2525	2528	rBV5	5245	8387	1.49%	0.246%
18	18.504	2569	2573	2577	rVV6	9319	11081	1.96%	0.325%
19	18.639	2591	2596	2600	rBV8	8890	18754	3.32%	0.550%
20	19.626	2761	2764	2769	rVB	31118	40303	7.14%	1.182%
21	20.172	2853	2857	2864	rBV	242801	313613	55.57%	9.200%
22	21.888	3144	3149	3156	rBV2	265064	454101	80.47%	13.321%




Sum of corrected areas: 3408870

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
Data File : BG052641.D
Acq On : 10 Mar 2022 19:33
Operator : CG/JU
Sample : N1845-02 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SAMPLE-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

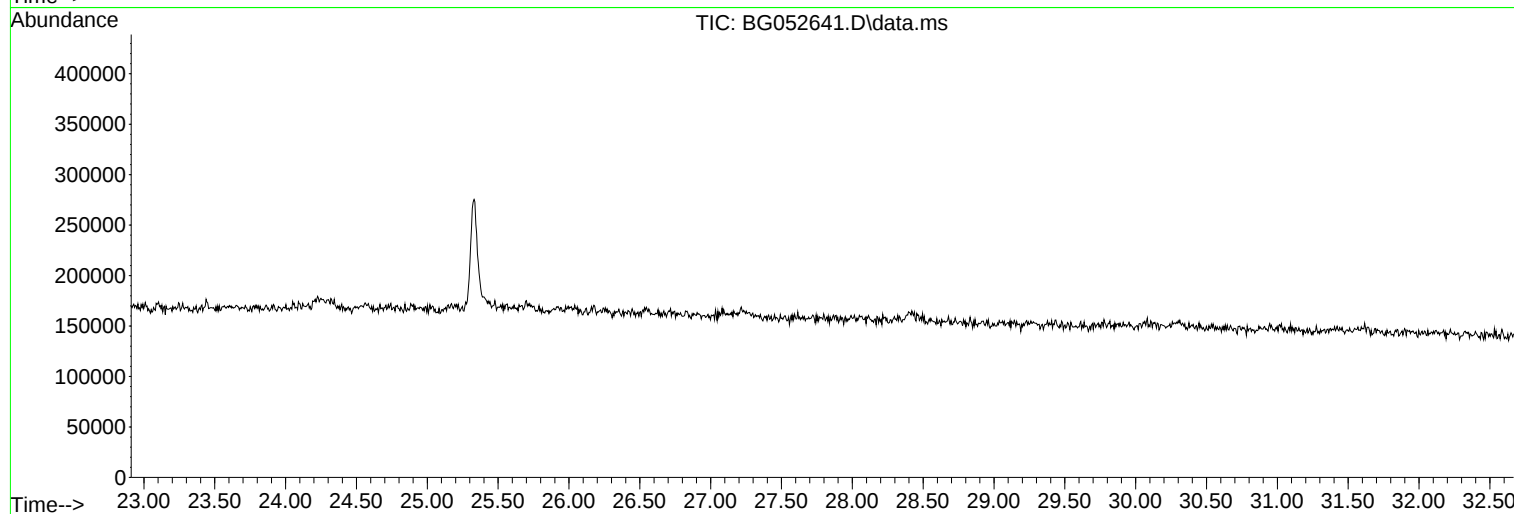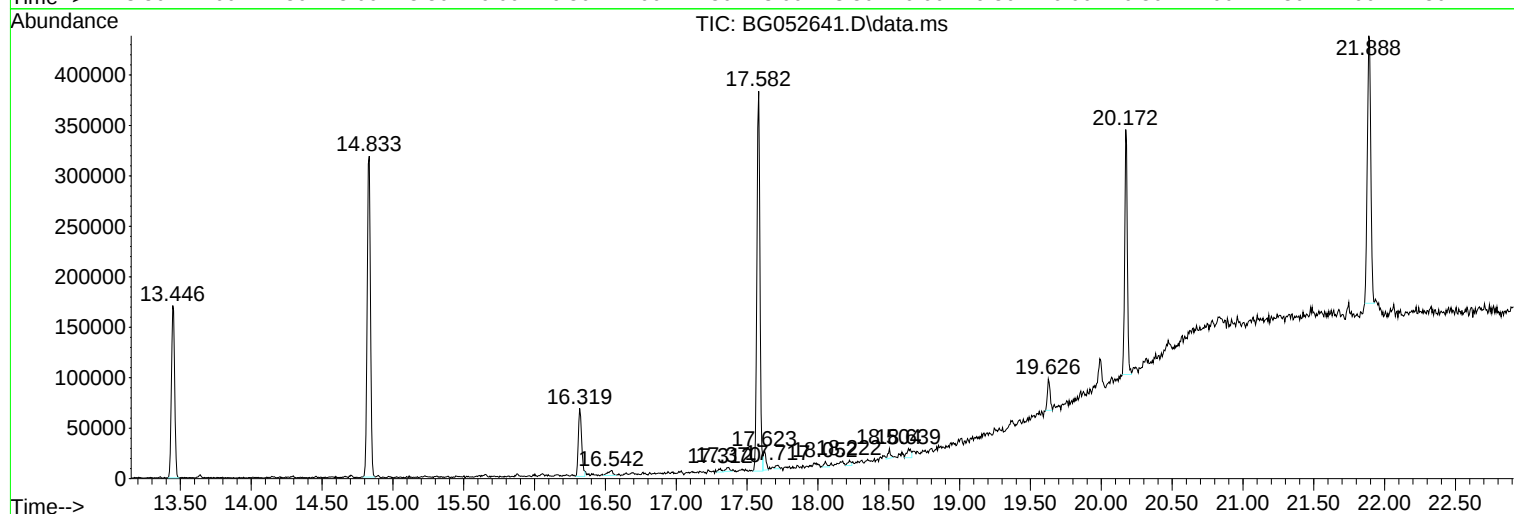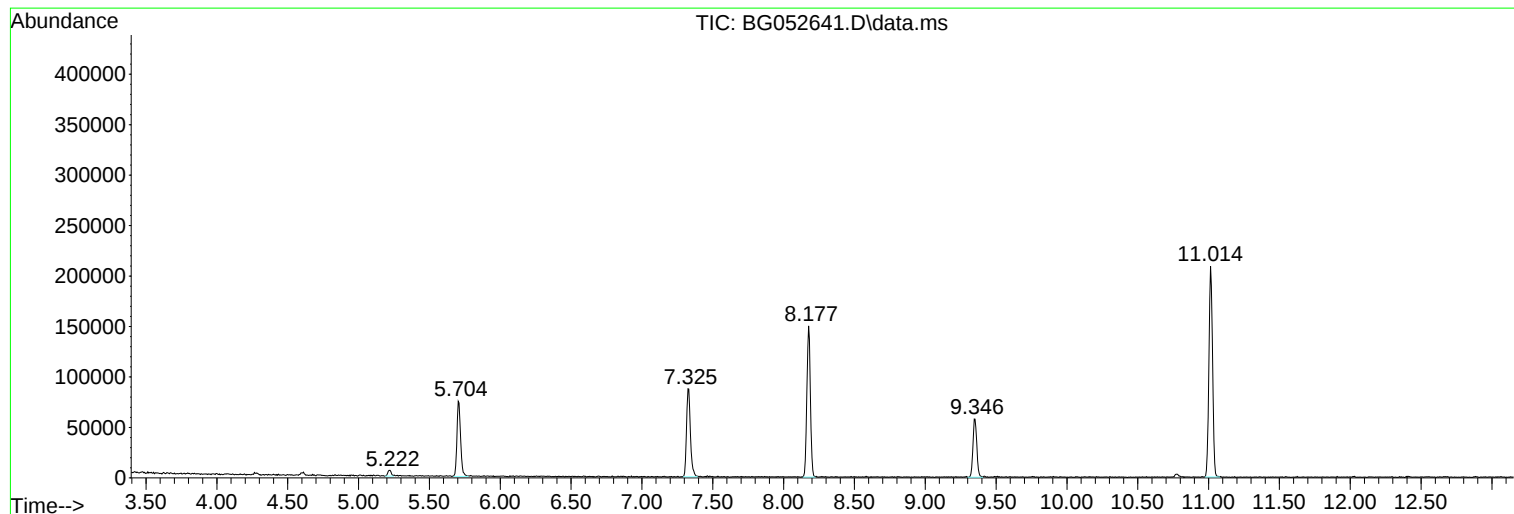

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
Data File : BG052641.D
Acq On : 10 Mar 2022 19:33
Operator : CG/JU
Sample : N1845-02 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SAMPLE-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
Data File : BG052641.D
Acq On : 10 Mar 2022 19:33
Operator : CG/JU
Sample : N1845-02 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SAMPLE-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------