
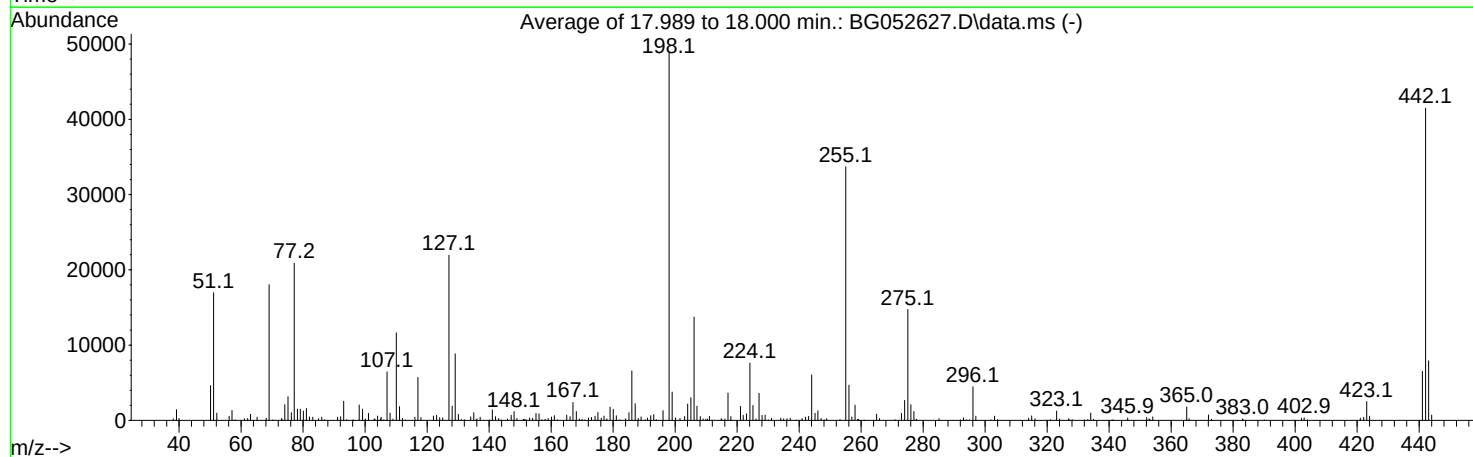


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
 Data File : BG052627.D
 Acq On : 10 Mar 2022 10:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 10 06:37:54 2022

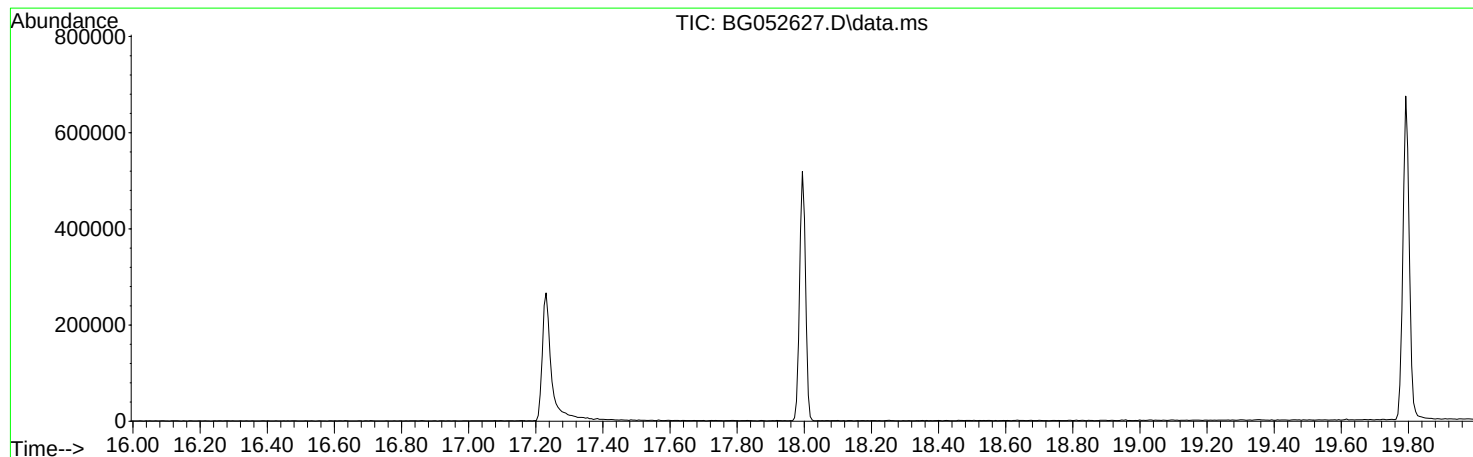

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	16972	PASS
68	69	0.00	2	1.6	284	PASS
69	198	0.00	100	36.9	18026	PASS
70	69	0.00	2	0.3	60	PASS
127	198	10	80	44.9	21933	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48877	PASS
199	198	5	9	7.7	3769	PASS
275	198	10	60	30.1	14736	PASS
365	198	1	100	3.7	1797	PASS
441	198	0.01	100	13.3	6496	PASS
442	442	50	100	100.0	41472	PASS
443	442	15	24	19.1	7918	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/10/2022	BNA_G	<u>BG052627.D</u>
Compound Name	Response	Retention Time
DDT	203889	21.03
DDD	1040	20.63
DDE	0	19.98
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1040	204929	0.51

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
Data File : BG052627.D
Acq On : 10 Mar 2022 10:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 10 13:13:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 10 06:37:54 2022
Response via : Initial Calibration

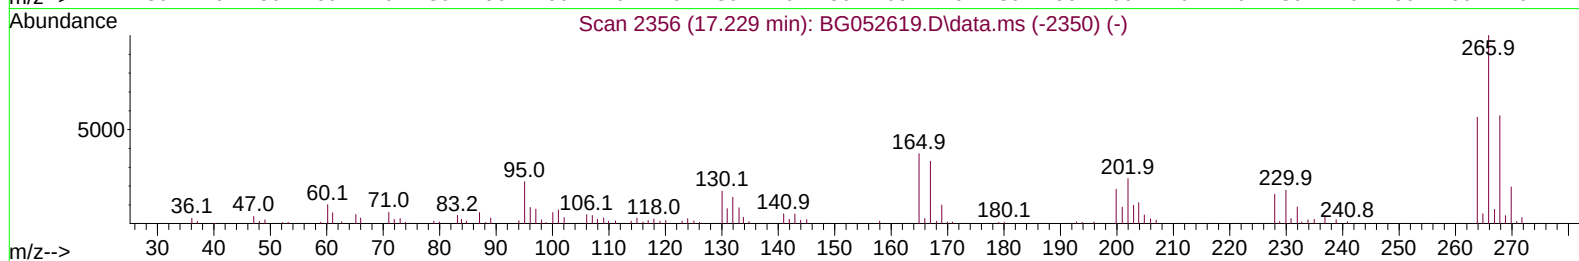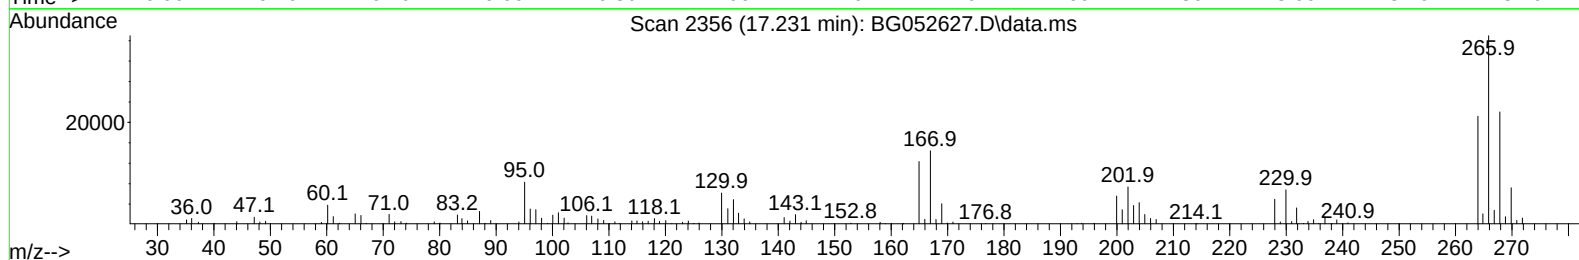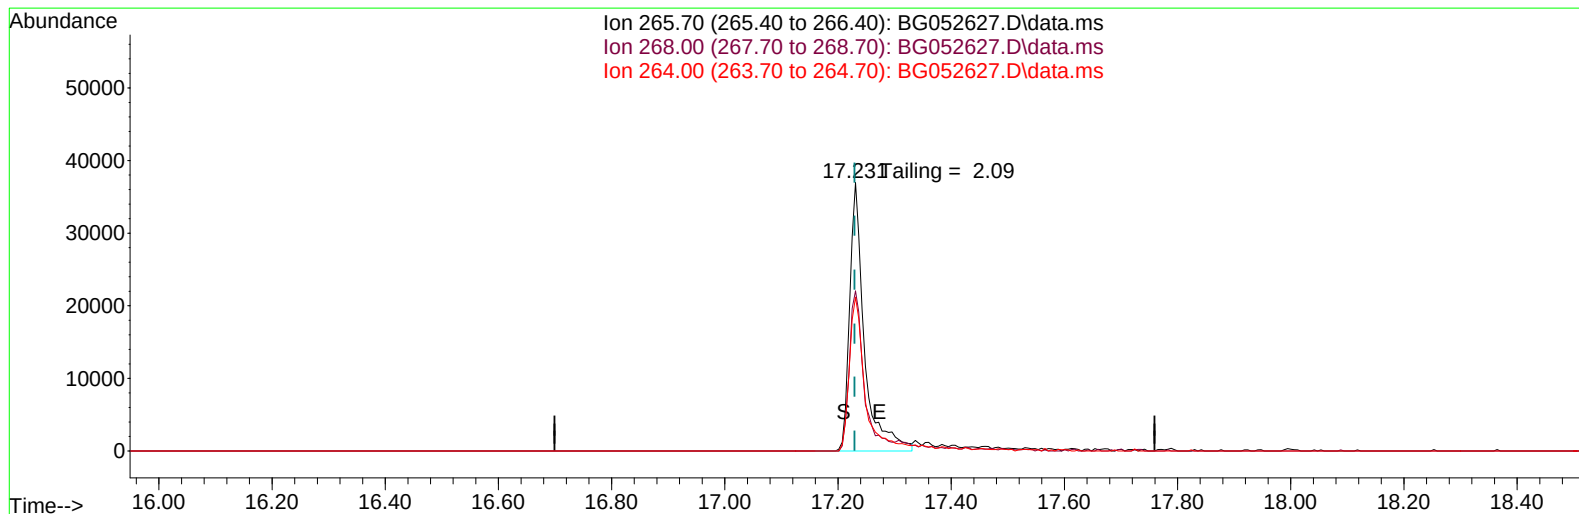

TIC: BG052627.D\data.ms

(70) Pentachlorophenol (C)

17.231min (+ 0.002) 34429.96 ng




response 67147

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	59.68
264.00	56.60	57.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031022\
Data File : BG052627.D
Acq On : 10 Mar 2022 10:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 10 13:13:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 10 06:37:54 2022
Response via : Initial Calibration

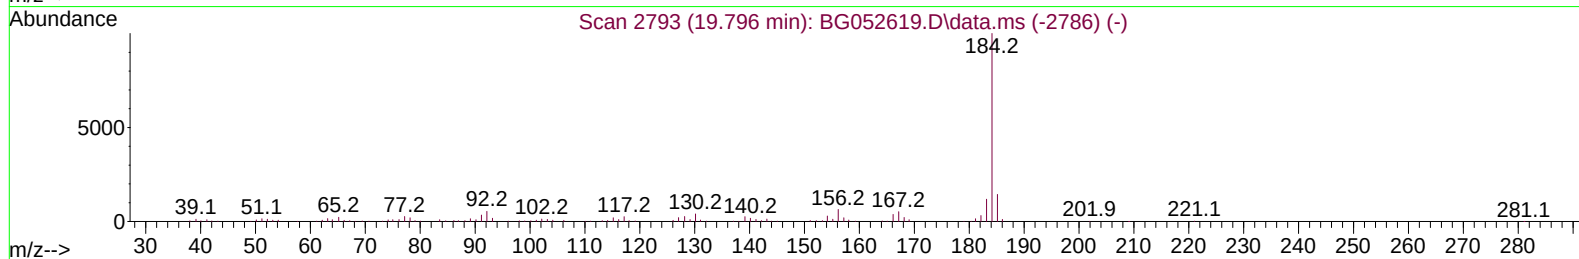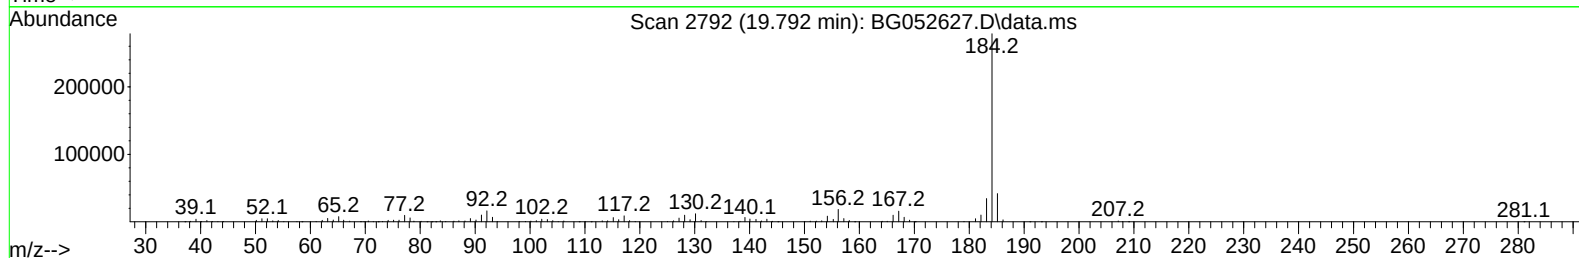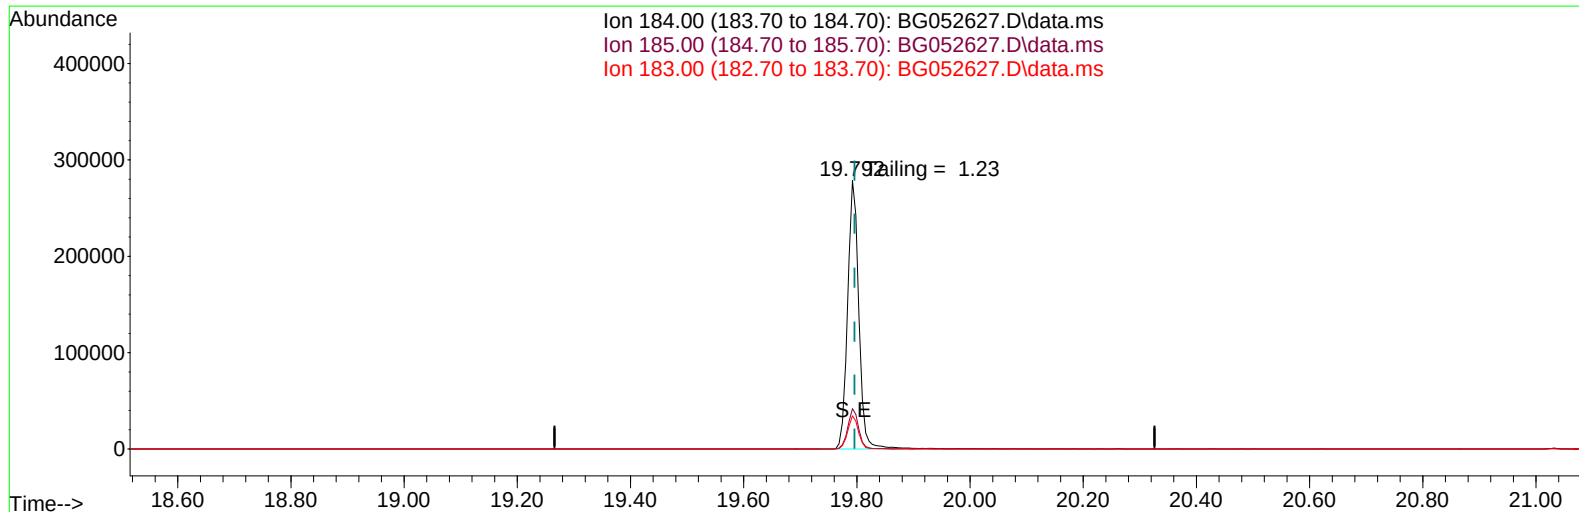

TIC: BG052627.D\data.ms

(77) Benzidine

19.792min (-0.004) 204882.35 ng

response 382517

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	15.04
183.00	11.80	12.43
0.00	0.00	0.00