
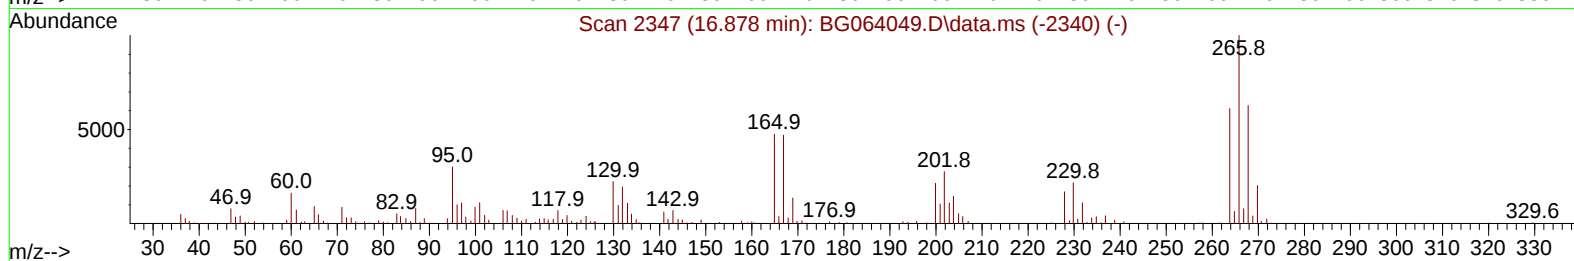
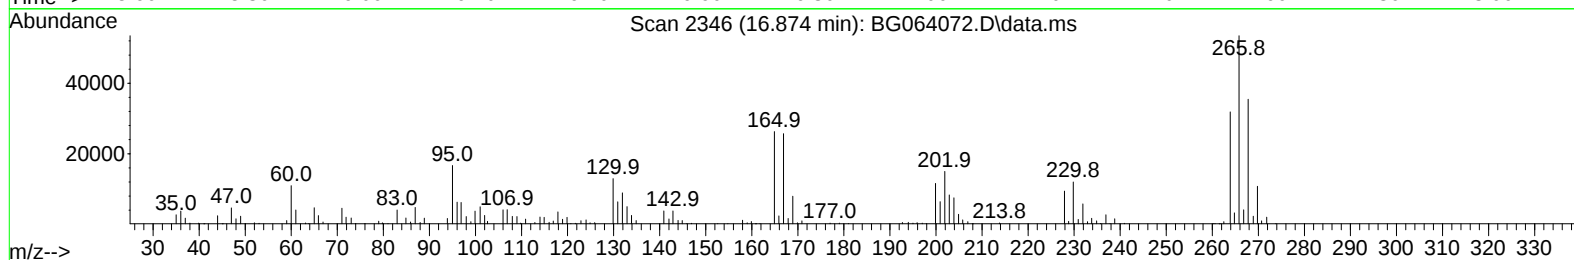


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031025\
Data File : BG064072.D
Acq On : 10 Mar 2025 8:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 10 11:22:27 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 05 15:39:19 2025
Response via : Initial Calibration

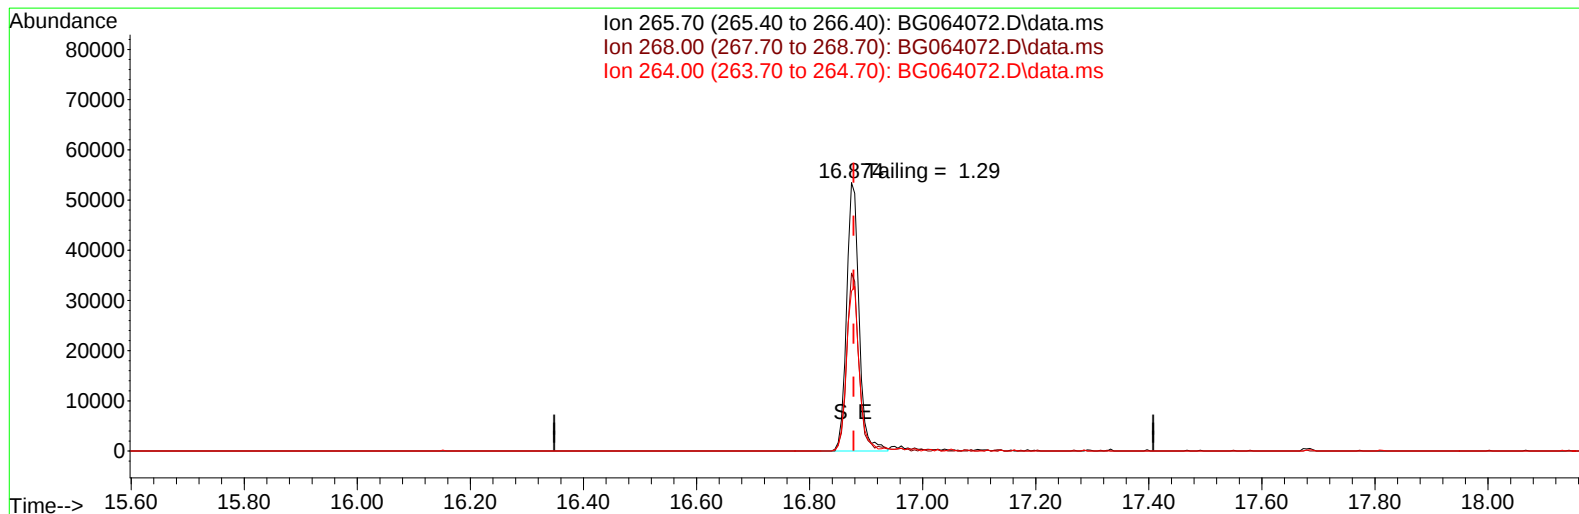

TIC: BG064072.D\data.ms

(70) Pentachlorophenol (C)




16.874min (-0.004) 137114.61 ng

response 81997

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	66.31
264.00	61.10	59.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031025\
Data File : BG064072.D
Acq On : 10 Mar 2025 8:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 10 11:22:27 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 05 15:39:19 2025
Response via : Initial Calibration

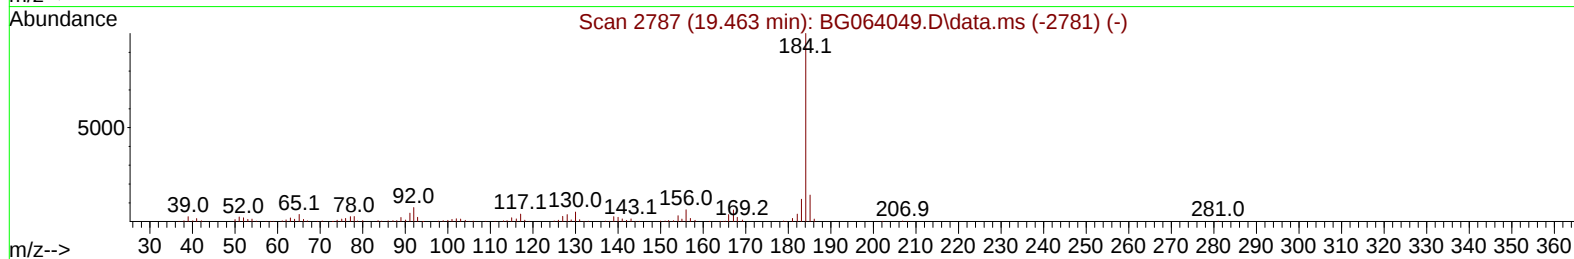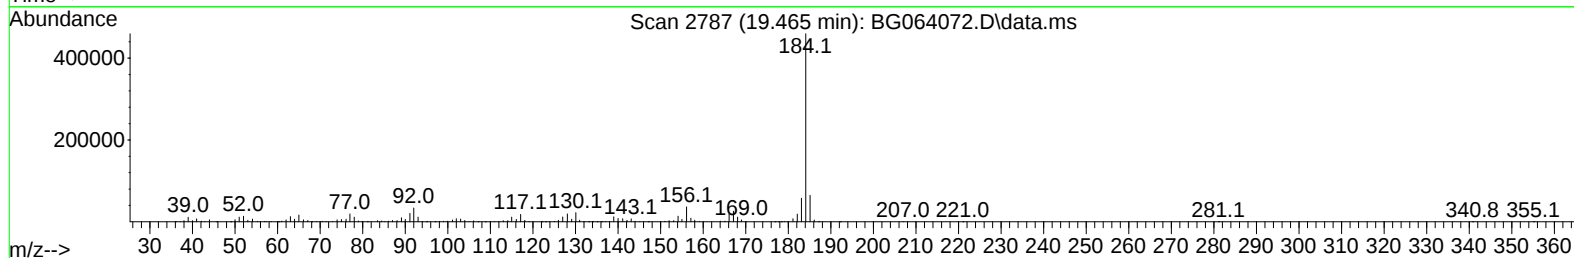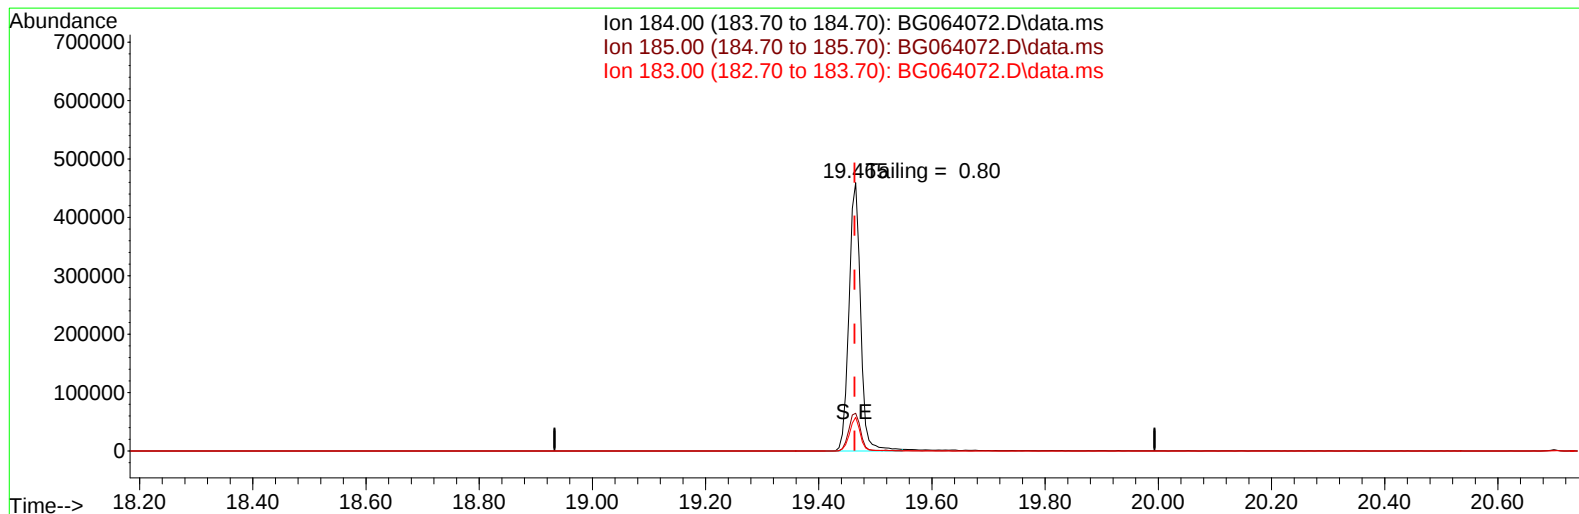

TIC: BG064072.D\data.ms

(77) Benzidine**19.465min (+ 0.002) 21680.85 ng****response 657177**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.11
183.00	11.90	12.58
0.00	0.00	0.00