
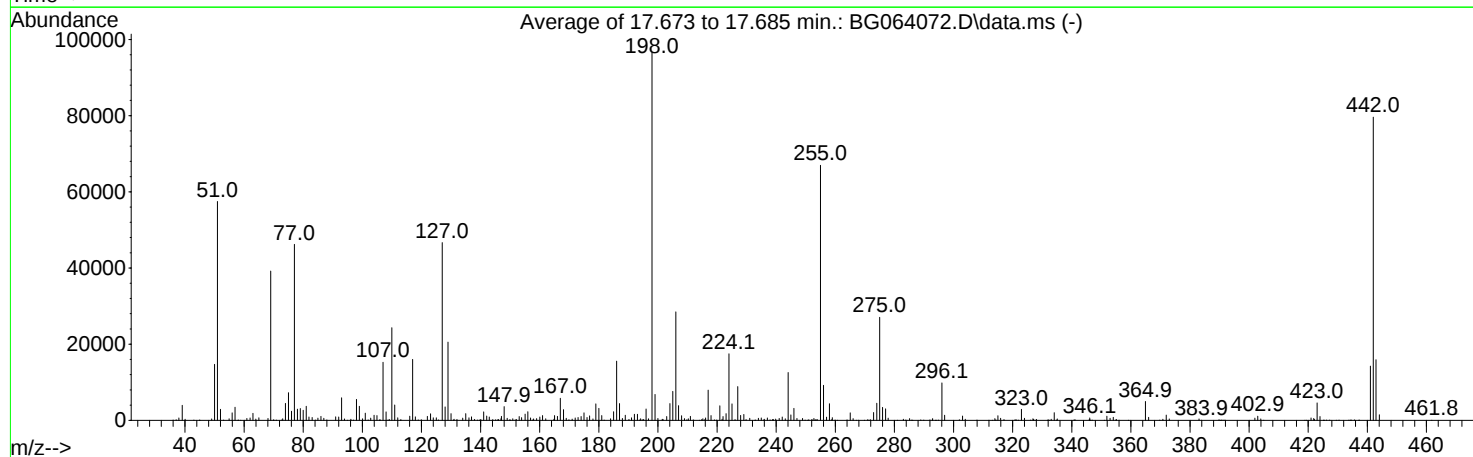


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031025\
Data File : BG064072.D
Acq On : 10 Mar 2025 8:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Mar 05 15:39:19 2025

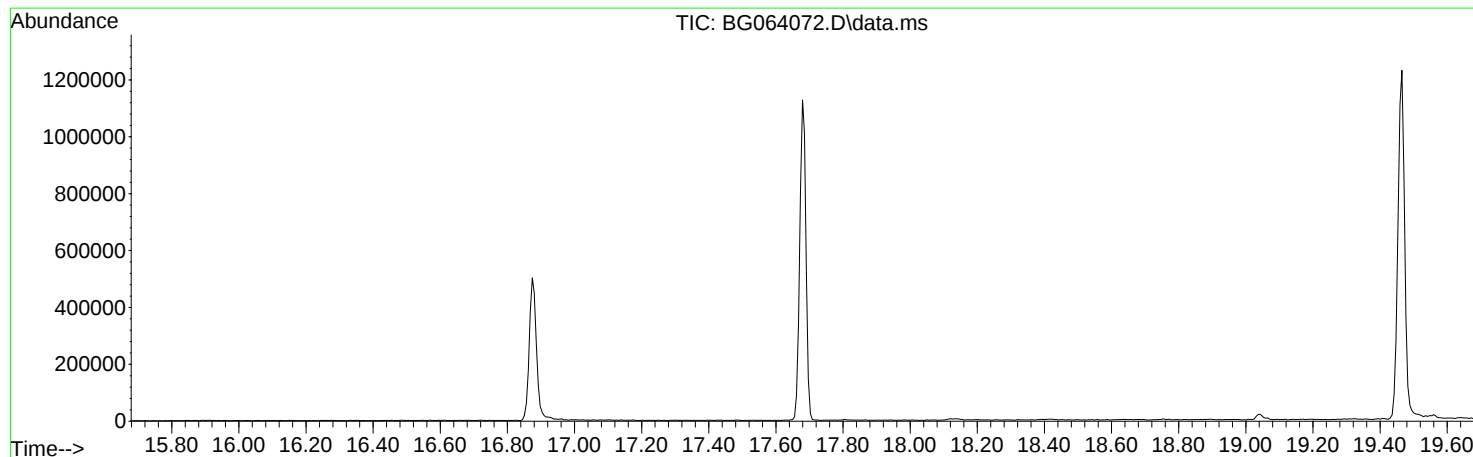

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.5	57453	PASS
68	69	0.00	2	1.3	493	PASS
69	198	0.00	100	40.6	39211	PASS
70	69	0.00	2	0.3	124	PASS
127	198	10	80	48.3	46659	PASS
197	198	0.00	2	0.4	406	PASS
198	198	100	100	100.0	96579	PASS
199	198	5	9	7.1	6824	PASS
275	198	10	60	28.0	27064	PASS
365	198	1	100	5.1	4947	PASS
441	198	0.01	100	14.7	14243	PASS
442	442	50	100	100.0	79621	PASS
443	442	15	24	20.0	15934	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/10/2025	BNA_G	<u>BG064072.D</u>
Compound Name	Response	Retention Time
DDT	255684	20.699
DDD	8972	20.258
DDE	1084	19.753
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10056	265740	3.78

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031025\
Data File : BG064072.D
Acq On : 10 Mar 2025 8:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 10 11:22:27 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 05 15:39:19 2025
Response via : Initial Calibration

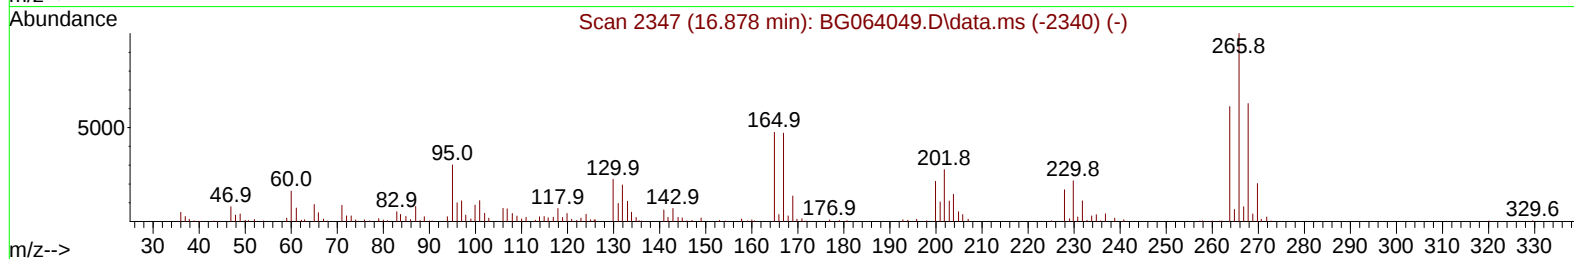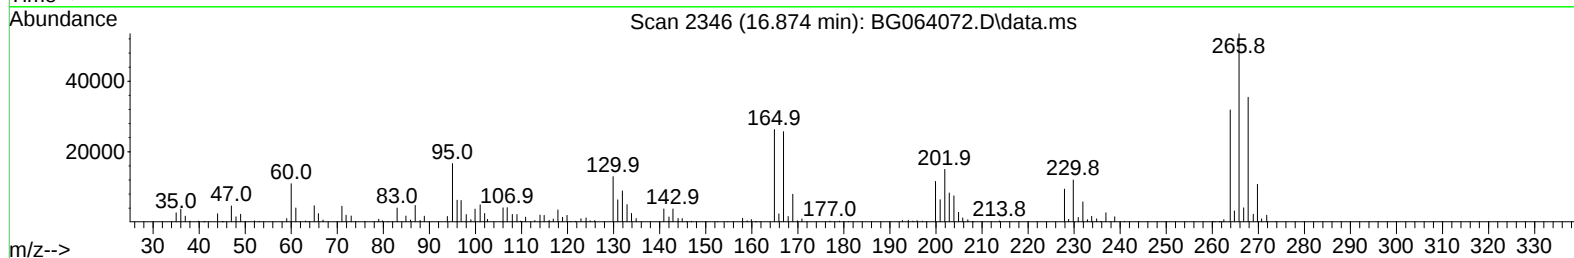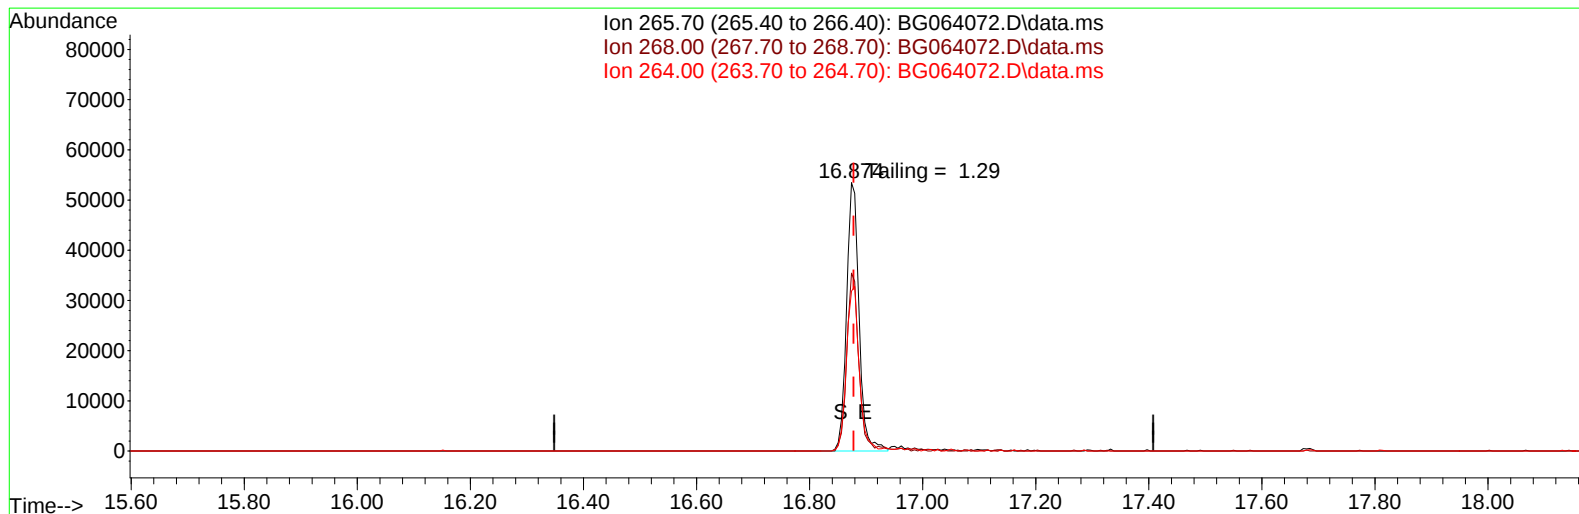

TIC: BG064072.D\data.ms

(70) Pentachlorophenol (C)

16.874min (-0.004) 137114.61 ng




response 81997

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	66.31
264.00	61.10	59.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031025\
Data File : BG064072.D
Acq On : 10 Mar 2025 8:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 10 11:22:27 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 05 15:39:19 2025
Response via : Initial Calibration

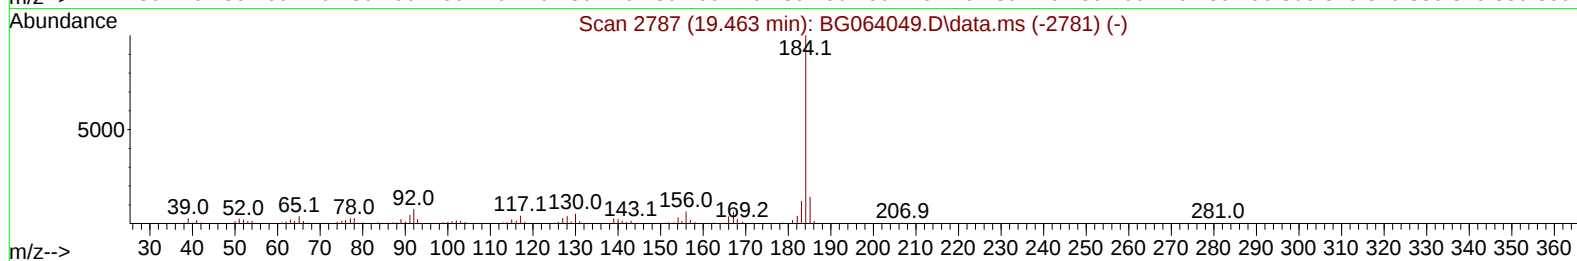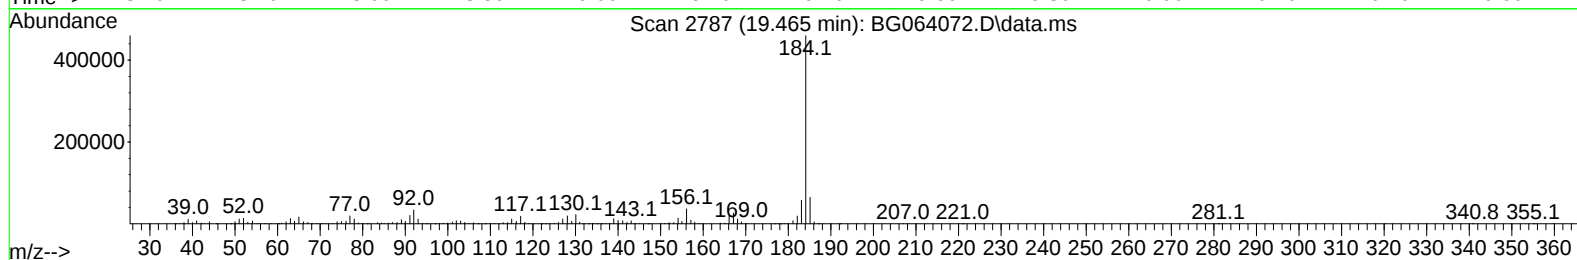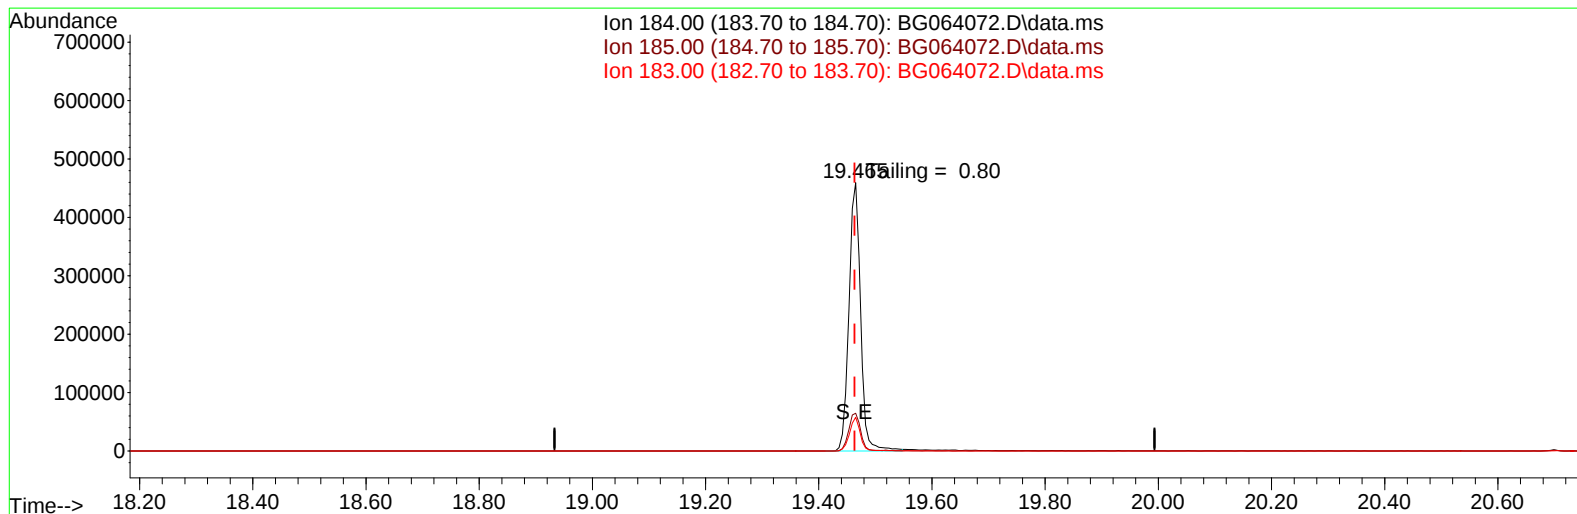

TIC: BG064072.D\data.ms

(77) Benzidine

19.465min (+ 0.002) 21680.85 ng

response 657177

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.11
183.00	11.90	12.58
0.00	0.00	0.00