




Data Path : S:\HPCHEM1\BNA\_G\DATA\BG031116\  
Data File : BG021420.D  
Acq On : 11 Mar 2016 15:26  
Operator : UM/SJ  
Sample : SSTDCCC020  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
BNA\_G  
LabSampleId :  
SSTD02032

Manual Integrations  
APPROVED

UMANGI  
3/11/2016 6:31:45 PM

Quant Time: Mar 11 17:34:16 2016  
Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\SOM02.2-EPA-BG031016.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Fri Mar 11 17:22:23 2016  
Response via : Initial Calibration

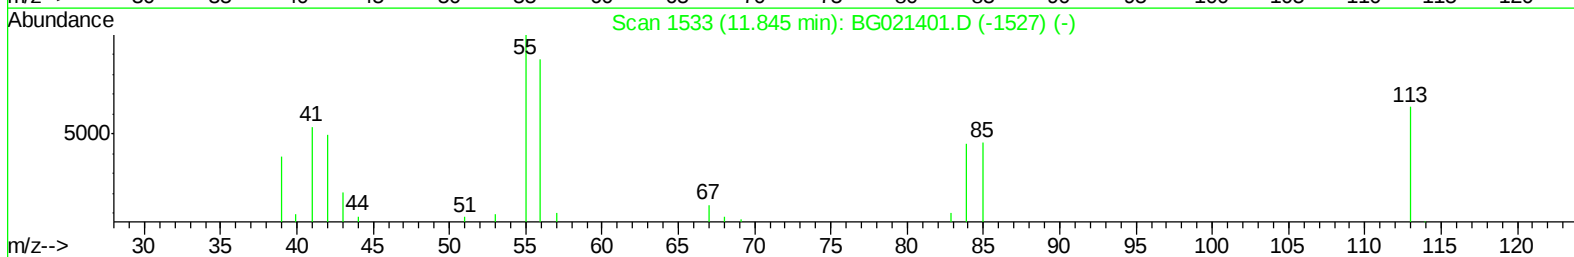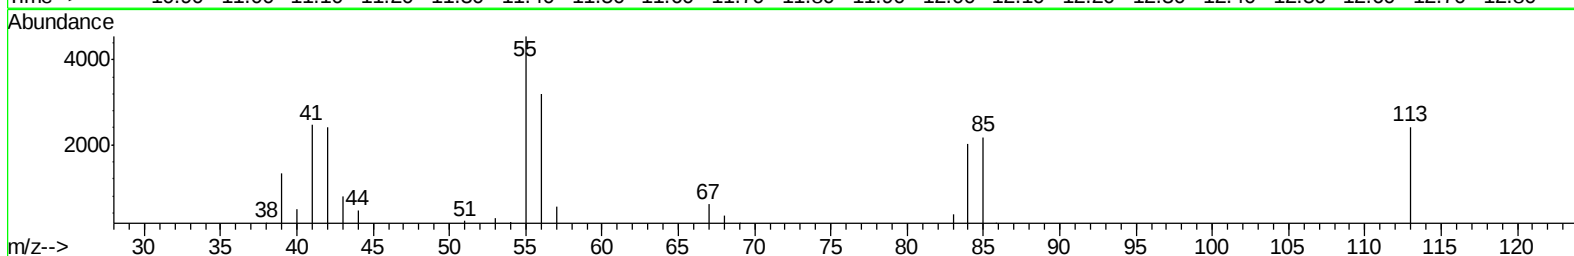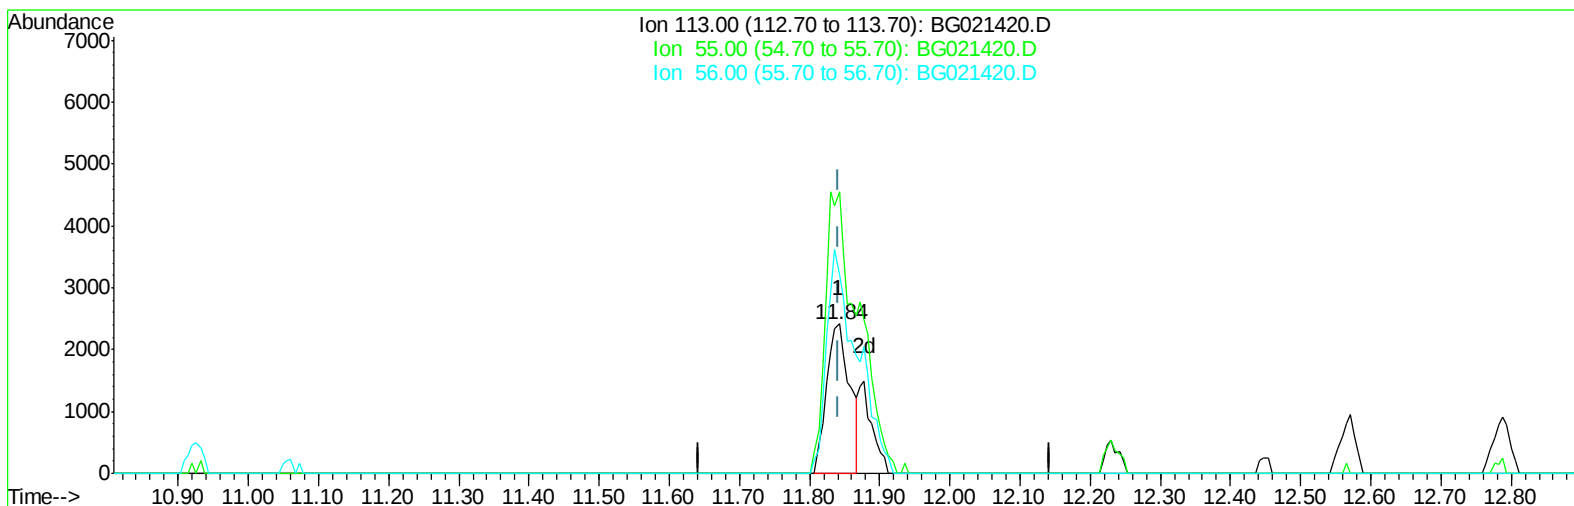

TIC: BG021420.D

(32) Caprolactam

11.842min (0.000) 13.17ng/ul

response 5471

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 113.00 | 100    | 100    |
| 55.00  | 194.40 | 188.37 |
| 56.00  | 132.10 | 132.78 |
| 0.00   | 0.00   | 0.00   |




Data Path : S:\HPCHEM1\BNA\_G\DATA\BG031116\  
Data File : BG021420.D  
Acq On : 11 Mar 2016 15:26  
Operator : UM/SJ  
Sample : SSTDCCC020  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
BNA\_G  
LabSampleId :  
SSTD02032

Manual Integrations  
APPROVED

UMANGI  
3/11/2016 6:31:45 PM

Quant Time: Mar 11 17:34:16 2016  
Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\SOM02.2-EPA-BG031016.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Fri Mar 11 17:22:23 2016  
Response via : Initial Calibration

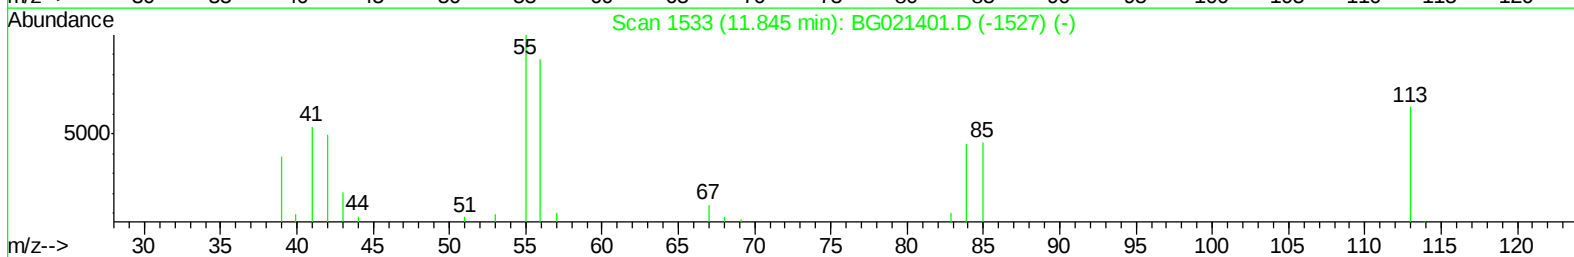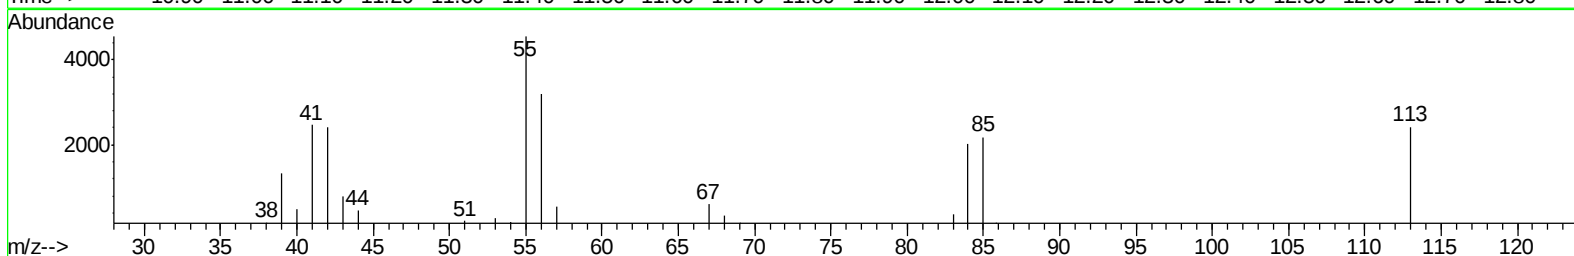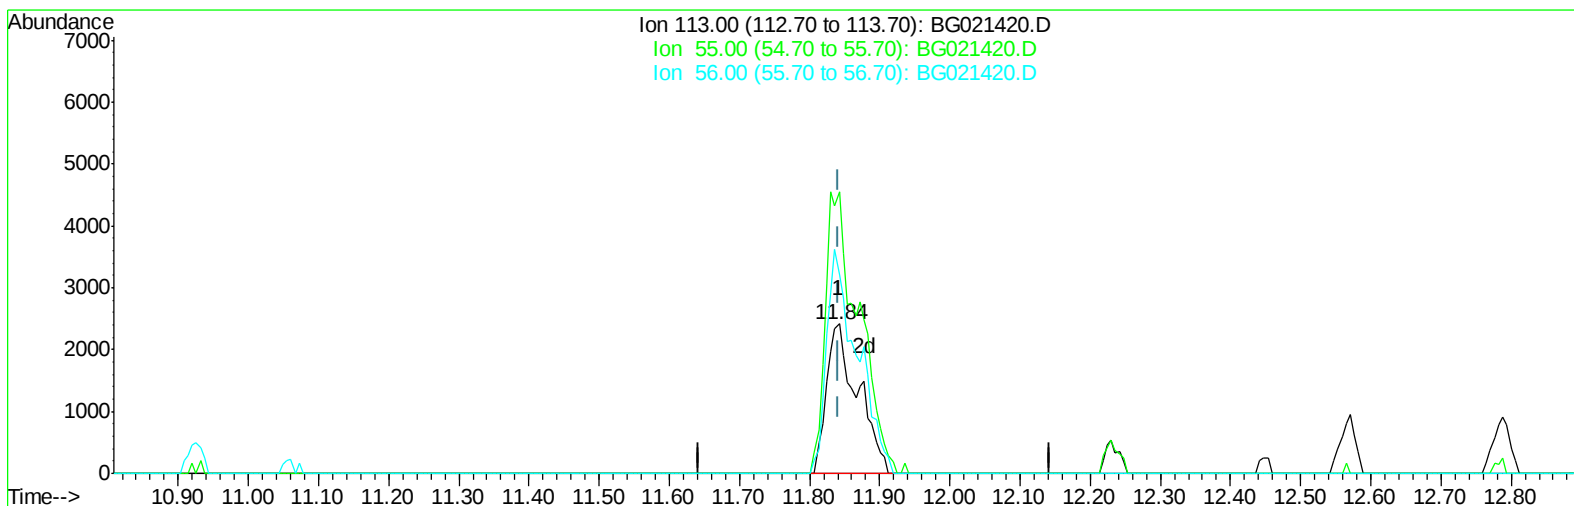

TIC: BG021420.D

(32) Caprolactam

11.842min (0.000) 18.02ng/ul m

response 7484

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 113.00 | 100    | 100    |
| 55.00  | 194.40 | 188.37 |
| 56.00  | 132.10 | 132.78 |
| 0.00   | 0.00   | 0.00   |

Data Path : S:\HPCHEM1\BNA\_G\DATA\BG031116\  
 Data File : BG021420.D  
 Acq On : 11 Mar 2016 15:26  
 Operator : UM/SJ  
 Sample : SSTDCCC020  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 LabSampleId :  
 SSTD02032

Manual Integrations  
 APPROVED

UMANGI  
 3/11/2016 6:31:45 PM

Quant Time: Mar 11 17:35:45 2016  
 Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\SOM02.2-EPA-BG031016.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Fri Mar 11 17:22:23 2016  
 Response via : Initial Calibration

| Internal Standards        | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|---------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 8.12  | 152  | 11601    | 20.00 | ng/ul | 0.00     |
| 18) Naphthalene-d8        | 10.93 | 136  | 57086    | 20.00 | ng/ul | 0.00     |
| 36) Acenaphthene-d10      | 14.73 | 164  | 35739    | 20.00 | ng/ul | 0.00     |
| 62) Phenanthrene-d10      | 17.46 | 188  | 86415    | 20.00 | ng/ul | 0.00     |
| 78) Chrysene-d12          | 21.73 | 240  | 90132    | 20.00 | ng/ul | 0.00     |
| 86) Perylene-d12          | 24.99 | 264  | 84413    | 20.00 | ng/ul | 0.00     |

## System Monitoring Compounds

|                                |       |     |       |       |       |      |
|--------------------------------|-------|-----|-------|-------|-------|------|
| 3) 1,4-Dioxane-d8              | 3.52  | 96  | 2016  | 8.15  | ng/uL | 0.00 |
| 5) Phenol-d5                   | 7.31  | 99  | 23738 | 18.08 | ng/ul | 0.00 |
| 7) Bis-(2-Chloroethyl)ether-d  | 7.44  | 67  | 16570 | 19.63 | ng/ul | 0.00 |
| 9) 2-Chlorophenol-d4           | 7.66  | 132 | 17626 | 19.66 | ng/ul | 0.00 |
| 13) 4-Methylphenol-d8          | 8.85  | 113 | 19474 | 18.35 | ng/ul | 0.00 |
| 19) Nitrobenzene-d5            | 9.29  | 128 | 9191  | 19.98 | ng/ul | 0.00 |
| 22) 2-Nitrophenol-d4           | 10.00 | 143 | 9925  | 19.65 | ng/ul | 0.00 |
| 26) 2,4-Dichlorophenol-d3      | 10.57 | 165 | 17414 | 18.97 | ng/ul | 0.00 |
| 29) 4-Chloroaniline-d4         | 11.06 | 131 | 24758 | 20.56 | ng/ul | 0.00 |
| 44) Dimethylphthalate-d6       | 14.13 | 166 | 59964 | 19.39 | ng/ul | 0.00 |
| 47) Acenaphthylene-d8          | 14.43 | 160 | 73212 | 19.42 | ng/ul | 0.00 |
| 52) 4-Nitrophenol-d4           | 15.00 | 143 | 10132 | 17.33 | ng/ul | 0.00 |
| 58) Fluorene-d10               | 15.71 | 176 | 52842 | 19.44 | ng/ul | 0.00 |
| 63) 4,6-Dinitro-2-methylphenol | 15.84 | 200 | 11209 | 19.39 | ng/ul | 0.00 |
| 71) Anthracene-d10             | 17.56 | 188 | 84164 | 19.51 | ng/ul | 0.00 |
| 79) Pyrene-d10                 | 19.84 | 212 | 89457 | 19.45 | ng/ul | 0.00 |
| 90) Benzo(a)pyrene-d12         | 24.76 | 264 | 88348 | 19.57 | ng/ul | 0.00 |

## Target Compounds

|                                |       |     |       |             | Qvalue |
|--------------------------------|-------|-----|-------|-------------|--------|
| 2) 1,4-Dioxane                 | 3.55  | 88  | 2585  | 7.77 ng/uL# | 87     |
| 4) Benzaldehyde                | 7.25  | 77  | 19093 | 22.76 ng/ul | 96     |
| 6) Phenol                      | 7.34  | 94  | 25940 | 18.65 ng/ul | 92     |
| 8) Bis(2-Chloroethyl)ether     | 7.53  | 93  | 19348 | 19.35 ng/ul | 97     |
| 10) 2-Chlorophenol             | 7.69  | 128 | 18264 | 18.98 ng/ul | 95     |
| 11) 2-Methylphenol             | 8.58  | 108 | 19161 | 18.39 ng/ul | 95     |
| 12) 2,2'-oxybis(1-Chloropropan | 8.64  | 45  | 31800 | 20.18 ng/ul | 98     |
| 14) Acetophenone               | 8.94  | 105 | 33317 | 18.99 ng/ul | 97     |
| 15) N-Nitroso-di-n-propylamine | 8.92  | 70  | 22418 | 19.89 ng/ul | 94     |
| 16) 4-Methylphenol             | 8.91  | 108 | 22114 | 18.82 ng/ul | 90     |
| 17) Hexachloroethane           | 9.20  | 117 | 8229  | 19.71 ng/ul | 87     |
| 20) Nitrobenzene               | 9.33  | 77  | 29573 | 20.00 ng/ul | 99     |
| 21) Isophorone                 | 9.84  | 82  | 56498 | 19.33 ng/ul | 98     |
| 23) 2-Nitrophenol              | 10.04 | 139 | 11156 | 19.01 ng/ul | 94     |
| 24) 2,4-Dimethylphenol         | 10.10 | 107 | 26546 | 19.38 ng/ul | 97     |
| 25) Bis(2-Chloroethoxy)methane | 10.32 | 93  | 27983 | 19.41 ng/ul | 98     |
| 27) 2,4-Dichlorophenol         | 10.60 | 162 | 17428 | 18.06 ng/ul | 91     |
| 28) Naphthalene                | 10.97 | 128 | 62882 | 19.64 ng/ul | 99     |
| 30) 4-Chloroaniline            | 11.08 | 127 | 26617 | 20.38 ng/ul | 96     |
| 31) Hexachlorobutadiene        | 11.25 | 225 | 12668 | 20.32 ng/ul | 97     |
| 32) Caprolactam                | 11.84 | 113 | 7484m | 18.02 ng/ul |        |
| 33) 4-Chloro-3-methylphenol    | 12.23 | 107 | 24389 | 17.83 ng/ul | 94     |
| 34) 2-Methylnaphthalene        | 12.57 | 142 | 45377 | 19.08 ng/ul | 99     |

Data Path : S:\HPCHEM1\BNA\_G\DATA\BG031116\  
 Data File : BG021420.D  
 Acq On : 11 Mar 2016 15:26  
 Operator : UM/SJ  
 Sample : SSTDCCC020  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 LabSampleId :  
 SSTD02032

Manual Integrations  
 APPROVED

UMANGI  
 3/11/2016 6:31:45 PM

Quant Time: Mar 11 17:35:45 2016  
 Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\SOM02.2-EPA-BG031016.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Fri Mar 11 17:22:23 2016  
 Response via : Initial Calibration

| Internal Standards             | R.T.  | QIon | Response | Conc  | Units  | Dev(Min) |
|--------------------------------|-------|------|----------|-------|--------|----------|
| 35) 1-Methylnaphthalene        | 12.79 | 142  | 43036    | 19.05 | ng/ul  | 98       |
| 37) 1,2,4,5-Tetrachlorobenzene | 12.93 | 216  | 23139    | 19.62 | ng/ul  | 90       |
| 38) Hexachlorocyclopentadiene  | 12.91 | 237  | 9121     | 13.33 | ng/ul# | 96       |
| 39) 2,4,6-Trichlorophenol      | 13.18 | 196  | 15721    | 18.53 | ng/ul  | 99       |
| 40) 2,4,5-Trichlorophenol      | 13.29 | 196  | 17504    | 18.57 | ng/ul  | 96       |
| 41) 1,1'-Biphenyl              | 13.56 | 154  | 59692    | 19.91 | ng/ul  | 96       |
| 42) 2-Chloronaphthalene        | 13.61 | 162  | 46154    | 19.80 | ng/ul  | 97       |
| 43) 2-Nitroaniline             | 13.82 | 65   | 21828    | 19.68 | ng/ul  | 96       |
| 45) Dimethylphthalate          | 14.17 | 163  | 63339    | 19.17 | ng/ul  | 98       |
| 46) 2,6-Dinitrotoluene         | 14.30 | 165  | 13399    | 19.37 | ng/ul  | 99       |
| 48) Acenaphthylene             | 14.46 | 152  | 75750    | 19.57 | ng/ul  | 98       |
| 49) 3-Nitroaniline             | 14.64 | 138  | 14088    | 20.68 | ng/ul# | 92       |
| 50) Acenaphthene               | 14.79 | 153  | 52195    | 19.44 | ng/ul  | 98       |
| 51) 2,4-Dinitrophenol          | 14.84 | 184  | 7822     | 22.57 | ng/ul  | 94       |
| 53) 4-Nitrophenol              | 15.01 | 109  | 14116    | 19.88 | ng/ul  | 97       |
| 54) Dibenzofuran               | 15.13 | 168  | 71431    | 19.31 | ng/ul  | 100      |
| 55) 2,4-Dinitrotoluene         | 15.09 | 165  | 20067    | 19.31 | ng/ul# | 97       |
| 56) 2,3,4,6-Tetrachlorophenol  | 15.36 | 232  | 13871    | 16.84 | ng/ul  | 94       |
| 57) Diethylphthalate           | 15.53 | 149  | 70510    | 19.41 | ng/ul  | 98       |
| 59) Fluorene                   | 15.77 | 166  | 62015    | 19.18 | ng/ul  | 98       |
| 60) 4-Chlorophenyl-phenylether | 15.76 | 204  | 31097    | 19.19 | ng/ul  | 96       |
| 61) 4-Nitroaniline             | 15.80 | 138  | 15686    | 19.22 | ng/ul  | 97       |
| 64) 4,6-Dinitro-2-methylphenol | 15.85 | 198  | 12311    | 19.64 | ng/ul# | 85       |
| 65) N-Nitrosodiphenylamine     | 15.97 | 169  | 54480    | 19.02 | ng/ul  | 98       |
| 66) 4-Bromophenyl-phenylether  | 16.65 | 248  | 18491    | 18.95 | ng/ul  | 97       |
| 67) Hexachlorobenzene          | 16.77 | 284  | 19012    | 18.32 | ng/ul  | 99       |
| 68) Atrazine                   | 16.91 | 200  | 21477    | 19.74 | ng/ul  | 98       |
| 69) Pentachlorophenol          | 17.12 | 266  | 9260     | 15.86 | ng/ul  | 90       |
| 70) Phenanthrene               | 17.51 | 178  | 98730    | 19.20 | ng/ul  | 99       |
| 72) Anthracene                 | 17.60 | 178  | 100107   | 19.13 | ng/ul  | 98       |
| 73) 1,2,3,4-Tetrachlorobenzene | 13.53 | 216  | 22099    | 20.09 | ng/uL  | 92       |
| 74) Pentachlorobenzene         | 15.04 | 250  | 22397    | 19.08 | ng/uL  | 98       |
| 75) Carbazole                  | 17.87 | 167  | 87960    | 19.44 | ng/ul  | 99       |
| 76) Di-n-butylphthalate        | 18.41 | 149  | 120964   | 19.62 | ng/ul  | 99       |
| 77) Fluoranthene               | 19.51 | 202  | 113191   | 19.07 | ng/ul  | 98       |
| 80) Pyrene                     | 19.87 | 202  | 118435   | 19.64 | ng/ul  | 98       |
| 81) Butylbenzylphthalate       | 20.74 | 149  | 54446    | 19.66 | ng/ul  | 96       |
| 82) 3,3'-Dichlorobenzidine     | 21.62 | 252  | 42255    | 21.32 | ng/ul  | 95       |
| 83) Benzo(a)anthracene         | 21.71 | 228  | 112027   | 19.04 | ng/ul  | 98       |
| 84) Bis(2-ethylhexyl)phthalate | 21.59 | 149  | 79574    | 19.31 | ng/ul  | 99       |
| 85) Chrysene                   | 21.78 | 228  | 104942   | 19.27 | ng/ul  | 98       |
| 87) Di-n-octyl phthalate       | 22.81 | 149  | 138350   | 19.84 | ng/ul  | 100      |
| 88) Benzo(b)fluoranthene       | 23.95 | 252  | 110005   | 19.05 | ng/ul  | 99       |
| 89) Benzo(k)fluoranthene       | 24.02 | 252  | 109199   | 19.42 | ng/ul  | 98       |
| 91) Benzo(a)pyrene             | 24.83 | 252  | 107307   | 18.92 | ng/ul  | 98       |
| 92) Indeno(1,2,3-cd)pyrene     | 28.70 | 276  | 121119   | 19.45 | ng/ul  | 98       |
| 93) Dibenzo(a,h)anthracene     | 28.76 | 278  | 103208   | 19.50 | ng/ul  | 98       |
| 94) Benzo(g,h,i)perylene       | 29.87 | 276  | 99360    | 19.34 | ng/ul# | 95       |

Data Path : S:\HPCHEM1\BNA\_G\DATA\BG031116\  
Data File : BG021420.D  
Acq On : 11 Mar 2016 15:26  
Operator : UM/SJ  
Sample : SSTDCCC020  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
BNA\_G  
LabSampleId :  
SSTD02032

Manual Integrations  
APPROVED

UMANGI  
3/11/2016 6:31:45 PM

Quant Time: Mar 11 17:35:45 2016  
Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\SOM02.2-EPA-BG031016.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Fri Mar 11 17:22:23 2016  
Response via : Initial Calibration

| Internal Standards                                                   | R.T. | QIon | Response | Conc | Units | Dev(Min) |
|----------------------------------------------------------------------|------|------|----------|------|-------|----------|
| -----                                                                |      |      |          |      |       |          |
| (#)=qualifier out of range (m)=manual integration (+)=signals summed |      |      |          |      |       |          |

Data Path : S:\HPCHEM1\BNA\_G\DATA\BG031116\  
Data File : BG021420.D  
Acq On : 11 Mar 2016 15:26  
Operator : UM/SJ  
Sample : SSTDCCC020  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
BNA\_G  
LabSampleId :  
SSTD02032

Manual Integrations  
APPROVED

UMANGI  
3/11/2016 6:31:45 PM

Quant Time: Mar 11 17:35:45 2016  
Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\SOM02.2-EPA-BG031016.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Fri Mar 11 17:22:23 2016  
Response via : Initial Calibration

