


Data Path : S:\HPCHEM1\BNA_G\DATA\BG031116\
Data File : BG021419.D
Acq On : 11 Mar 2016 11:47
Operator : UM/SJ
Sample : DFTPP07
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP07

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031016.M
Title : SVOA CALIBRATION
Last Update : Fri Mar 11 00:30:31 2016

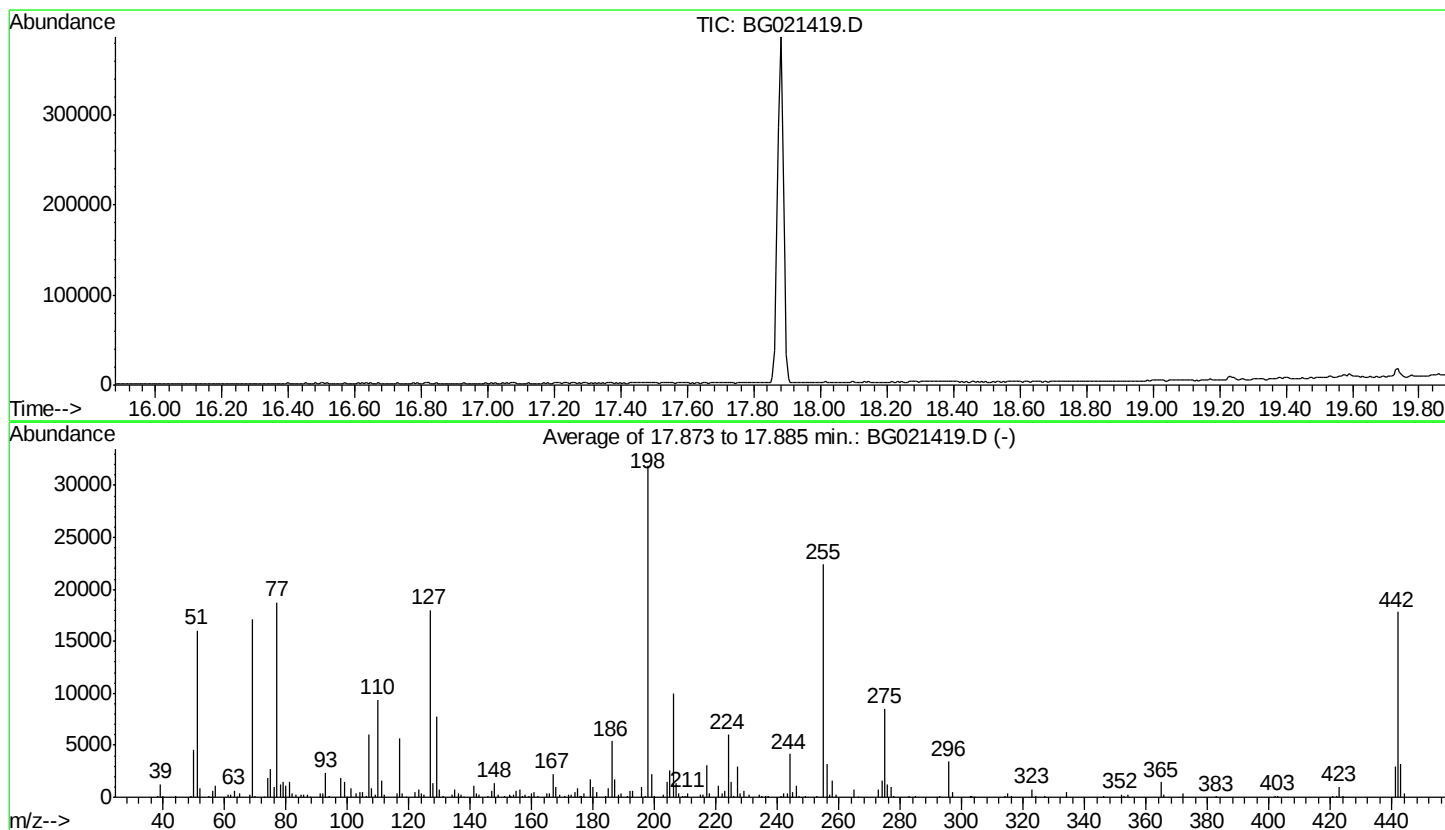

AutoFind: Scans 2559, 2560, 2561; Background Corrected with Scan 2554

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.2	16016	PASS
68	69	0.00	2	1.6	278	PASS
69	198	0.00	100	53.8	17152	PASS
70	69	0.00	2	0.7	115	PASS
127	198	10	80	56.4	17983	PASS
197	198	0.00	2	0.2	76	PASS
198	198	100	100	100.0	31901	PASS
199	198	5	9	7.1	2271	PASS
275	198	10	60	26.8	8562	PASS
365	198	1	100	4.5	1429	PASS
441	442	0.01	100	16.4	2922	PASS
442	198	50	100	56.0	17852	PASS
443	442	15	24	18.2	3243	PASS

m/z	Abundance
37.90	186.0
39.00	1295.0
41.00	232.0
43.00	260.0
49.00	628.0
50.00	4916.0
51.00	16102.0
52.00	872.0
55.00	239.0
55.90	516.0
57.00	1259.0
60.90	206.0
62.00	228.0
63.00	572.0
65.00	338.0
68.00	455.0
68.90	16632.0
70.10	178.0
72.90	316.0
74.00	1985.0
74.90	2588.0
76.00	854.0
77.00	18992.0
78.00	1375.0
78.90	1468.0
79.90	885.0
80.90	1416.0
81.90	411.0
83.00	456.0
83.90	364.0
84.90	289.0
85.90	592.0
86.90	245.0
90.90	387.0
91.90	376.0
92.90	2517.0
93.90	201.0
97.90	1819.0
98.90	1395.0
99.90	154.0
100.90	709.0
102.90	269.0
103.90	500.0
104.90	463.0
105.90	246.0
106.90	5536.0
107.90	809.0
109.00	235.0
109.90	8903.0
110.90	1412.0
111.90	254.0
115.90	315.0
116.90	5302.0
117.90	408.0
121.90	311.0
123.00	609.0
123.90	248.0
124.90	197.0
126.90	16664.0
127.90	1425.0
128.90	7004.0
129.90	687.0
130.90	171.0
133.80	198.0
134.90	615.0
135.90	366.0
136.90	280.0
140.90	981.0
141.90	242.0
142.90	295.0
145.80	243.0
146.90	620.0
147.90	1176.0
148.90	319.0
152.80	372.0
153.90	176.0
154.90	466.0
155.90	655.0
157.00	155.0
157.90	220.0
158.90	182.0
159.90	353.0
160.80	442.0
161.90	164.0
164.80	344.0
165.90	258.0
166.90	2189.0
167.90	761.0
168.90	217.0
170.90	182.0
171.90	228.0

Instrument :
BNA_G
ClientSampleId :
DFTPP07

172.80	232.0
173.90	479.0
174.90	927.0
175.80	250.0
176.90	341.0
178.80	1402.0
179.90	952.0
180.90	458.0
184.90	603.0
185.90	4745.0
186.90	1612.0
187.90	216.0
188.80	353.0
191.90	519.0
192.90	525.0
195.80	986.0
196.80	228.0
197.80	27344.0
198.90	1865.0
202.80	279.0
203.90	1298.0
204.90	1964.0
205.90	8489.0
206.90	1359.0
207.90	385.0
210.00	203.0
210.90	429.0
214.90	153.0
215.80	233.0
216.90	2835.0
217.80	354.0
220.90	950.0
221.80	404.0
222.90	478.0
223.90	4915.0
224.90	1302.0
226.90	2431.0
227.80	262.0
228.90	413.0
230.90	205.0
233.90	200.0
236.80	179.0
240.90	151.0
241.80	288.0
242.90	440.0
243.90	3524.0
244.90	360.0
245.90	923.0
246.90	186.0
254.90	18520.0
255.90	2453.0
256.80	213.0
257.90	1217.0
258.90	259.0
264.90	671.0
272.90	533.0
273.90	1387.0
274.90	6392.0
275.90	1036.0
276.90	845.0
277.90	172.0
284.80	153.0
295.80	2435.0
296.90	460.0
314.00	172.0
314.80	265.0
322.90	553.0
333.90	498.0
345.80	160.0
351.90	191.0
353.90	241.0
364.80	1055.0
365.80	162.0
371.80	234.0
422.90	700.0
440.90	2059.0
441.90	11781.0
442.90	2111.0
443.90	289.0

Instrument :
BNA_G
ClientSampleId :
DFTPP07

m/z	Abundance
38.00	266.0
39.00	1363.0
40.00	276.0
41.00	218.0
43.00	270.0
44.10	186.0
48.90	635.0
50.00	5227.0
51.00	18768.0
52.00	993.0
55.00	429.0
55.90	774.0
56.90	1378.0
61.00	287.0
61.90	313.0
62.90	831.0
64.00	161.0
65.00	378.0
68.90	20496.0
69.90	167.0
72.90	336.0
74.00	2091.0
75.00	3168.0
76.00	1173.0
77.00	21912.0
78.00	1272.0
78.90	1673.0
79.90	1387.0
80.90	1759.0
81.90	335.0
82.90	457.0
83.80	473.0
84.90	317.0
85.90	675.0
87.00	312.0
87.80	190.0
90.90	513.0
91.90	471.0
92.90	2552.0
97.90	2349.0
98.90	1851.0
100.90	981.0
102.90	418.0
103.90	703.0
104.90	671.0
105.90	213.0
106.90	7489.0
107.90	1128.0
109.00	218.0
109.90	11508.0
110.90	1742.0
111.90	200.0
115.90	576.0
116.90	6830.0
117.90	465.0
121.90	590.0
122.90	882.0
123.80	349.0
124.90	331.0
126.90	21048.0
127.90	1549.0
128.90	9448.0
129.90	812.0
130.90	188.0
133.90	310.0
134.90	875.0
135.90	371.0
136.90	375.0
137.80	160.0
140.90	1400.0
141.90	398.0
142.80	262.0
145.90	190.0
146.90	683.0
147.90	1665.0
148.80	240.0
152.80	311.0
153.90	247.0
154.90	717.0
156.00	1005.0
157.00	181.0
157.90	203.0
158.90	273.0
159.90	368.0
160.80	459.0
161.80	247.0
164.80	493.0
165.80	443.0
166.90	2522.0
167.90	1278.0
168.90	234.0

Instrument :
BNA_G
ClientSampleId :
DFTPP07

170.80	190.0
171.90	194.0
172.90	290.0
173.90	465.0
174.90	1138.0
176.00	288.0
176.90	467.0
178.90	2233.0
179.90	1134.0
180.90	628.0
183.90	232.0
185.00	952.0
185.90	6735.0
186.90	1968.0
188.00	252.0
188.80	356.0
191.00	236.0
191.90	727.0
192.90	695.0
195.90	1108.0
197.80	37848.0
198.80	2828.0
199.90	275.0
202.80	349.0
203.90	1668.0
204.90	3168.0
205.90	11580.0
206.90	1896.0
207.90	519.0
208.80	188.0
209.90	287.0
210.80	418.0
214.90	264.0
215.90	375.0
216.80	3623.0
217.80	518.0
220.90	1290.0
221.80	423.0
222.90	665.0
223.90	7303.0
224.90	1753.0
225.80	192.0
226.90	3574.0
227.90	558.0
228.90	703.0
230.80	234.0
233.80	221.0
234.90	211.0
235.90	153.0
236.80	253.0
240.90	245.0
241.80	432.0
242.90	461.0
243.90	4741.0
244.90	690.0
245.90	1202.0
246.80	236.0
248.80	245.0
252.90	206.0
254.90	26216.0
255.90	3958.0
256.80	360.0
257.90	2067.0
258.90	309.0
264.80	813.0
265.90	171.0
272.80	856.0
273.90	1691.0
274.90	10643.0
275.80	1462.0
276.80	1225.0
277.80	217.0
282.90	242.0
284.80	174.0
292.90	209.0
295.90	3882.0
296.90	533.0
302.80	420.0
303.90	178.0
313.80	215.0
314.90	360.0
315.90	249.0
322.90	911.0
323.90	220.0
326.90	181.0
333.90	583.0
345.90	194.0
351.80	246.0
352.80	175.0
353.90	181.0
364.90	1542.0
365.80	240.0
371.90	382.0
401.80	153.0
402.80	250.0

Instrument :
BNA_G
ClientSampleId :
DFTPP07

420.90	151.0
421.90	177.0
422.90	1049.0
423.90	223.0
440.90	3333.0
441.90	20752.0
442.90	3997.0
443.80	333.0

Instrument :
BNA_G
ClientSampleId :
DFTPP07

m/z	Abundance
39.00	1042.0
41.00	247.0
43.00	262.0
44.00	154.0
49.00	619.0
50.00	3609.0
51.00	13669.0
51.90	585.0
55.00	241.0
56.00	457.0
57.00	1048.0
60.90	164.0
61.90	235.0
63.00	492.0
64.90	315.0
68.00	380.0
68.90	14781.0
72.90	447.0
74.00	1654.0
74.90	2429.0
76.00	902.0
77.00	15303.0
78.00	1064.0
79.00	1240.0
79.90	966.0
80.90	1251.0
81.90	424.0
82.90	287.0
83.90	438.0
84.90	322.0
85.90	546.0
86.90	220.0
90.80	243.0
91.90	312.0
92.90	2106.0
97.90	1477.0
98.90	1101.0
100.90	754.0
102.90	302.0
103.80	447.0
104.90	457.0
106.90	5258.0
107.90	742.0
109.00	199.0
109.90	7776.0
110.90	1486.0
111.90	173.0
115.90	214.0
116.90	4929.0
117.90	319.0
119.00	158.0
121.90	453.0
122.90	691.0
123.90	355.0
124.90	202.0
126.90	16239.0
127.90	1077.0
128.90	7017.0
129.90	615.0
133.90	345.0
134.90	698.0
135.90	240.0
136.90	262.0
140.90	1100.0
141.90	318.0
142.80	208.0
146.90	647.0
147.90	1325.0
148.90	218.0
151.00	234.0
153.00	331.0
153.90	219.0
154.90	537.0
155.90	724.0
157.80	216.0
159.90	370.0
160.90	546.0
164.90	397.0
165.90	337.0
166.90	2054.0
167.90	872.0
168.80	179.0
171.90	184.0
172.90	252.0
174.00	445.0
174.90	717.0
176.90	296.0
178.90	1500.0
179.90	1048.0
180.90	518.0
184.90	943.0

Instrument :
BNA_G
ClientSampleId :
DFTPP07

185.90	4753.0
186.90	1465.0
187.90	172.0
188.80	414.0
190.80	222.0
191.90	543.0
192.90	598.0
195.90	885.0
197.80	30512.0
198.80	2120.0
199.80	162.0
202.80	305.0
203.90	1647.0
204.90	2508.0
205.90	10035.0
206.90	1543.0
207.90	390.0
208.90	213.0
210.20	184.0
210.90	406.0
214.90	174.0
215.80	315.0
216.90	2939.0
217.80	374.0
220.80	1030.0
221.90	270.0
222.90	578.0
223.90	5739.0
224.90	1387.0
225.90	204.0
226.90	2904.0
227.90	333.0
228.90	568.0
230.90	183.0
233.80	291.0
234.90	215.0
235.90	150.0
240.90	154.0
241.80	255.0
243.00	331.0
243.90	4209.0
244.90	605.0
245.90	1055.0
248.80	199.0
254.90	22480.0
255.90	3158.0
256.80	298.0
257.90	1582.0
259.00	264.0
264.90	646.0
272.90	710.0
273.90	1813.0
274.90	8651.0
275.90	1347.0
276.90	1077.0
295.90	3887.0
296.90	602.0
303.00	411.0
314.80	388.0
315.90	221.0
322.90	857.0
323.80	159.0
326.90	168.0
333.90	460.0
346.00	180.0
351.80	364.0
352.80	179.0
353.80	187.0
364.80	1691.0
365.80	258.0
371.90	336.0
382.80	216.0
401.80	168.0
402.80	267.0
420.80	158.0
421.90	154.0
422.90	1216.0
423.90	272.0
440.90	3375.0
441.90	21024.0
442.90	3622.0
443.90	363.0

Instrument :
BNA_G
ClientSampleId :
DFTPP07

Scan 2554 (17.844 min): BG021419.D
DFTPP07

m/z	Abundance
40.90	341.0
43.00	299.0
46.90	167.0
48.90	556.0
51.00	163.0
54.90	227.0
57.00	176.0
69.00	151.0
72.90	309.0
83.00	173.0
83.80	490.0
85.80	318.0
206.90	191.0

Instrument :
BNA_G
ClientSampleId :
DFTPP07