
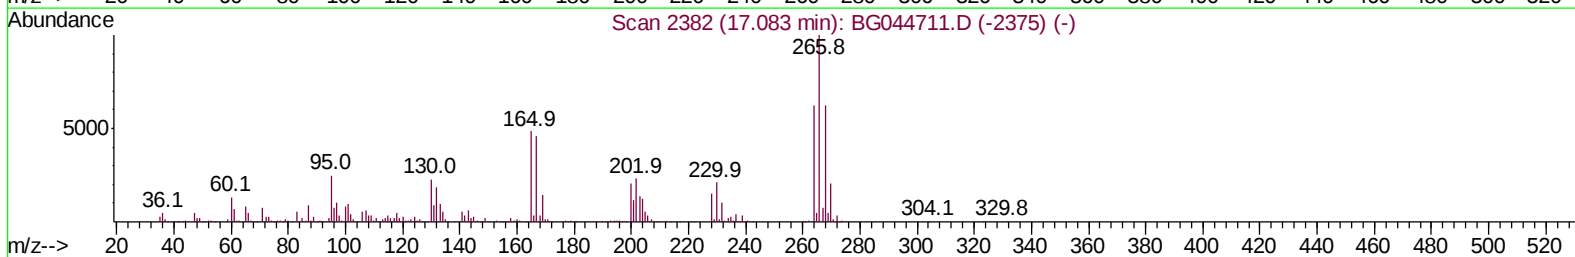
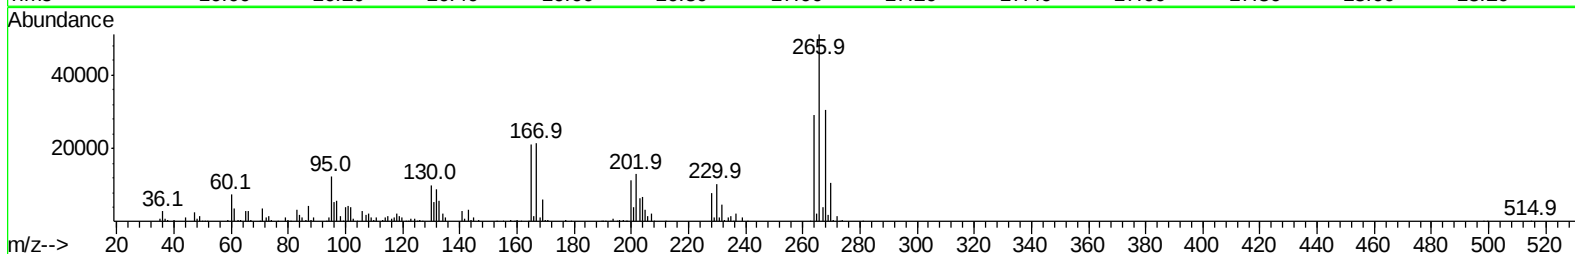


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG031120\
Data File : BG044717.D
Acq On : 11 Mar 2020 11:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 12 05:58:12 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG031020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 10 16:27:39 2020
Response via : Initial Calibration

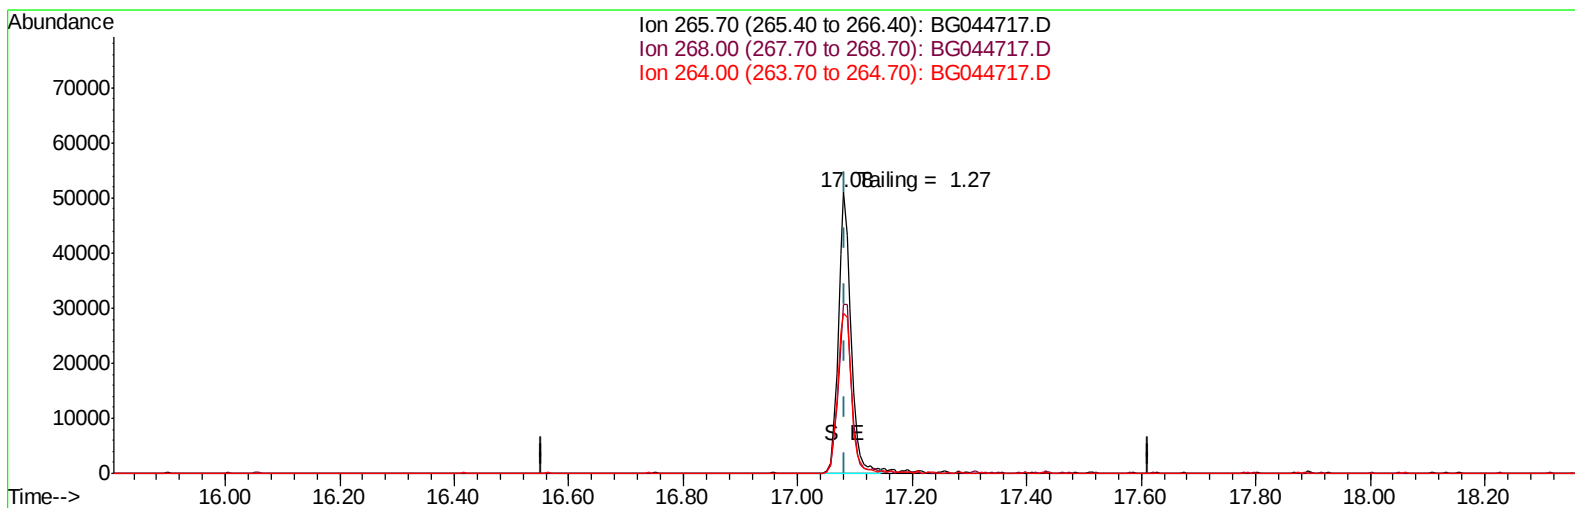

TIC: BG044717.D

(70) Pentachlorophenol (C)



17.080min (-0.003) 14636.92ng

response 79626

Ion	Exp%	Act%
265.70	100	100
268.00	62.40	59.88
264.00	62.40	56.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG031120\
 Data File : BG044717.D
 Acq On : 11 Mar 2020 11:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 12 05:58:12 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG031020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 10 16:27:39 2020
 Response via : Initial Calibration

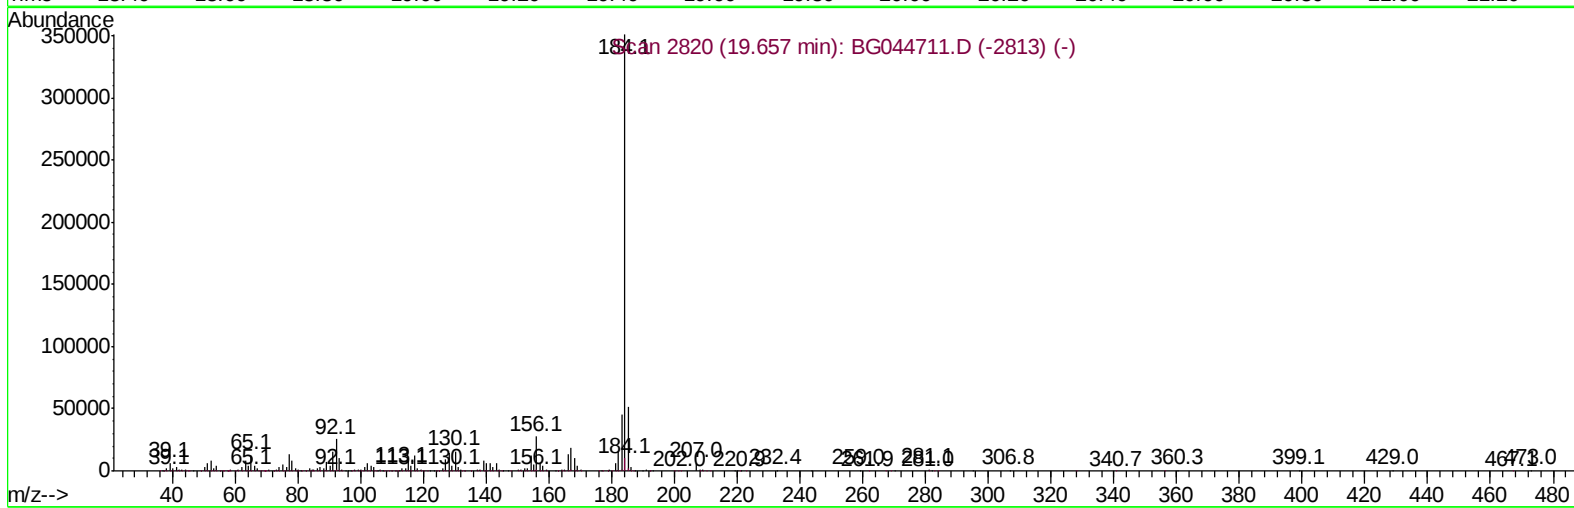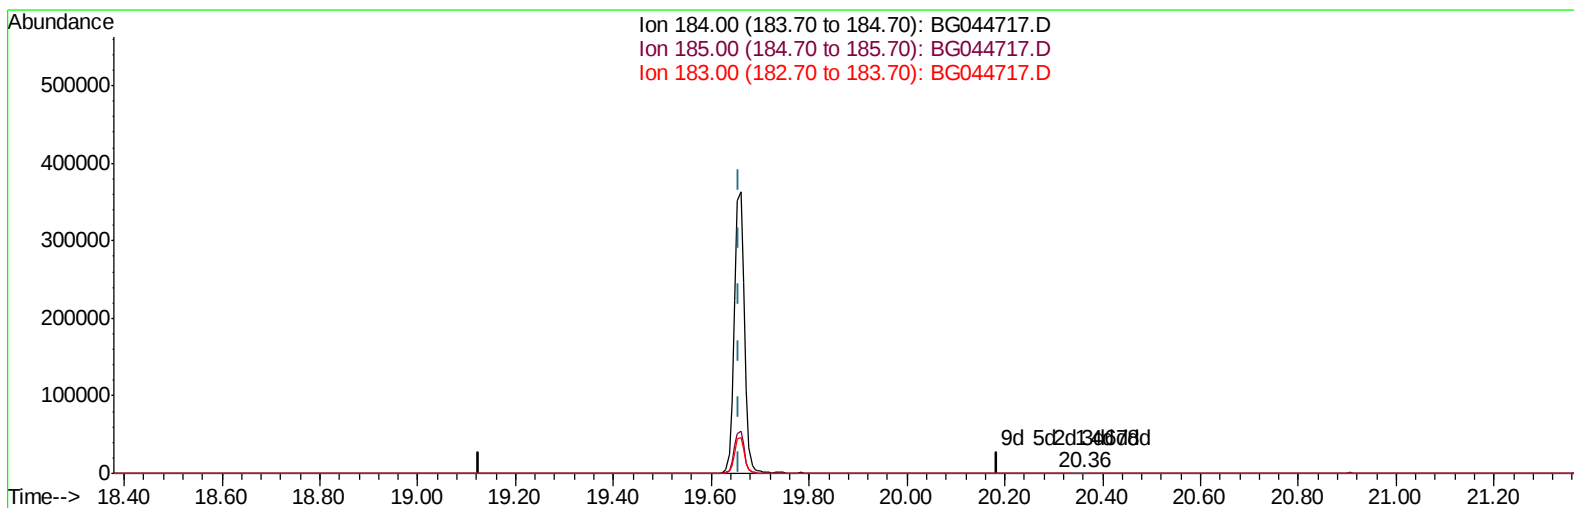

TIC: BG044717.D

(77) Benzidine

20.359min (+0.702) 155.53ng

response 308

Ion	Exp%	Act%
184.00	100	100
185.00	16.10	0.00#
183.00	13.20	0.00#
0.00	0.00	0.00