

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG031120\
 Data File : BG044724.D
 Acq On : 11 Mar 2020 17:52
 Operator : CG/JU
 Sample : L1798-06DL 5X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PT-ACIDS-WPDL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031020.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.161	7	12	18	rVB2	69310	140933	7.40%	0.655%
2	3.238	21	25	34	rVB2	99777	164010	8.61%	0.763%
3	5.165	349	353	359	rVB2	22210	32940	1.73%	0.153%
4	5.623	425	431	441	rVB	388686	667434	35.03%	3.103%
5	7.210	691	701	711	rBV	430985	736741	38.66%	3.426%
6	7.627	763	772	780	rBV	357851	636150	33.38%	2.958%
7	8.062	839	846	855	rVB	322122	559620	29.37%	2.602%
8	8.385	895	901	909	rBV	315005	569065	29.86%	2.646%
9	8.496	914	920	928	rVB	294868	498666	26.17%	2.319%
10	8.814	967	974	982	rBV	465507	813454	42.69%	3.782%
11	9.219	1035	1043	1050	rBV	248595	464718	24.39%	2.161%
12	9.977	1161	1172	1176	rBV2	128992	241443	12.67%	1.123%
13	10.036	1176	1182	1190	rVB	274962	488282	25.62%	2.270%
14	10.512	1255	1263	1273	rBV2	279434	503105	26.40%	2.339%
15	10.870	1315	1324	1334	rBV	423406	784458	41.17%	3.647%
16	11.046	1347	1354	1362	rVB	149842	272389	14.29%	1.266%
17	12.133	1531	1539	1547	rBV2	424892	733120	38.47%	3.409%
18	13.120	1700	1707	1713	rBV	217534	364005	19.10%	1.692%
19	13.191	1713	1719	1730	rVB	241289	400748	21.03%	1.863%
20	13.320	1733	1741	1748	rBV	720342	1119434	58.75%	5.205%
21	14.695	1966	1975	1983	rBV	703027	1133030	59.46%	5.268%
22	14.777	1983	1989	1997	rBV	139420	230704	12.11%	1.073%
23	14.877	1999	2006	2015	rBV	370880	622526	32.67%	2.894%
24	15.800	2158	2163	2171	rBV	294099	462271	24.26%	2.149%
25	16.176	2220	2227	2235	rBV	516365	810004	42.51%	3.766%
26	17.086	2375	2382	2390	rBV	649842	997692	52.36%	4.639%
27	17.439	2435	2442	2451	rBV	901739	1416034	74.31%	6.584%
28	20.047	2880	2886	2892	rBV	1407126	1905542	100.00%	8.860%
29	21.704	3162	3168	3177	rVB2	958136	1645355	86.35%	7.650%
30	23.279	3432	3436	3442	rVB4	44955	74305	3.90%	0.345%
31	24.102	3571	3576	3584	rVB3	62835	122855	6.45%	0.571%
32	24.930	3707	3717	3728	rVB	553904	1623731	85.21%	7.550%
33	25.077	3737	3742	3751	rVB5	59523	140132	7.35%	0.652%
34	26.228	3933	3938	3948	rVB7	42546	132347	6.95%	0.615%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG031120\
Data File : BG044724.D
Acq On : 11 Mar 2020 17:52
Operator : CG/JU
Sample : L1798-06DL 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PT-ACIDS-WPDL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031020.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION


Sum of corrected areas: 21507243

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG031120\
Data File : BG044724.D
Acq On : 11 Mar 2020 17:52
Operator : CG/JU
Sample : L1798-06DL 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PT-ACIDS-WPDL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG031020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

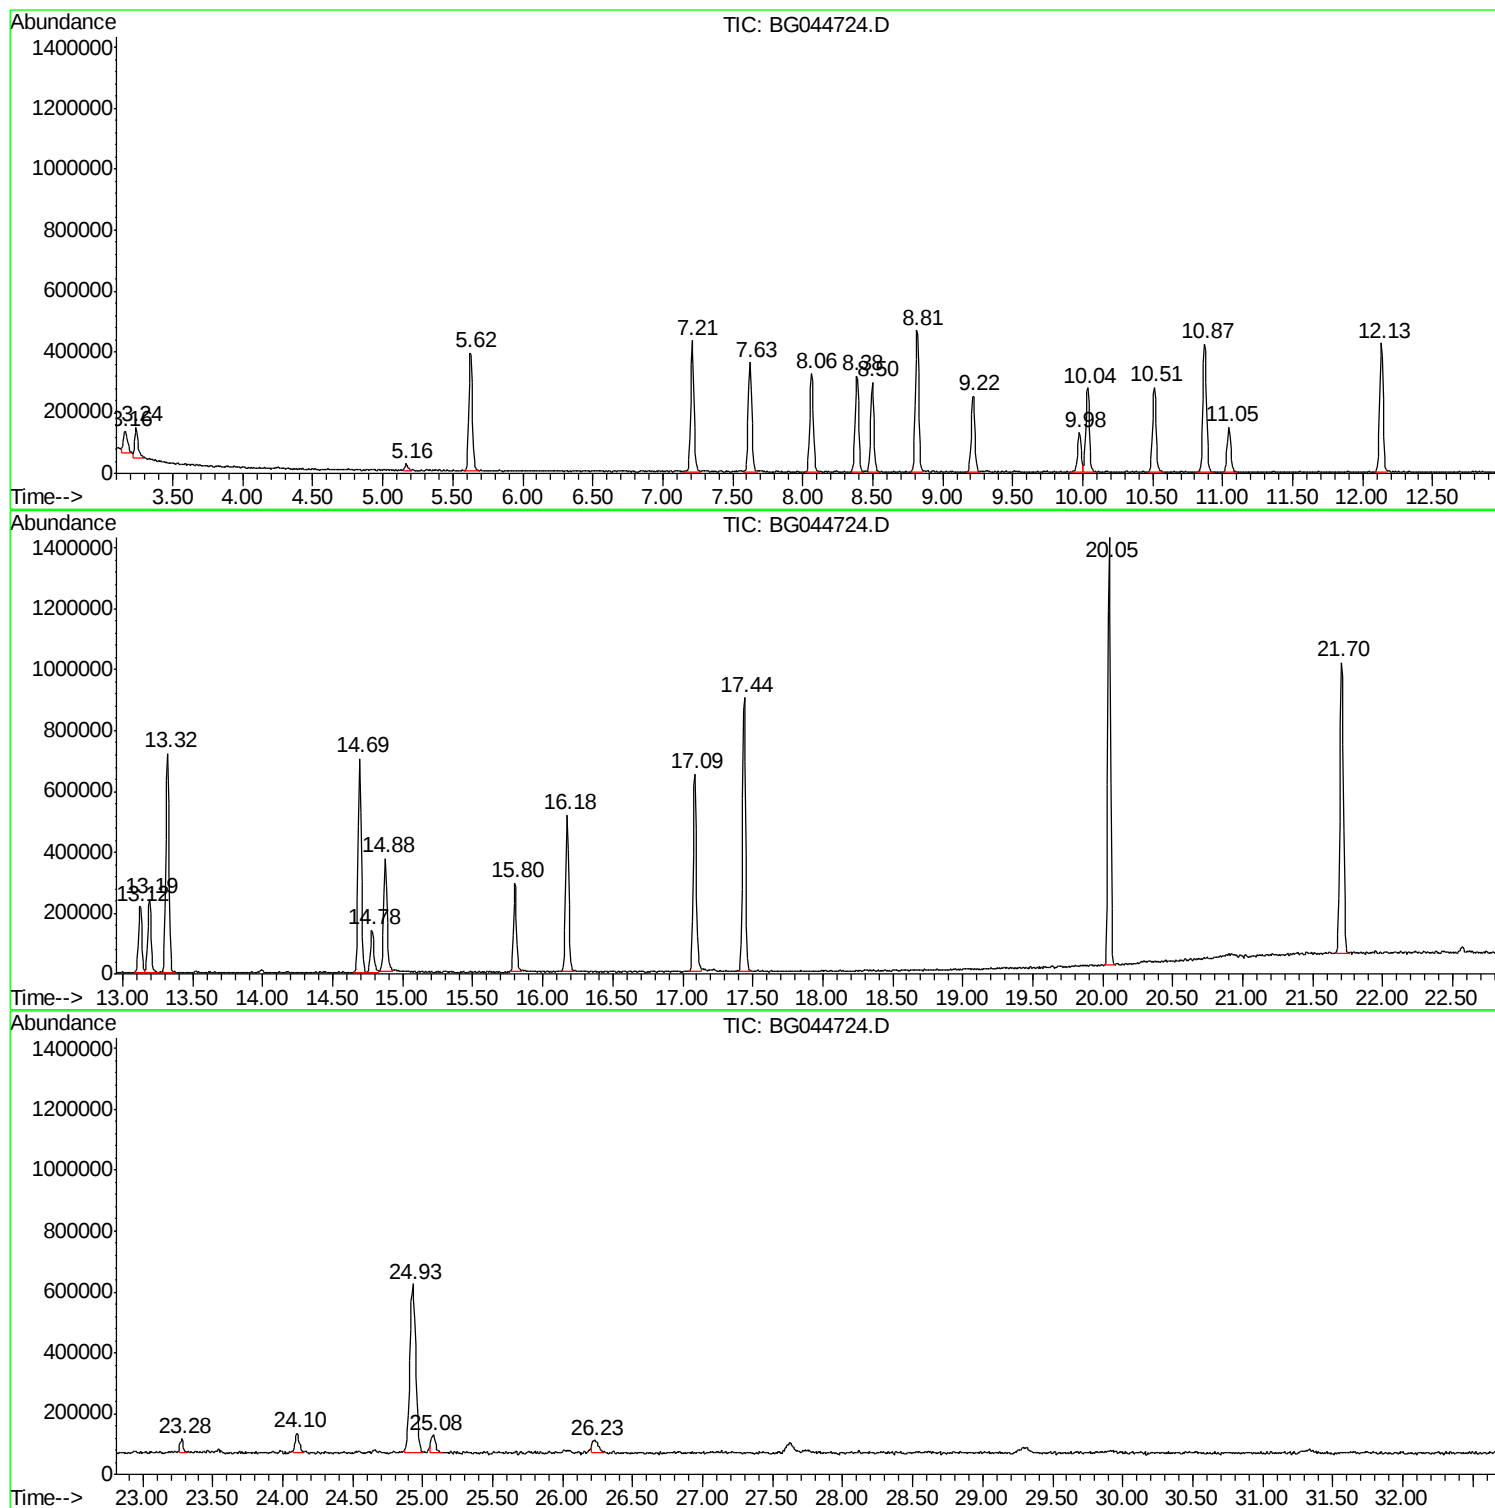

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG031120\
Data_File : BG044724.D
Acq_On : 11-Mar-2020 17:522
Operator : CG/JUU
Sample : L1798-06DL_5XX
Misc :
ALS_Vial : 8 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
PT-ACIDS-WPDL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031020.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
