
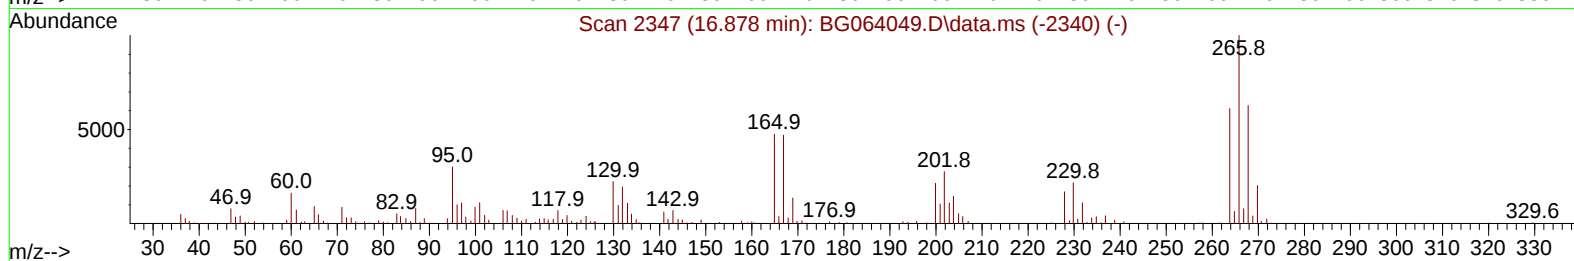
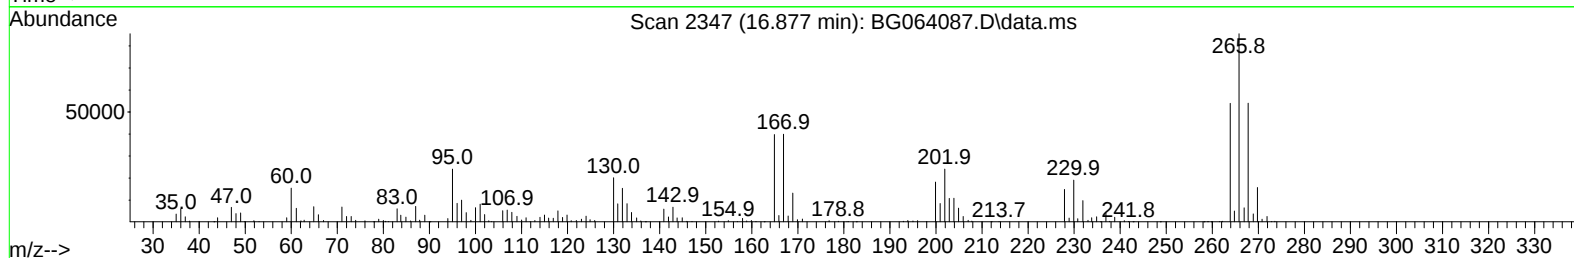


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031125\
Data File : BG064087.D
Acq On : 11 Mar 2025 7:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 11 10:54:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 05 15:39:19 2025
Response via : Initial Calibration

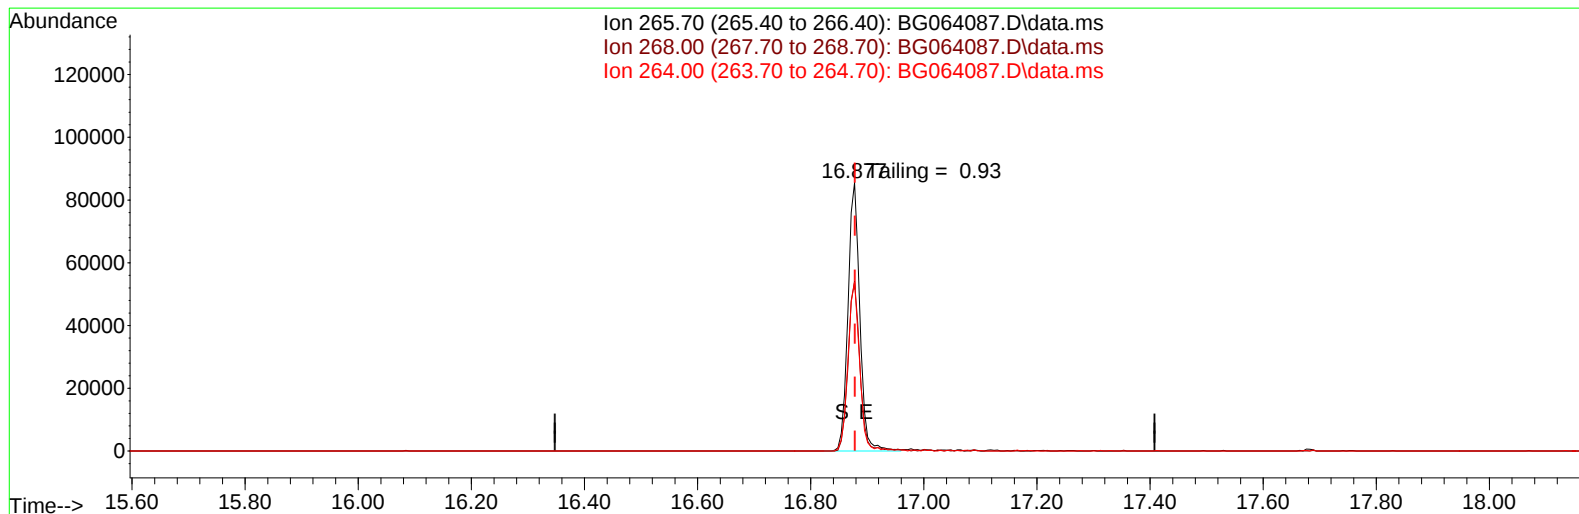

TIC: BG064087.D\data.ms

(70) Pentachlorophenol (C)




16.877min (-0.001) 19891.78 ng

response 124621

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	63.13
264.00	61.10	63.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031125\
Data File : BG064087.D
Acq On : 11 Mar 2025 7:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 11 10:54:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 05 15:39:19 2025
Response via : Initial Calibration

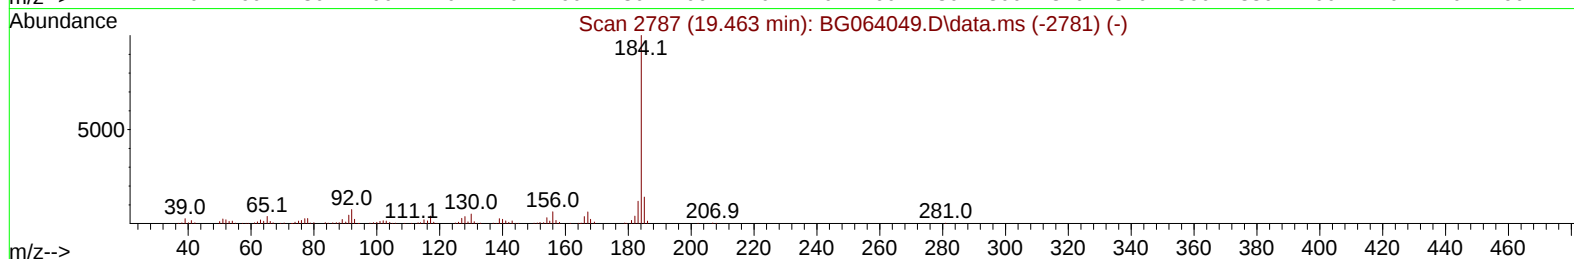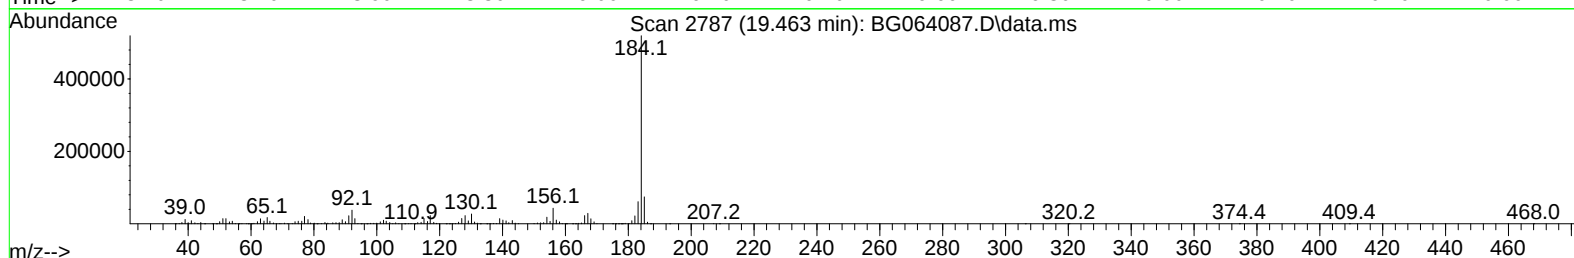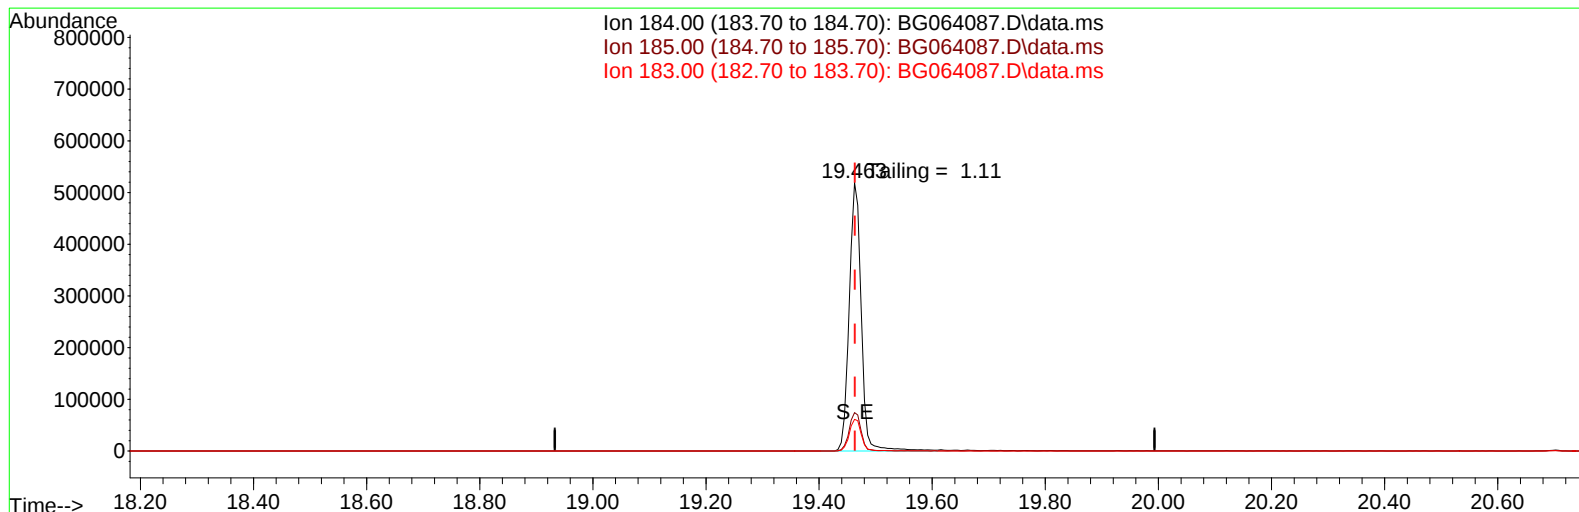

TIC: BG064087.D\data.ms

(77) Benzidine**19.463min (-0.000) 1010322.83 ng m****response 769455**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.30
183.00	11.90	11.82
0.00	0.00	0.00