
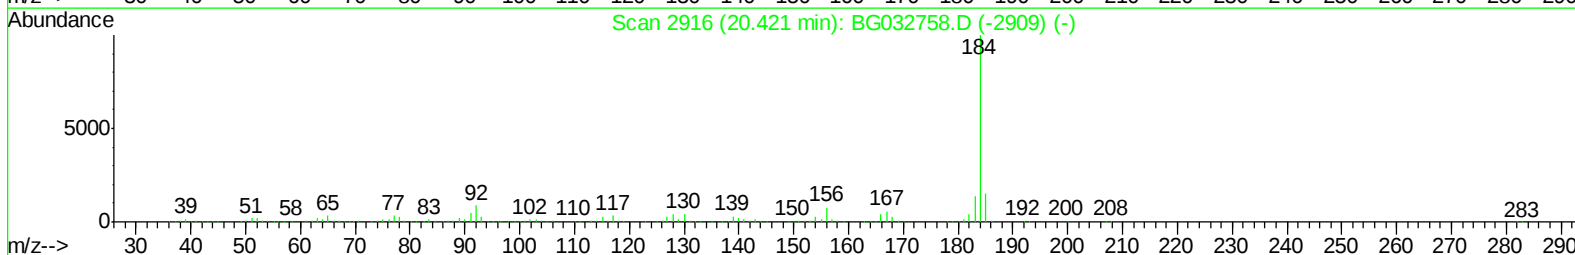
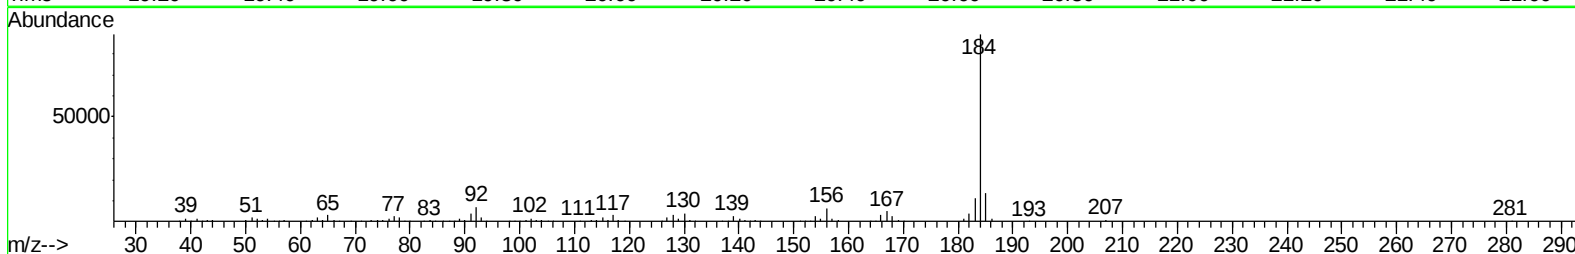


Data Path : Z:\HPCHEM1\BNA G\Data\BG031218\
Data File : BG033101.D
Acq On : 12 Mar 2018 23:06
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 13 03:47:28 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 09 15:10:14 2018
Response via : Initial Calibration

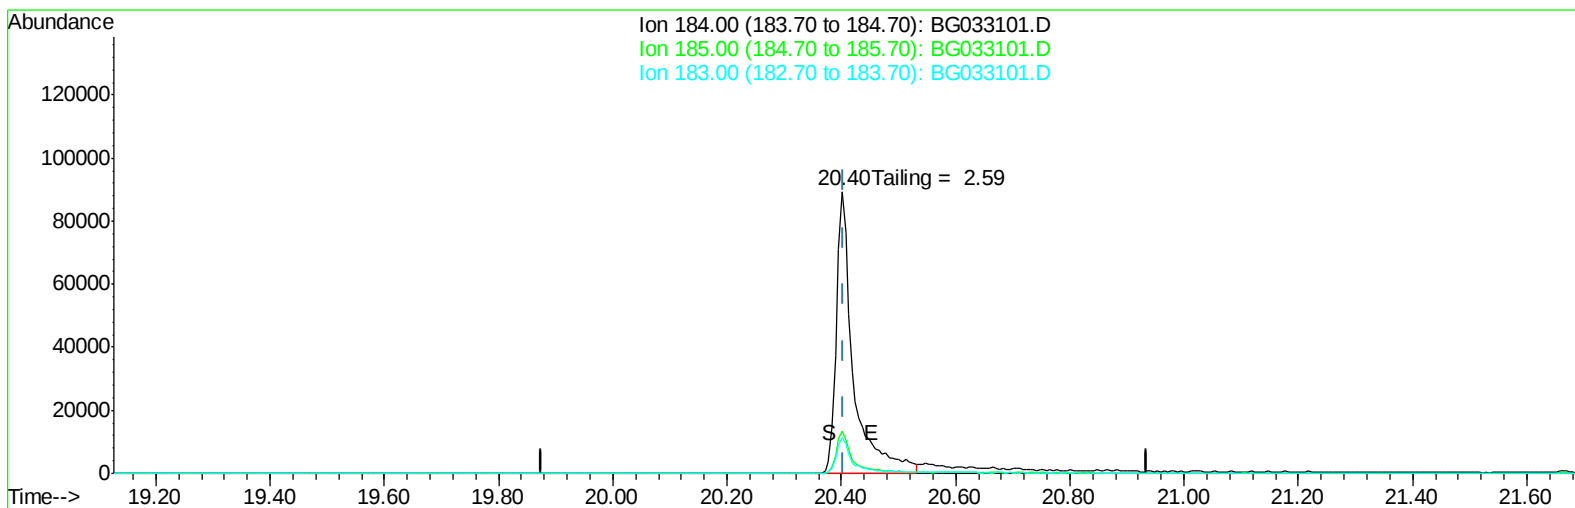

TIC: BG033101.D

(76) Benzidine

20.401min (-0.004) 0.00ng

response 185392

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.96
183.00	13.30	12.78
0.00	0.00	0.00