

Data Path : Z:\HPCHEM1\BNA G\DATA\BG031218\
 Data File : BG033089.D
 Acq On : 12 Mar 2018 14:54
 Operator : SJ/JU
 Sample : J1868-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 030818-TIDO-F-U-B

Quant Time: Mar 12 16:32:07 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 09 15:10:14 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.91	152	39511	20.00	ng	0.00
21) Naphthalene-d8	11.79	136	178502	20.00	ng	0.00
38) Acenaphthene-d10	15.52	164	101322	20.00	ng	0.00
63) Phenanthrene-d10	18.25	188	238885	20.00	ng	0.00
75) Chrysene-d12	22.60	240	232810	20.00	ng	0.00
86) Perylene-d12	26.39	264	230236	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	6.33	112	115576	46.80	ng	0.00
7) Phenol-d6	8.00	99	98098	28.50	ng	0.00
23) Nitrobenzene-d5	10.11	82	335540	125.15	ng	0.00
41) 2,4,6-Tribromophenol	16.99	330	128756	120.86	ng	0.00
44) 2-Fluorobiphenyl	14.15	172	734647	104.57	ng	0.00
78) Terphenyl-d14	20.77	244	1090311	105.22	ng	0.00
Target Compounds						
49) Dimethylphthalate	14.94	163	19897	2.313	ng	Qvalue 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG031218\
Data File : BG033089.D
Acq On : 12 Mar 2018 14:54
Operator : SJ/JU
Sample : J1868-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
030818-TIDO-F-U-B

Quant Time: Mar 12 16:32:07 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 09 15:10:14 2018
Response via : Initial Calibration

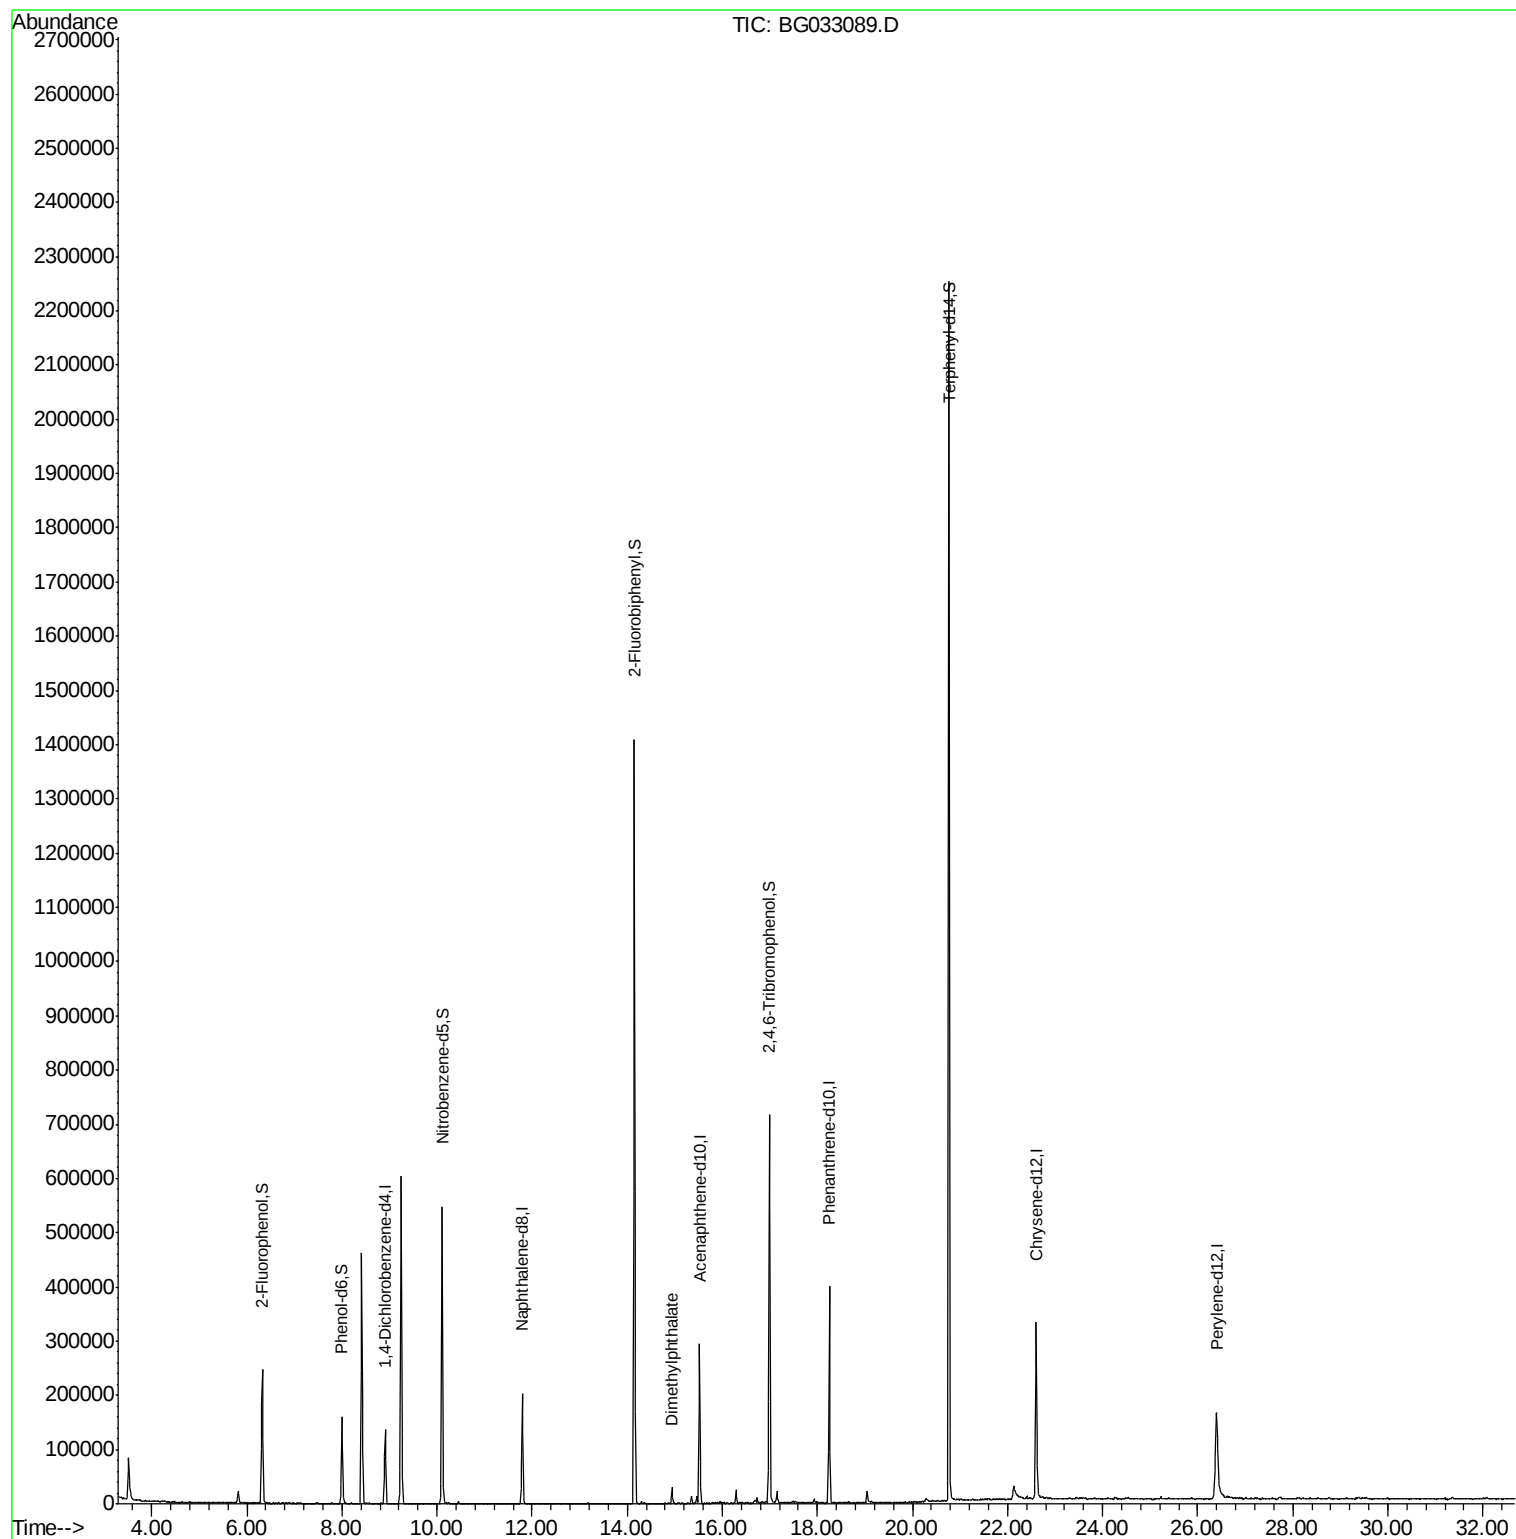




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.91 min Scan# 957
Delta R.T. 0.00 min
Lab File: BG033089.D
Acq: 12 Mar 2018 14:54

Instrument :
BNA_G
ClientSampleId :
030818-TIDO-F-U-B

Tot Ion:152 Resp: 39511
Ion Ratio Lower Upper
152 100
150 147.9 126.6 189.8
115 60.1 53.0 79.4

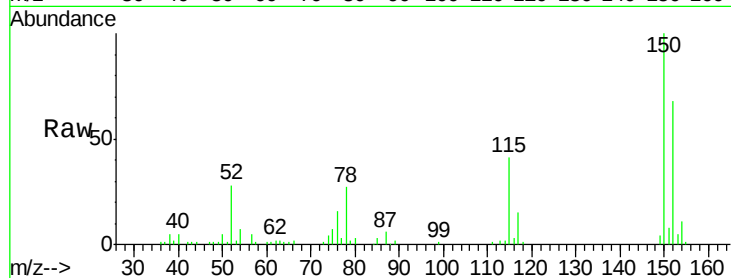


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

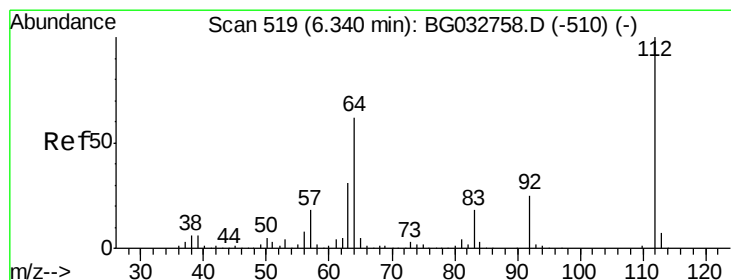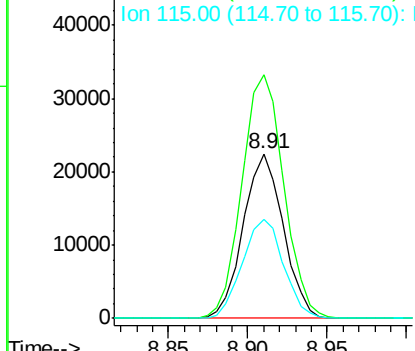



#5

2-Fluorophenol
Concen: 46.798 ng
RT: 6.33 min Scan# 517
Delta R.T. 0.00 min
Lab File: BG033089.D
Acq: 12 Mar 2018 14:54

Tgt Ion:112 Resp: 115576
Ion Ratio Lower Upper
112 100
64 68.9 56.3 84.5
63 35.8 30.1 45.1

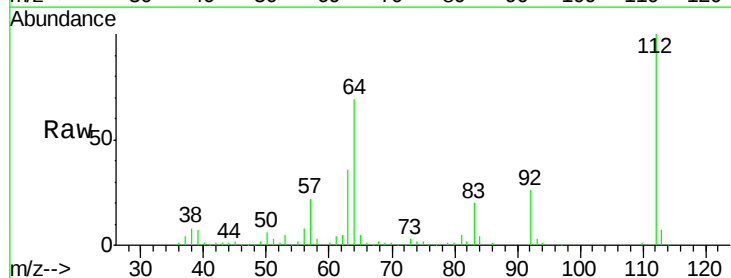

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

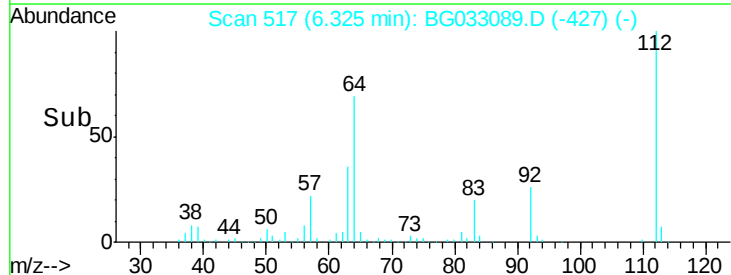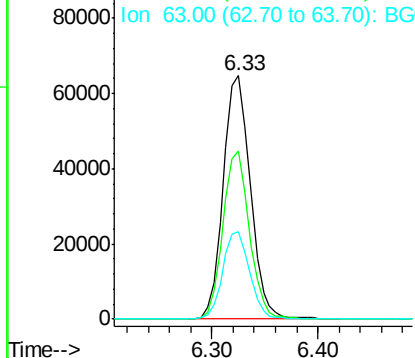



#7

Phenol-d6

Concen: 28.497 ng

RT: 8.00 min Scan# 802

Delta R.T. -0.01 min

Lab File: BG033089.D

Acq: 12 Mar 2018 14:54

Instrument :

BNA_G

ClientSampleId :

030818-TIDO-F-U-B


Tot Ion: 99 Resp: 98098

Ion Ratio Lower Upper



99 100

42 21.0 14.1 21.1

71 34.5 26.1 39.1

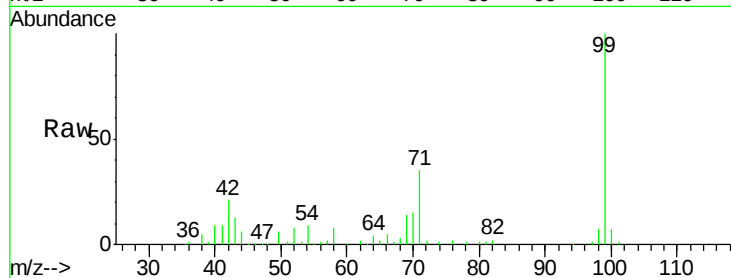

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

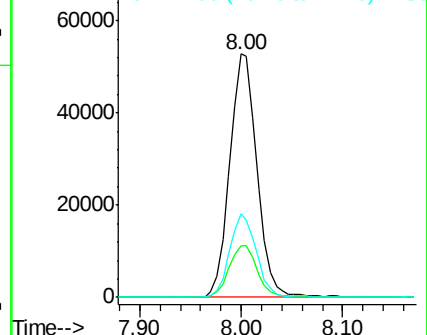

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.79 min Scan# 1448

Delta R.T. -0.01 min

Lab File: BG033089.D

Acq: 12 Mar 2018 14:54

Tgt Ion: 136 Resp: 178502


Ion Ratio Lower Upper

136 100



137 11.5 9.2 13.8

54 10.2 10.3 15.5#

68 6.4 4.5 6.7

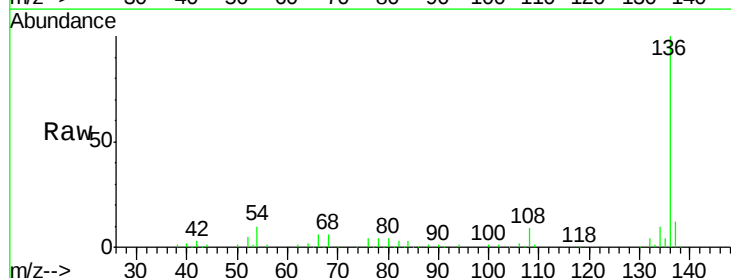

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



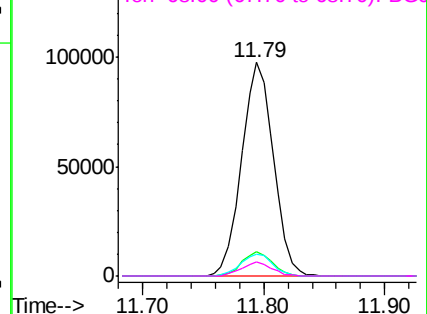




#23
 Nitrobenzene-d5
 Concen: 125.146 ng
 RT: 10.11 min Scan# 1161
 Delta R.T. -0.01 min
 Lab File: BG033089.D
 Acq: 12 Mar 2018 14:54




Instrument :
 BNA_G
 ClientSampleId :
 030818-TIDO-F-U-B


Tot Ion	82	Resp	33540
Ion Ratio	Lower	Upper	
82	100		
128	44.5	29.7	44.5#
54	60.8	43.1	64.7

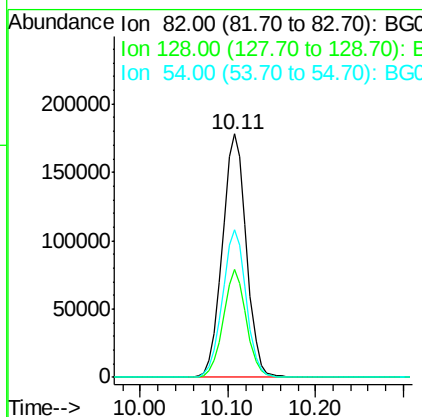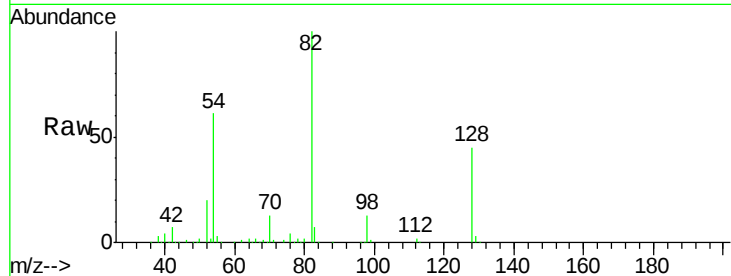

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 15.52 min Scan# 2083
 Delta R.T. -0.01 min
 Lab File: BG033089.D
 Acq: 12 Mar 2018 14:54

Tgt Ion	164	Resp	101322
Ion Ratio	Lower	Upper	
164	100		
162	103.3	78.8	118.2
160	47.0	35.4	53.0

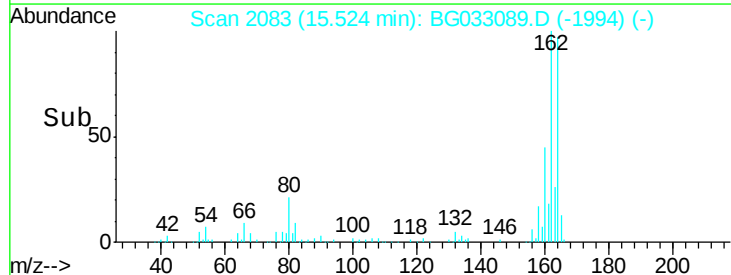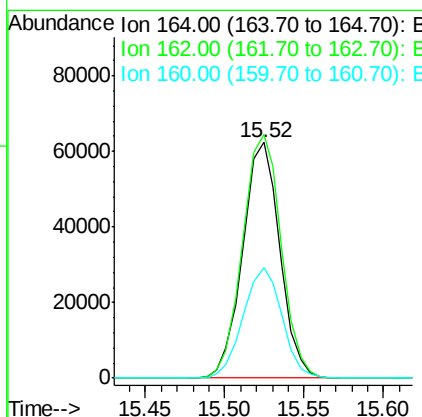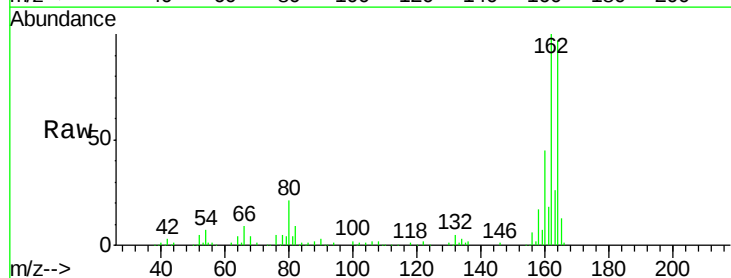


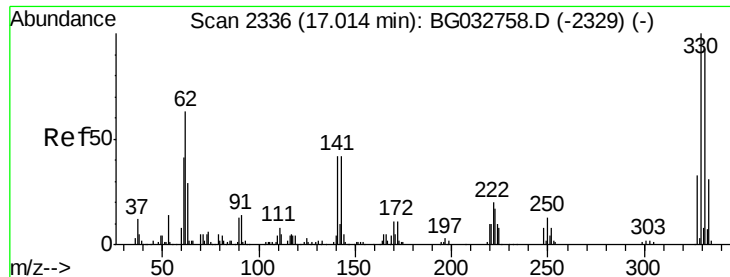




#41
 2,4,6-Tribromophenol
 Concen: 120.856 ng
 RT: 16.99 min Scan# 2333
 Delta R.T. -0.01 min
 Lab File: BG033089.D
 Acq: 12 Mar 2018 14:54

Instrument :
 BNA_G
 ClientSampleId :
 030818-TIDO-F-U-B

Tot Ion:330 Resp: 128756
 Ion Ratio Lower Upper
 330 100
 332 96.0 77.0 115.6
 141 41.5 25.2 37.8#

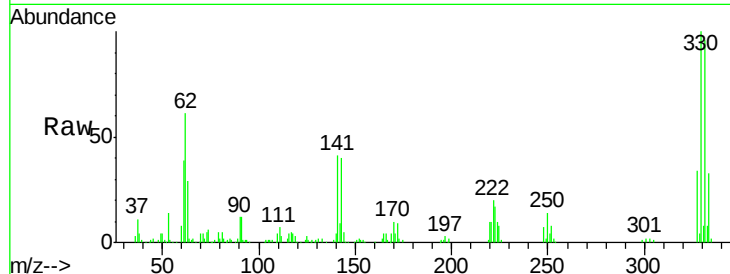


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

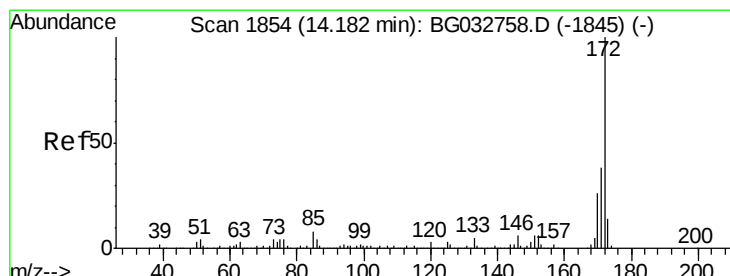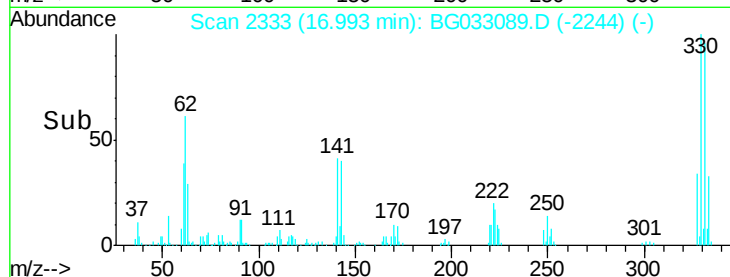
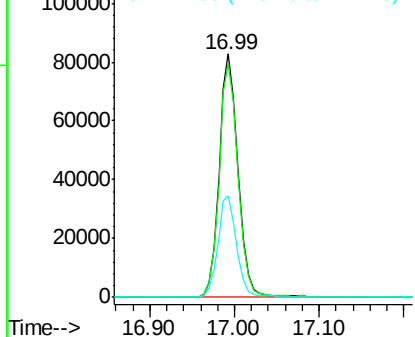



#44
 2-Fluorobiphenyl
 Concen: 104.572 ng
 RT: 14.15 min Scan# 1849
 Delta R.T. -0.01 min
 Lab File: BG033089.D
 Acq: 12 Mar 2018 14:54

Tgt Ion:172 Resp: 734647
 Ion Ratio Lower Upper
 172 100
 171 37.6 30.0 45.0
 170 24.6 19.5 29.3

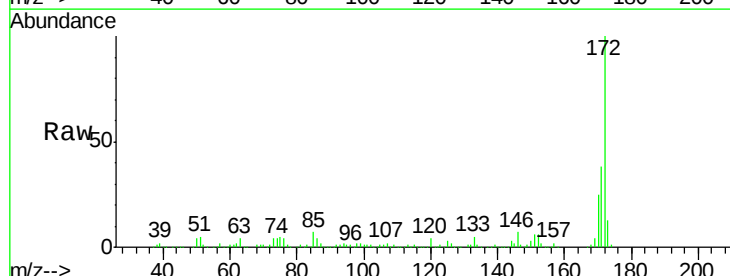

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

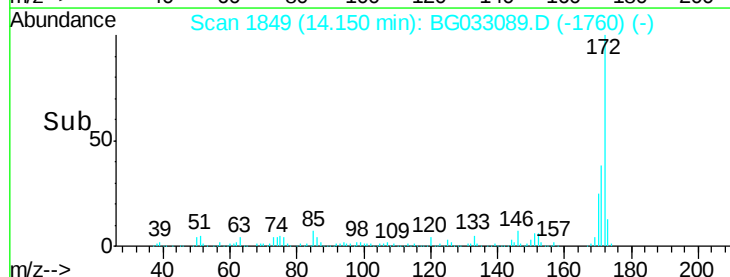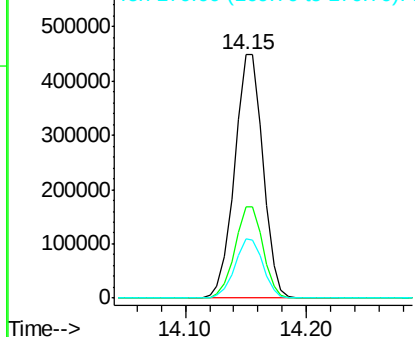



#49

Dimethylphthalate

Concen: 2.313 ng

RT: 14.94 min Scan# 1984

Delta R.T. -0.01 min

Lab File: BG033089.D

Acq: 12 Mar 2018 14:54

Instrument :

BNA_G

ClientSampleId :

030818-TIDO-F-U-B


Tot Ion:163 Resp: 19897

Ion Ratio Lower Upper

163 100

194 4.7 3.4 5.2




164 11.5 8.2 12.4

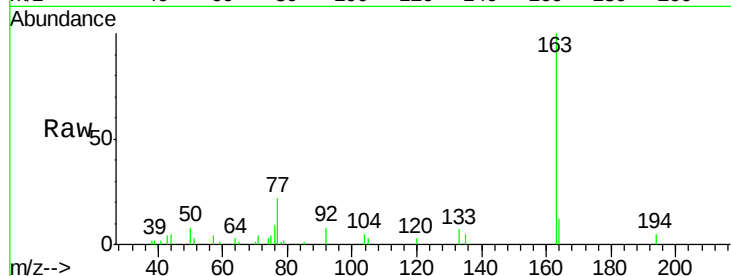

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

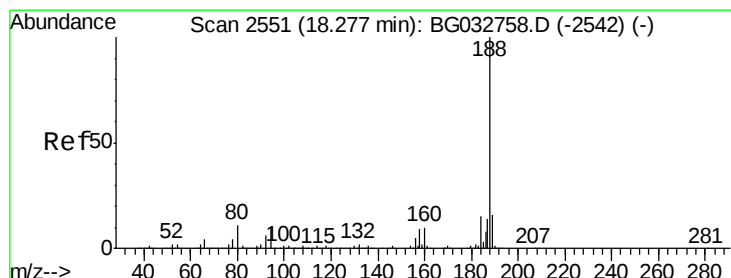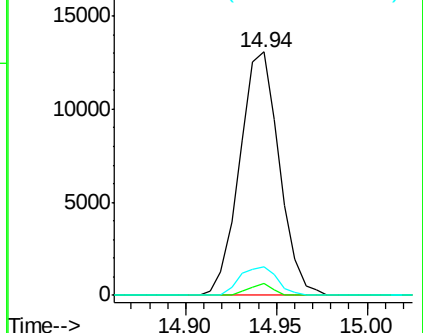

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 18.25 min Scan# 2547

Delta R.T. -0.01 min

Lab File: BG033089.D

Acq: 12 Mar 2018 14:54


Tgt Ion:188 Resp: 238885

Ion Ratio Lower Upper

188 100

94 10.5 6.9 10.3#



80 10.8 7.7 11.5

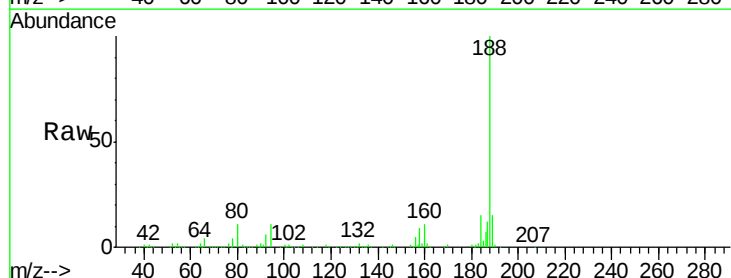


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

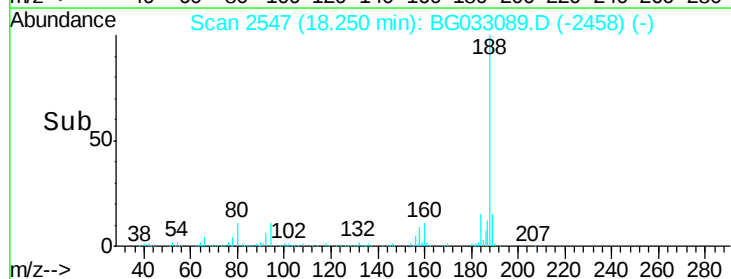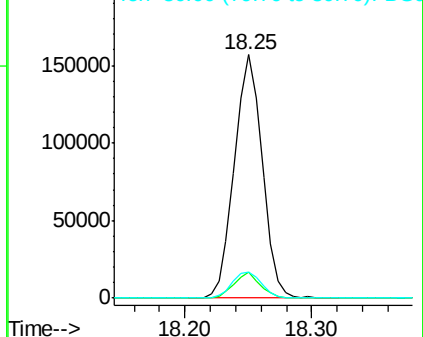



#75

Chrysene-d12

Concen: 20.000 ng

RT: 22.60 min Scan# 3288

Delta R.T. -0.01 min

Lab File: BG033089.D

Acq: 12 Mar 2018 14:54

Instrument :

BNA_G

ClientSampleId :

030818-TIDO-F-U-B


Tot Ion:240 Resp: 232810

Ion Ratio Lower Upper

240 100

120 11.4 6.8 10.2#




236 26.4 20.9 31.3

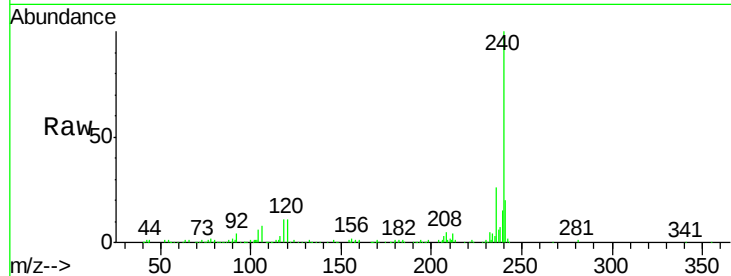

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

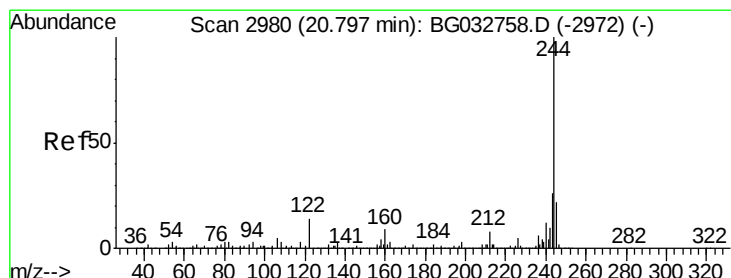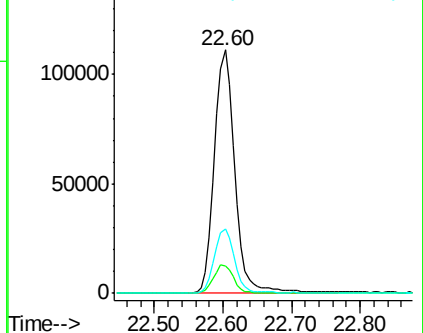

#78

Terphenyl-d14

Concen: 105.220 ng

RT: 20.77 min Scan# 2976

Delta R.T. 0.00 min

Lab File: BG033089.D

Acq: 12 Mar 2018 14:54


Tgt Ion:244 Resp: 1090311

Ion Ratio Lower Upper

244 100

212 8.1 5.8 8.8



122 12.1 7.0 10.4#



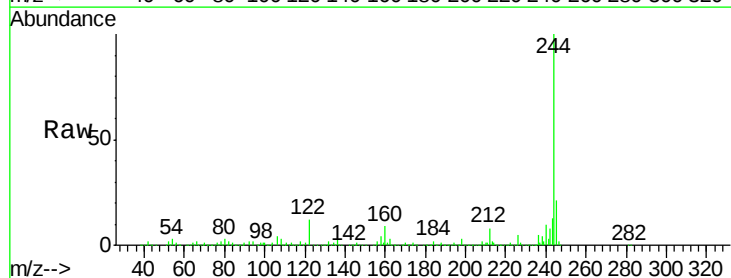


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

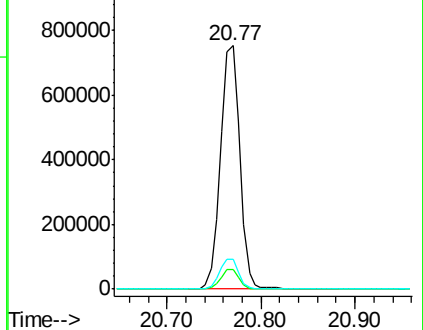

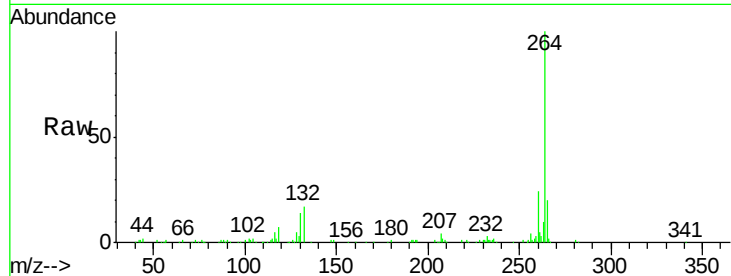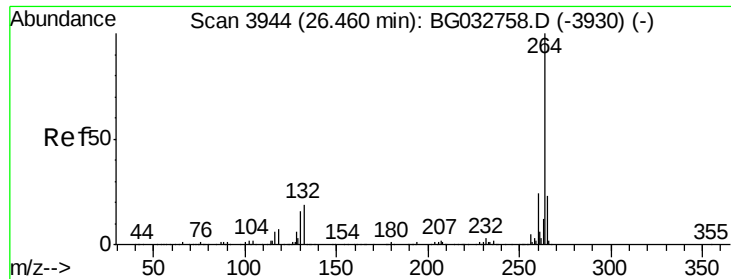

#86

Pervlene-d12

Concen: 20.000 ng

RT: 26.39 min Scan# 3933

Delta R.T. -0.02 min

Lab File: BG033089.D

Acq: 12 Mar 2018 14:54

Instrument :

BNA_G

ClientSampleId :

030818-TIDO-F-U-B

Tot Ion:264 Resp: 230236

Ion Ratio Lower Upper

264 100

260 23.9 17.4 26.0

265 20.1 17.7 26.5

