

Data Path : Z:\HPCHEM1\BNA G\DATA\BG031218\
 Data File : BG033091.D
 Acq On : 12 Mar 2018 16:10
 Operator : SJ/JU
 Sample : J1869-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 030618-JETT-E-D-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.517	32	39	52	rVB	78083	164626	5.26%	1.209%
2	6.319	510	516	525	rBV	227013	403051	12.88%	2.960%
3	7.999	796	802	813	rBV	142098	271793	8.69%	1.996%
4	8.416	865	873	885	rBV	440818	811741	25.95%	5.962%
5	8.909	950	957	965	rBV	141652	258922	8.28%	1.902%
6	9.244	1007	1014	1023	rBV	564425	1066918	34.11%	7.836%
7	10.108	1152	1161	1170	rBV	518506	982586	31.41%	7.216%
8	11.794	1440	1448	1459	rBV	209352	393136	12.57%	2.887%
9	14.155	1841	1850	1859	rBV	1334260	2199002	70.30%	16.150%
10	14.942	1977	1984	1989	rBV	31412	47198	1.51%	0.347%
11	15.524	2077	2083	2093	rVB2	328292	539505	17.25%	3.962%
12	16.287	2208	2213	2219	rVB2	33968	44229	1.41%	0.325%
13	16.992	2326	2333	2344	rBV	674060	1099094	35.14%	8.072%
14	17.145	2354	2359	2368	rVB	31644	51645	1.65%	0.379%
15	18.250	2540	2547	2554	rBV2	426123	665257	21.27%	4.886%
16	19.048	2677	2683	2688	rBV3	25792	42342	1.35%	0.311%
17	20.770	2969	2976	2989	rBV	2271395	3128188	100.00%	22.974%
18	22.133	3201	3208	3220	rBV4	28442	94391	3.02%	0.693%
19	22.602	3281	3288	3299	rBV2	352276	703042	22.47%	5.163%
20	26.397	3921	3934	3950	rBV2	173629	649285	20.76%	4.769%


Sum of corrected areas: 13615951

Data Path : Z:\HPCHEM1\BNA G\DATA\BG031218\
Data File : BG033091.D
Acq On : 12 Mar 2018 16:10
Operator : SJ/JU
Sample : J1869-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
030618-JETT-E-D-B

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

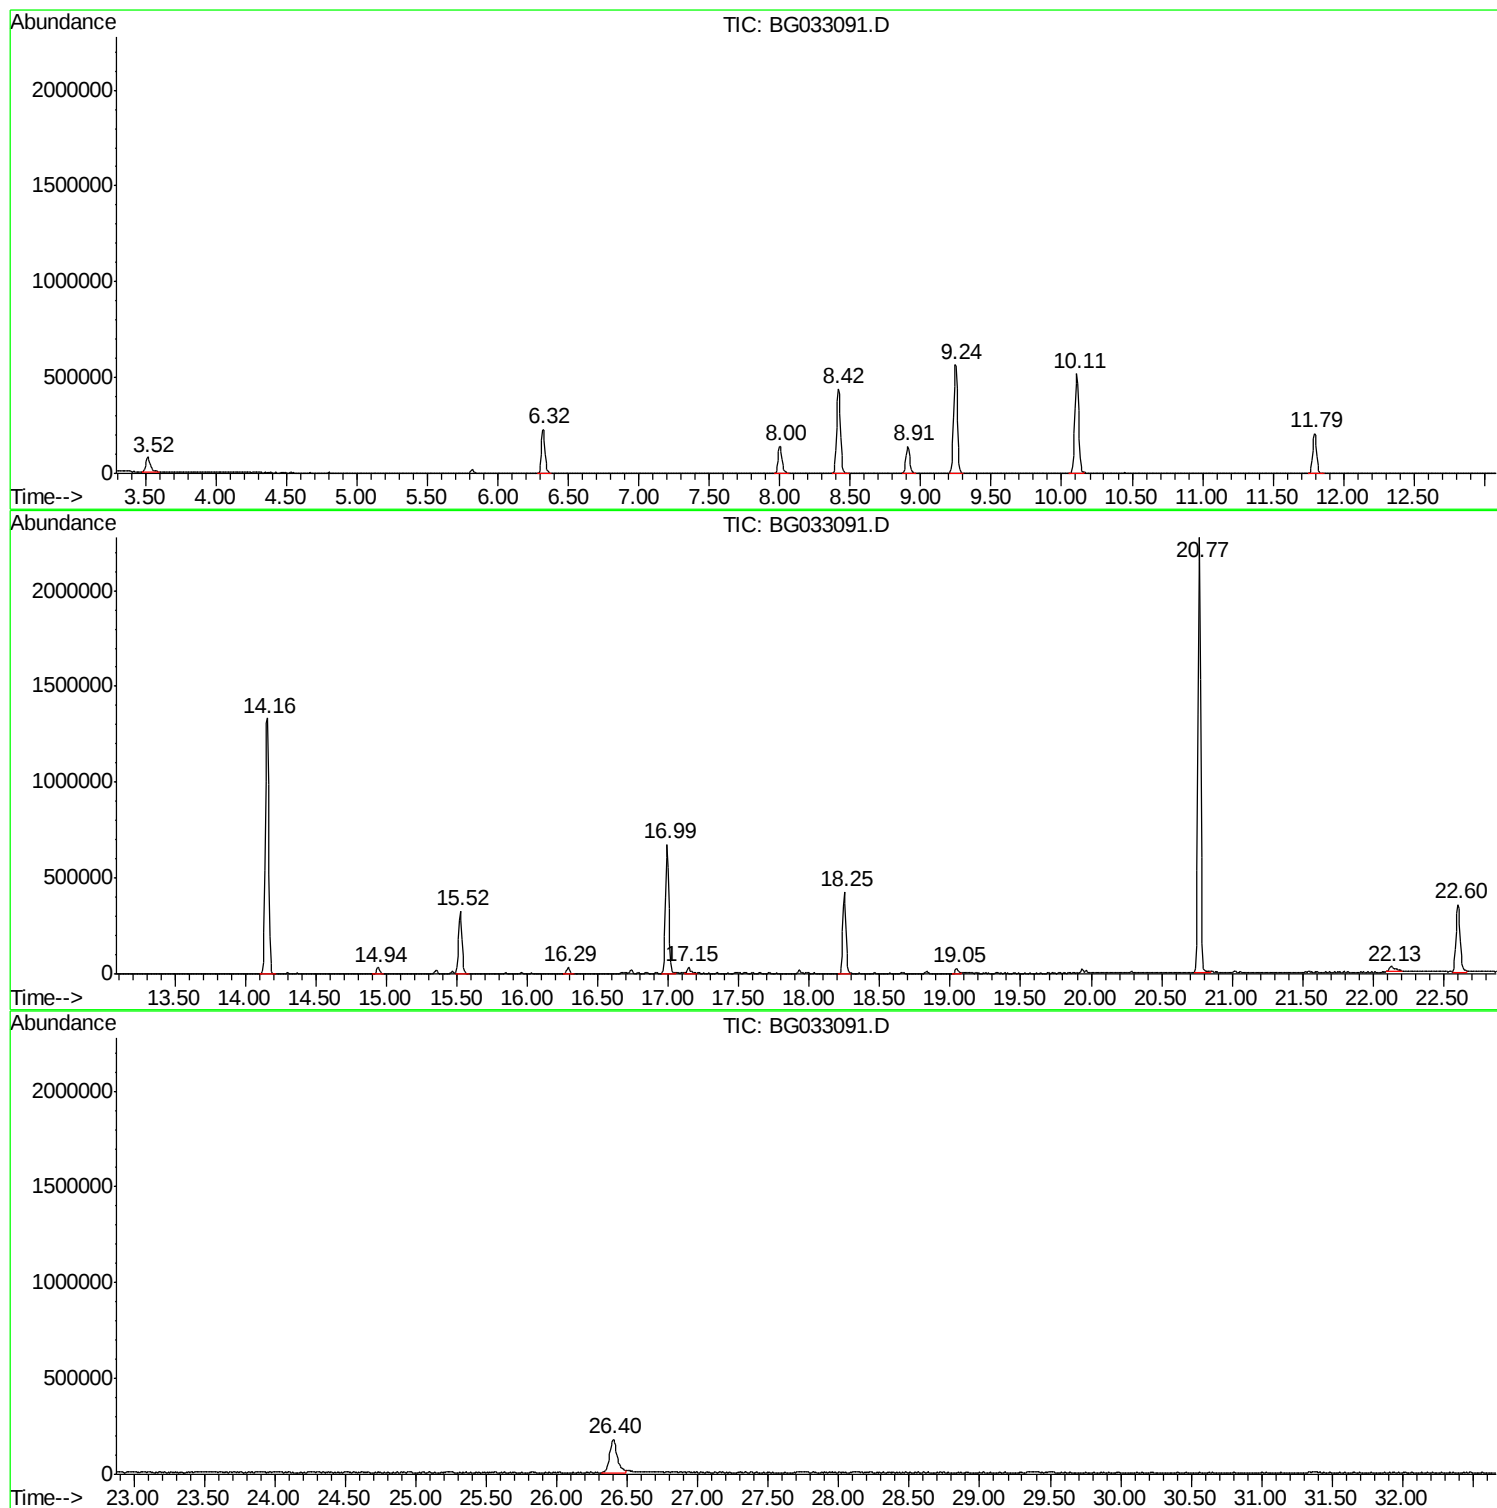

Data Path : Z:\HPCHEM1\BNA G\DATA\BG031218\
Data File : BG033091.D
Acq On : 12 Mar 2018 16:10
Operator : SJ/JU
Sample : J1869-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
030618-JETT-E-D-B










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown8.42 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.42	62.70 ng	811741	1,4-Dichlorobenzene-d4	8.91

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
3		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
4		Benzene, 1-ethenyl-3,5-dimethyl-	132	C10H12	005379-20-4	9
5		Xenon	132	Xe	007440-63-3	9

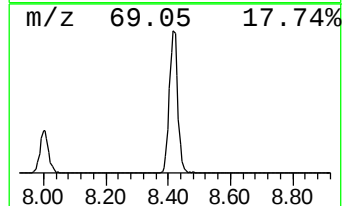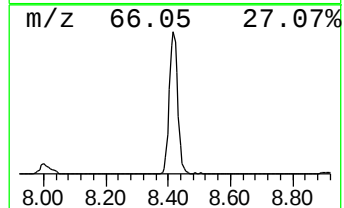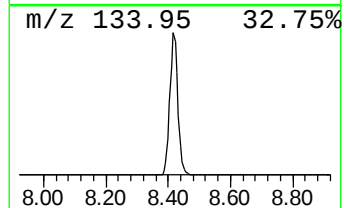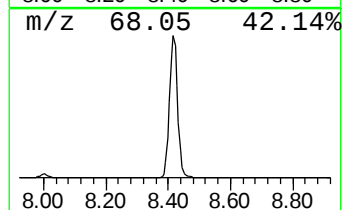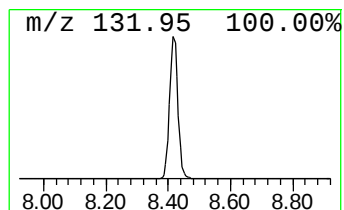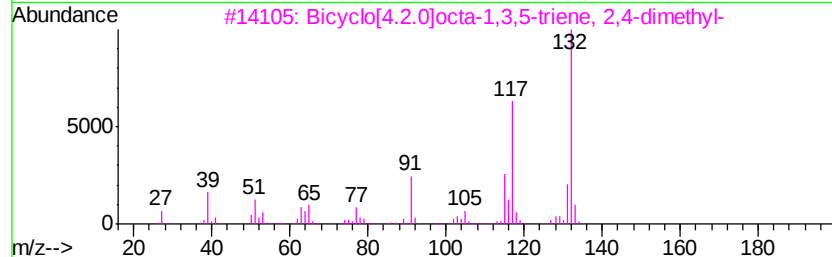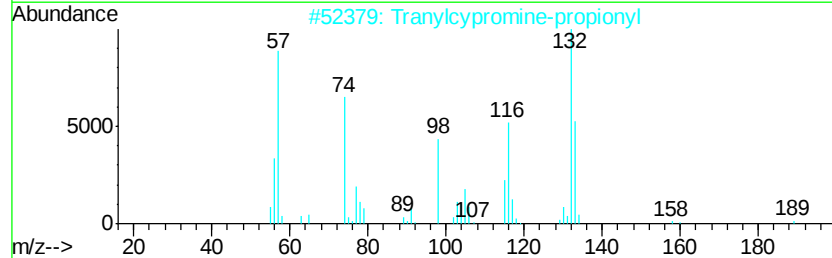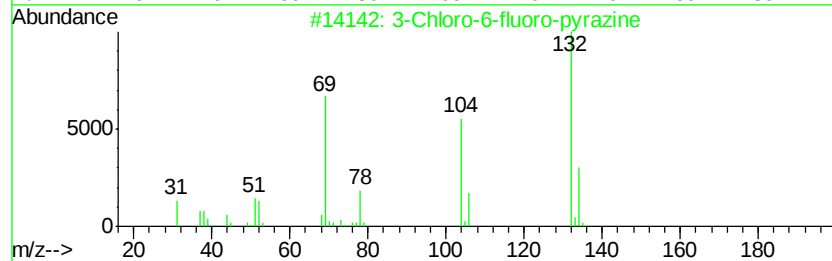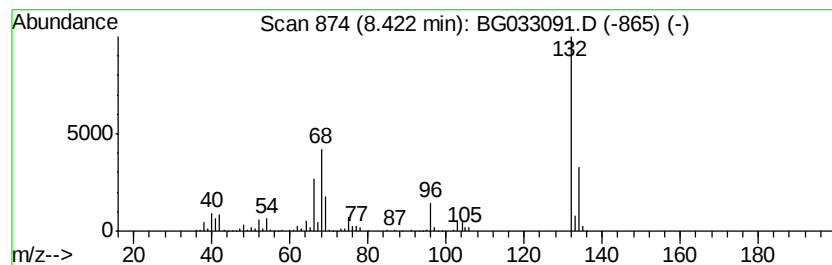

Data Path : Z:\HPCHEM1\BNA G\DATA\BG031218\
Data File : BG033091.D
Acq On : 12 Mar 2018 16:10
Operator : SJ/JU
Sample : J1869-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
030618-JETT-E-D-B










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 Cyclotetracosane Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
22.13	2.69 ng	94391	Chrysene-d12	22.60

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclotetracosane	336	C24H48	000297-03-0	90
2			10-Heneicosene (c,t)	294	C21H42	095008-11-0	87
3			Pentafluoropropionic acid, hexadecyl ester	388	C19H33F5O2	006222-07-7	87
4			Heptafluorobutyric acid, hexadecyl ester	438	C20H33F7O2	006385-15-5	87
5			Pentafluoropropionic acid, heptadecyl ester	402	C20H35F5O2	959218-78-1	81

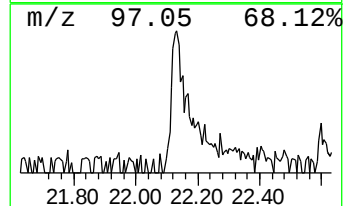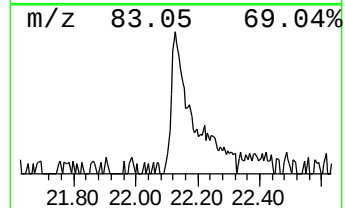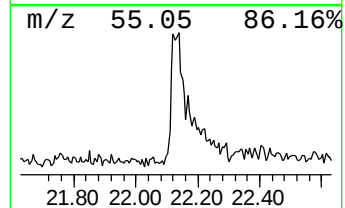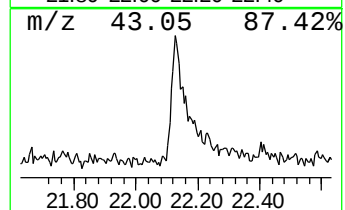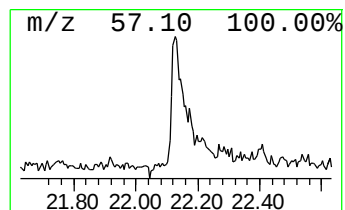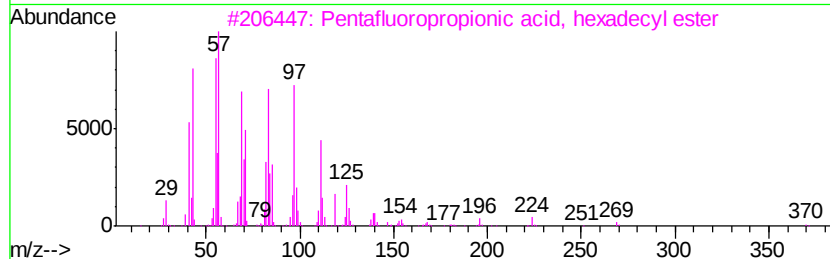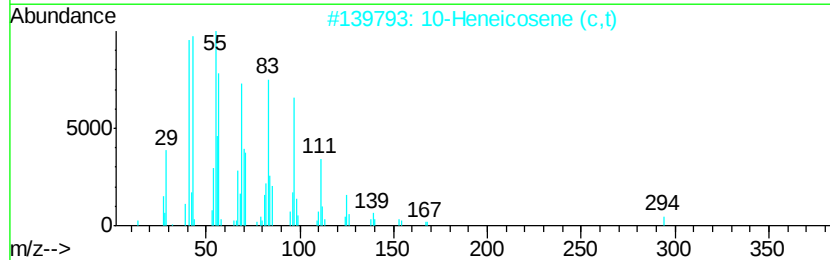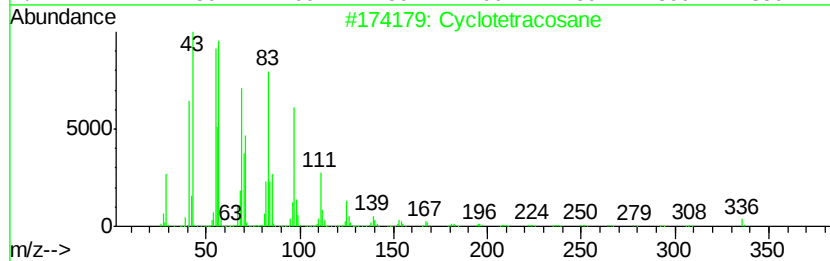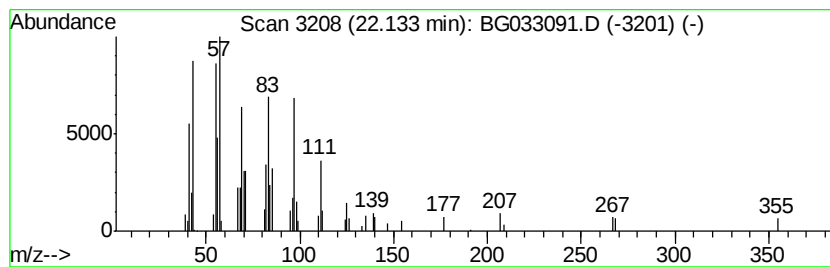

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG031218\
Data File : BG033091.D
Acq On : 12 Mar 2018 16:10
Operator : SJ/JU
Sample : J1869-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
030618-JETT-E-D-B

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown8.42	8.42	62.7	ng	811741	1	8.91	258922	20.0
Cyclotetracosane	22.13	2.7	ng	94391	5	22.60	703042	20.0