

Data Path : Z:\HPCHEM1\BNA G\DATA\BG031218\
 Data File : BG033092.D
 Acq On : 12 Mar 2018 16:47
 Operator : SJ/JU
 Sample : J1869-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 030618-JETT-E-D-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.513	32	38	52	rVB	78680	175600	5.20%	1.237%
2	6.321	507	516	528	rVB	250304	438565	12.99%	3.090%
3	8.001	795	802	814	rBV	160901	319756	9.47%	2.253%
4	8.418	864	873	886	rBV	484859	883305	26.17%	6.223%
5	8.912	948	957	966	rVB	144803	262724	7.78%	1.851%
6	9.246	1006	1014	1024	rVB	638893	1164167	34.49%	8.202%
7	10.110	1152	1161	1168	rBV	562395	1056497	31.30%	7.443%
8	11.796	1437	1448	1457	rBV	209269	393583	11.66%	2.773%
9	14.152	1841	1849	1862	rBV	1467030	2352831	69.70%	16.576%
10	14.939	1978	1983	1989	rBV	47196	68462	2.03%	0.482%
11	15.526	2076	2083	2090	rVB2	319767	534360	15.83%	3.765%
12	16.290	2208	2213	2218	rVB2	32569	43098	1.28%	0.304%
13	16.989	2325	2332	2341	rBV	654394	1035662	30.68%	7.297%
14	17.142	2353	2358	2366	rBV2	30042	48738	1.44%	0.343%
15	18.252	2540	2547	2556	rBV2	411979	673613	19.95%	4.746%
16	20.766	2969	2975	2986	rBV	2549900	3375700	100.00%	23.783%
17	22.599	3280	3287	3299	rBV	363744	711552	21.08%	5.013%
18	26.400	3920	3934	3950	rBV2	166200	655651	19.42%	4.619%


Sum of corrected areas: 14193864

Data Path : Z:\HPCHEM1\BNA G\DATA\BG031218\
Data File : BG033092.D
Acq On : 12 Mar 2018 16:47
Operator : SJ/JU
Sample : J1869-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
030618-JETT-E-D-S

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

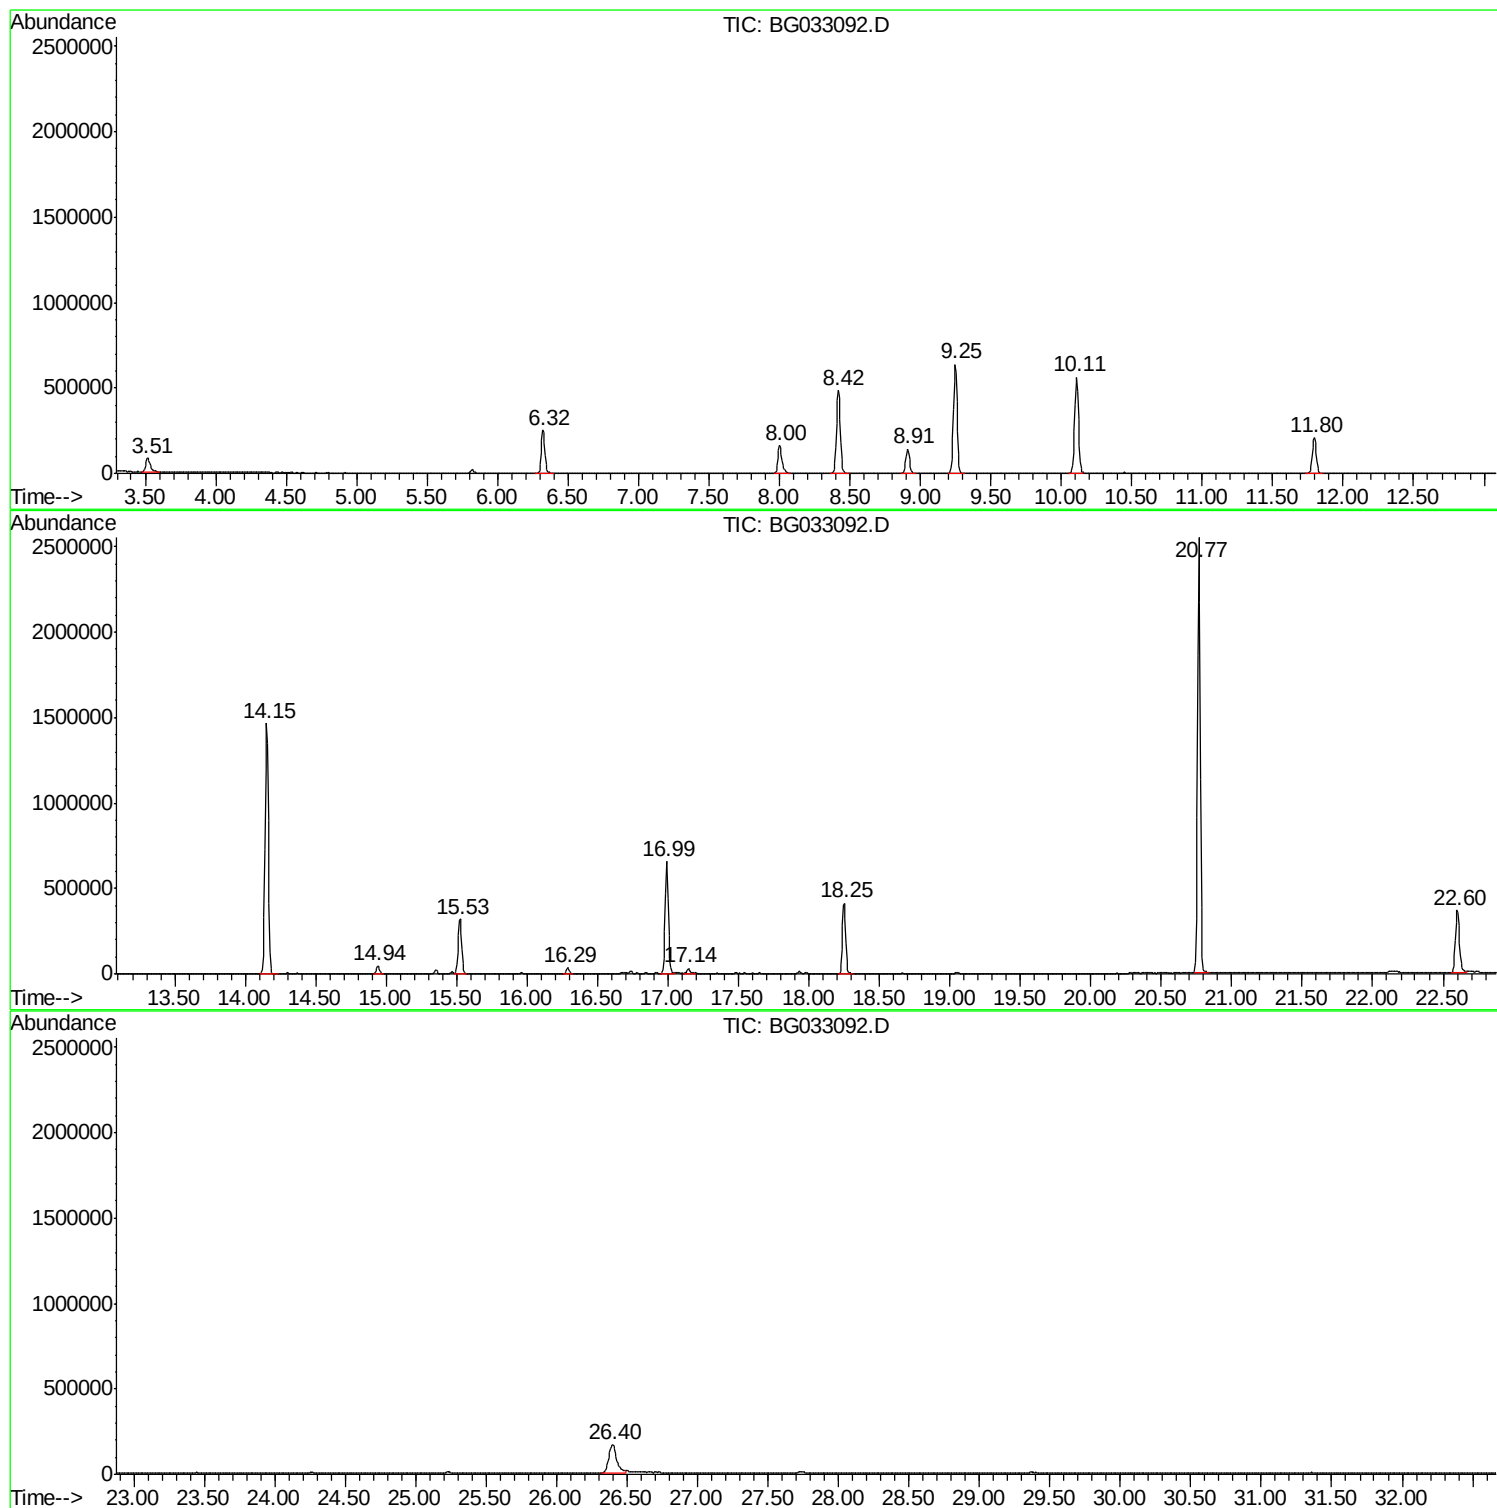

Data Path : Z:\HPCHEM1\BNA G\DATA\BG031218\
Data File : BG033092.D
Acq On : 12 Mar 2018 16:47
Operator : SJ/JU
Sample : J1869-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
030618-JETT-E-D-S










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown8.42 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.42	67.24 ng	883305	1,4-Dichlorobenzene-d4	8.91

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3		Tranvlcyproline-propionyl	189	C12H15NO	1000123-86-3	10
4		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9
5		Xenon	132	Xe	007440-63-3	9

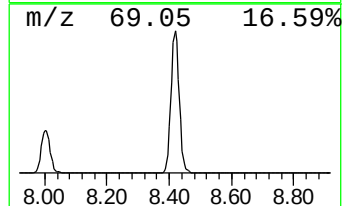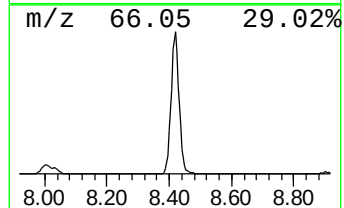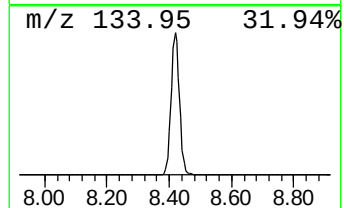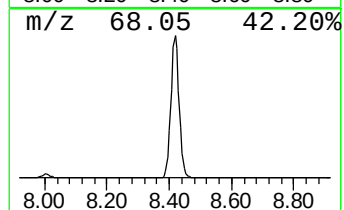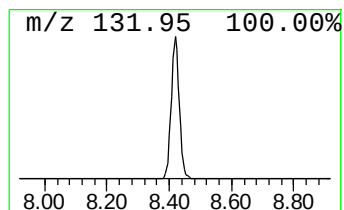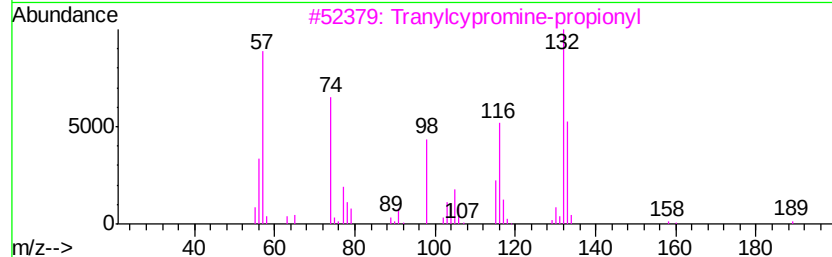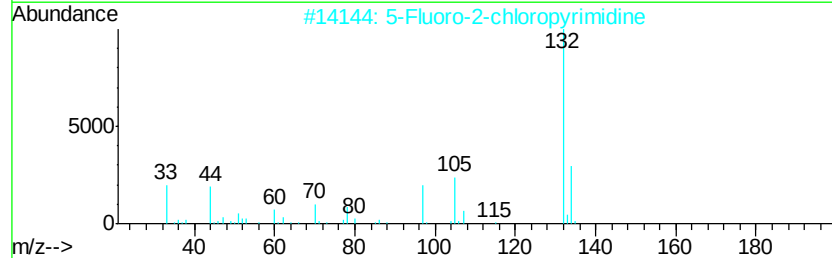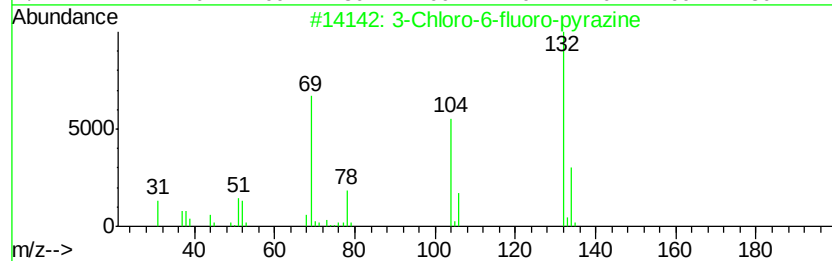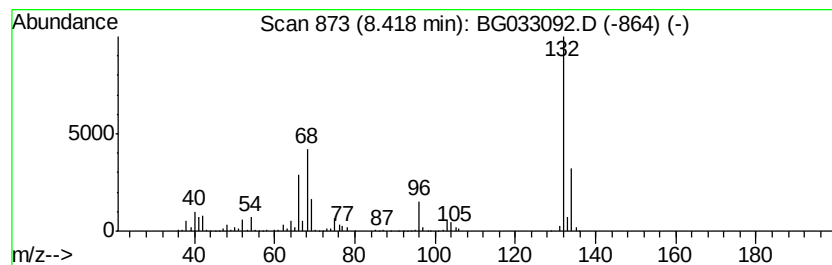

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG031218\
Data File : BG033092.D
Acq On : 12 Mar 2018 16:47
Operator : SJ/JU
Sample : J1869-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
030618-JETT-E-D-S

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown8.42	8.42	67.2	ng	883305	1	8.91	262724	20.0