

Data Path : Z:\HPCHEM1\BNA G\DATA\BG031218\
 Data File : BG033103.D
 Acq On : 13 Mar 2018 00:21
 Operator : SJ/JU
 Sample : J1867-10
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CPS073071

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.518	32	39	50	rBV	71118	157391	4.43%	0.996%
2	6.326	510	517	529	rBV	365791	653315	18.40%	4.136%
3	8.000	795	802	814	rBV	231738	436159	12.28%	2.761%
4	8.417	865	873	883	rBV	702494	1301306	36.65%	8.239%
5	8.910	949	957	968	rVB	136091	251353	7.08%	1.591%
6	9.245	1006	1014	1024	rBV	646540	1197362	33.72%	7.581%
7	10.109	1152	1161	1182	rBV	559853	1053892	29.68%	6.672%
8	11.795	1440	1448	1455	rBV	208635	379618	10.69%	2.403%
9	12.640	1585	1592	1604	rBV	48153	94693	2.67%	0.600%
10	14.150	1842	1849	1857	rBV	1495815	2368176	66.69%	14.994%
11	15.525	2076	2083	2092	rVB2	311144	517558	14.57%	3.277%
12	16.993	2326	2333	2344	rBV	1166330	1817098	51.17%	11.505%
13	18.251	2540	2547	2558	rBV2	400903	647920	18.25%	4.102%
14	19.044	2675	2682	2691	rBV2	29219	45924	1.29%	0.291%
15	20.771	2969	2976	2987	rBV	2526555	3551000	100.00%	22.482%
16	22.603	3280	3288	3305	rBV2	346362	689422	19.41%	4.365%
17	26.404	3921	3935	3958	rBV3	154602	632387	17.81%	4.004%


Sum of corrected areas: 15794574

Data Path : Z:\HPCHEM1\BNA G\DATA\BG031218\
Data File : BG033103.D
Acq On : 13 Mar 2018 00:21
Operator : SJ/JU
Sample : J1867-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CPS073071

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

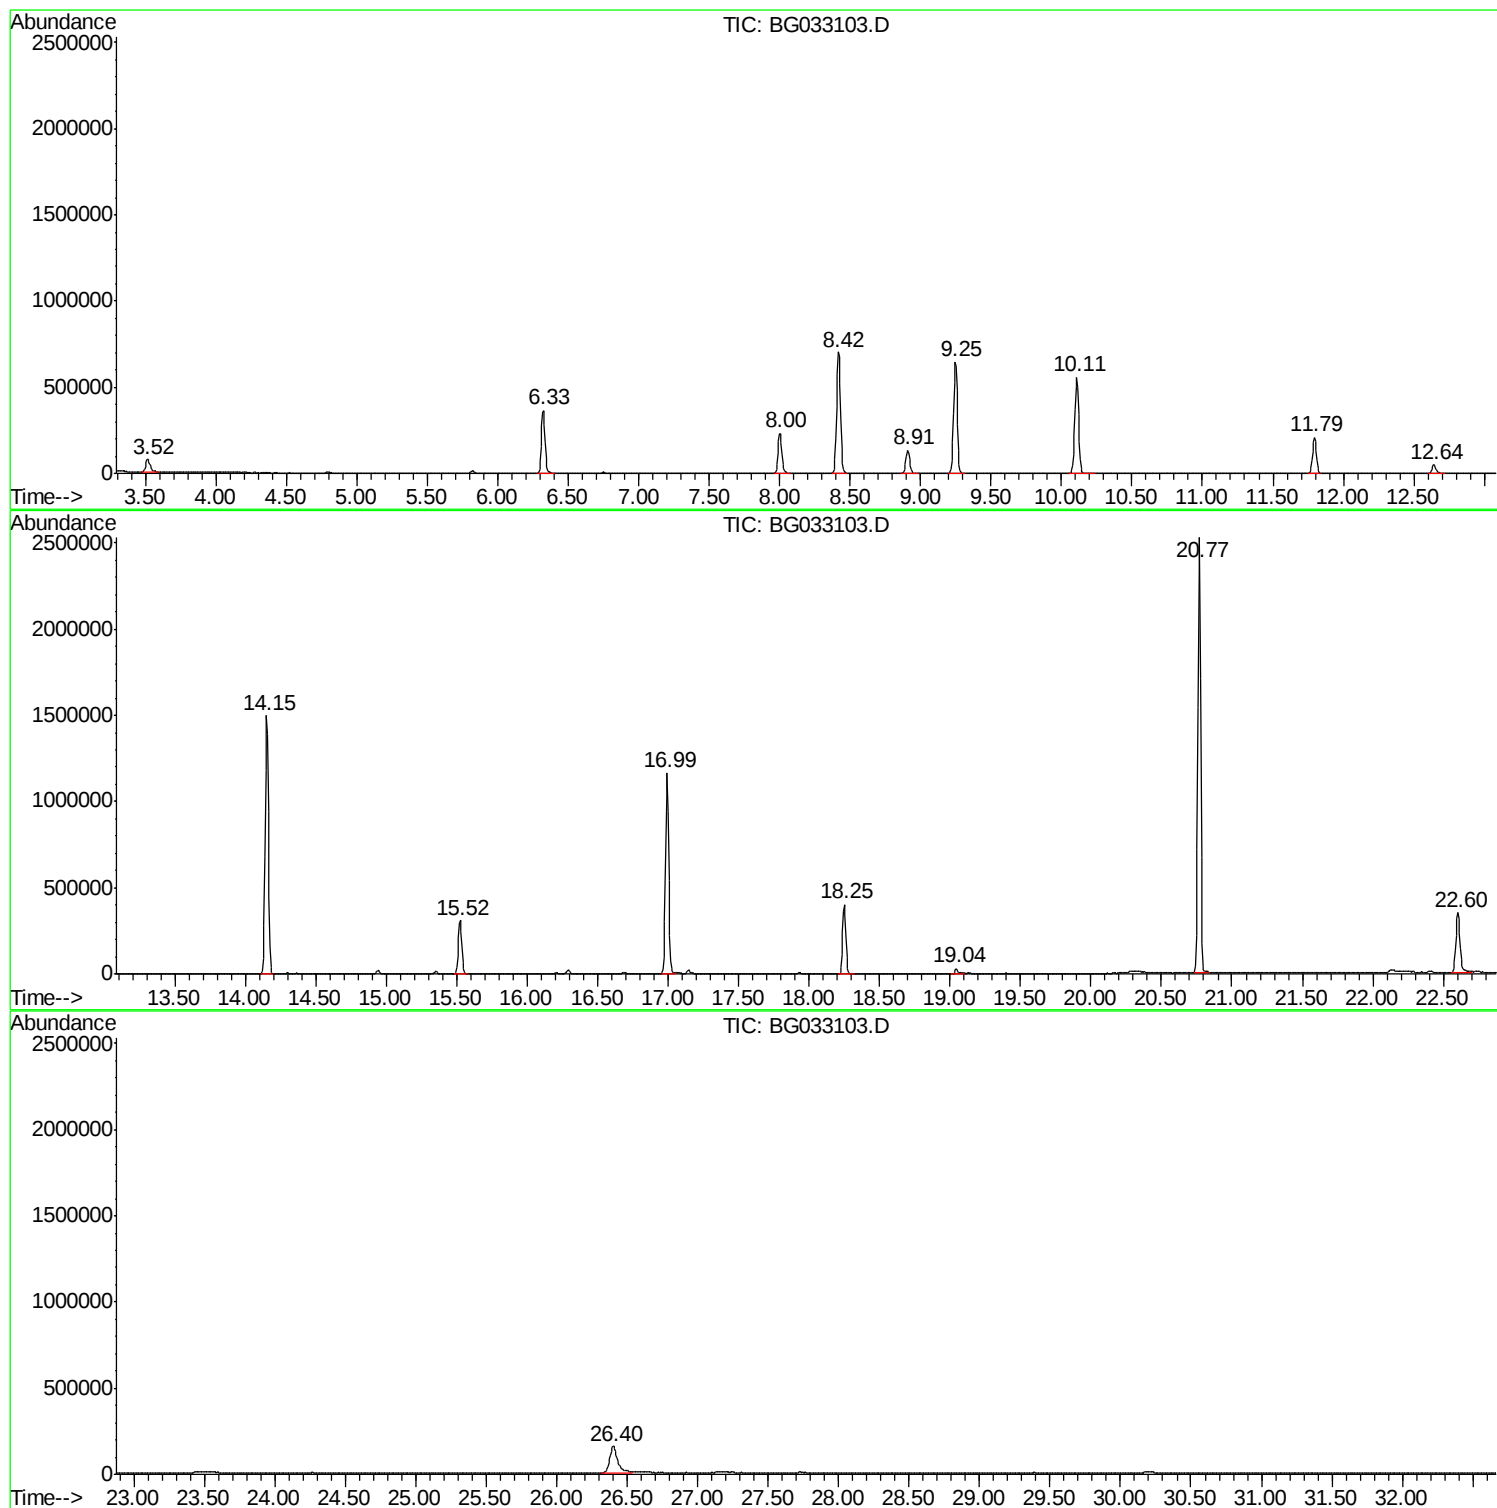

Data Path : Z:\HPCHEM1\BNA G\DATA\BG031218\
Data File : BG033103.D
Acq On : 13 Mar 2018 00:21
Operator : SJ/JU
Sample : J1867-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CPS073071










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown8.42 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.42	103.54 ng	1301310	1,4-Dichlorobenzene-d4	8.91

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	12
4		5-Aminoindole	132	C8H8N2	005192-03-0	12
5		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10

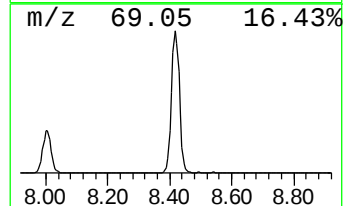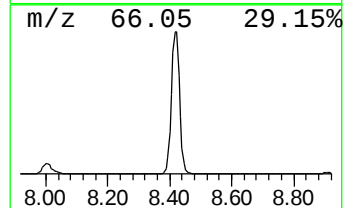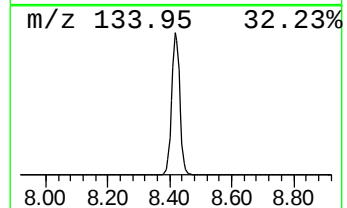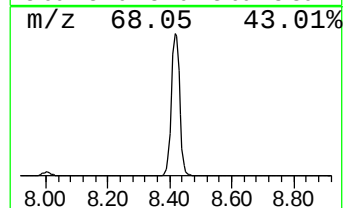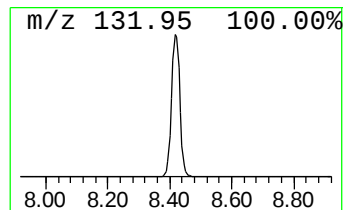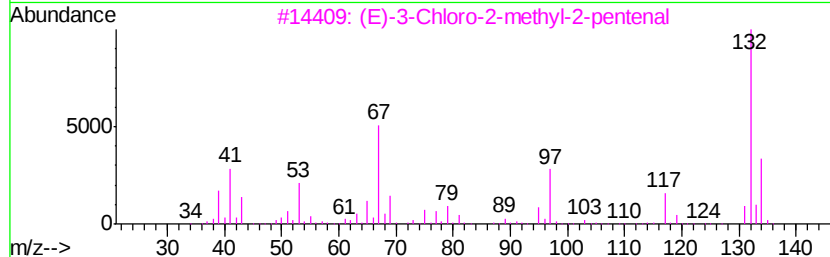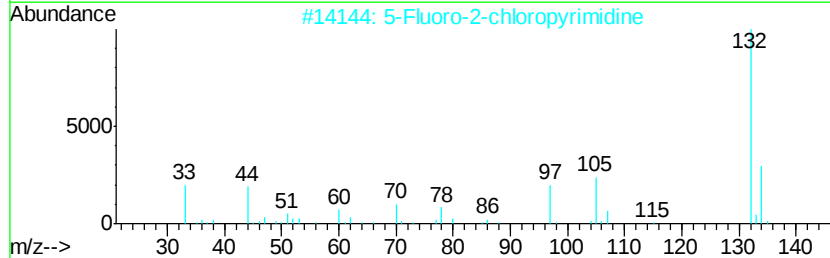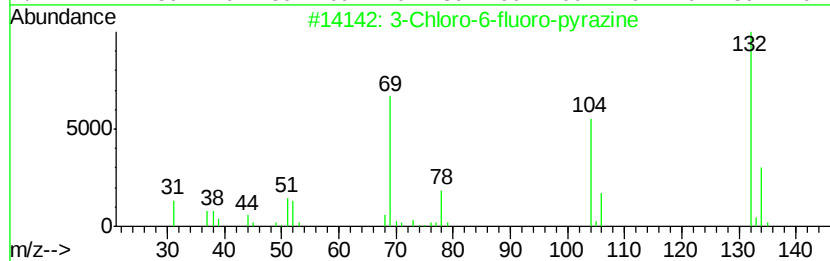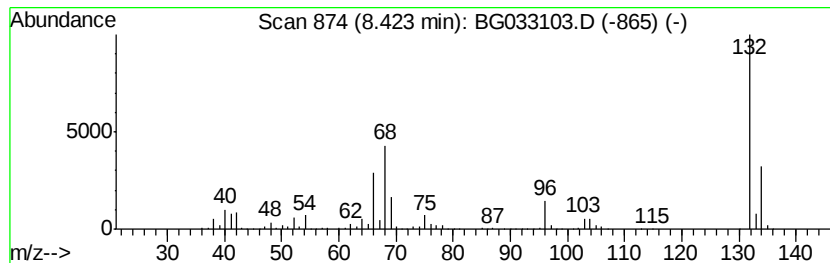

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG031218\
Data File : BG033103.D
Acq On : 13 Mar 2018 00:21
Operator : SJ/JU
Sample : J1867-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CPS073071

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown8.42	8.42	103.5	ng	1301310	1	8.91	251353	20.0