


Data Path : Z:\HPCHEM1\BNA G\Data\BG031218\
 Data File : BG033083.D
 Acq On : 12 Mar 2018 10:03
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 09 15:10:14 2018

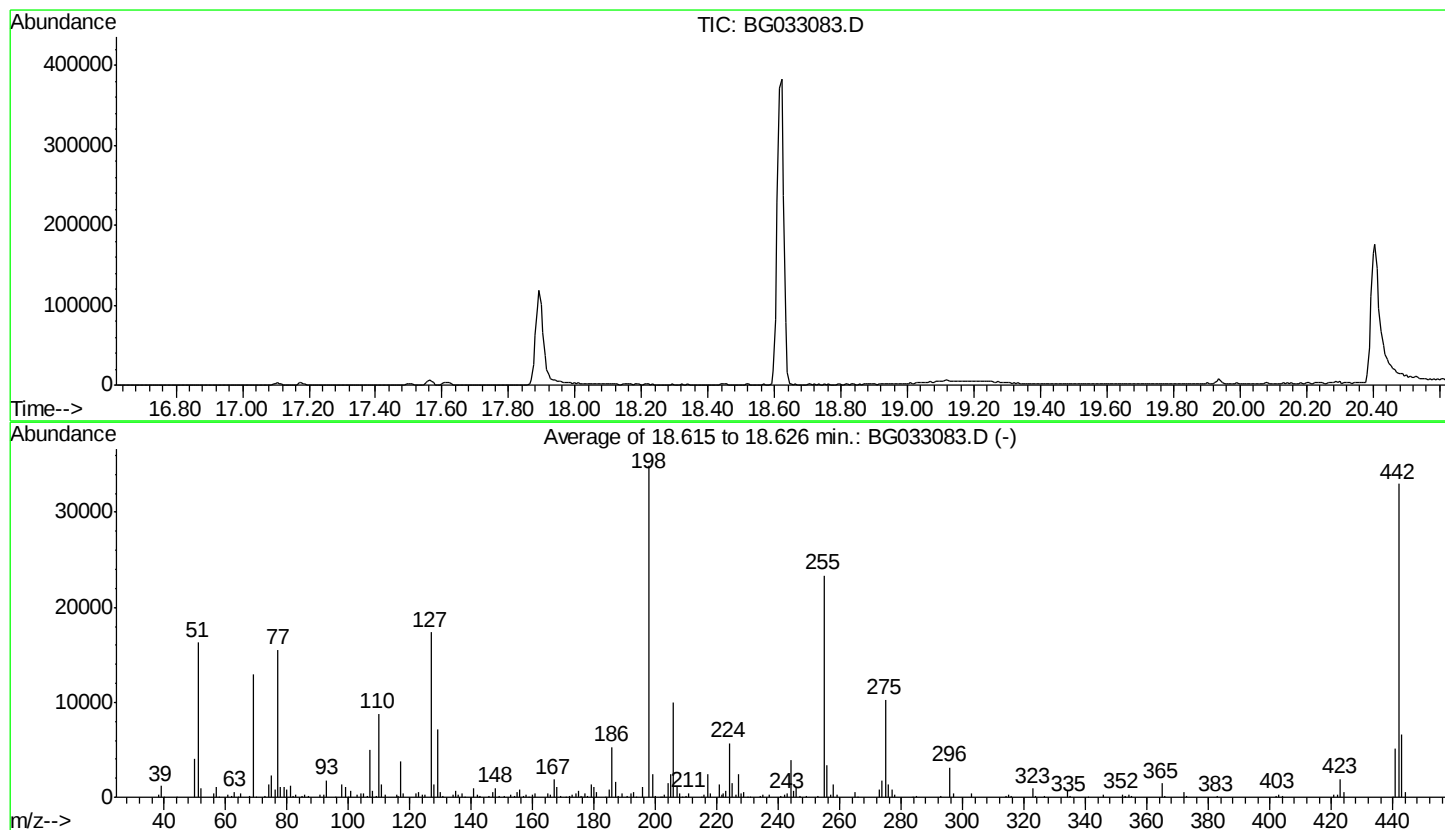

AutoFind: Scans 2609, 2610, 2611; Background Corrected with Scan 2602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.6	16278	PASS
68	69	0.00	2	0.6	77	PASS
69	198	0.00	100	37.2	12992	PASS
70	69	0.00	2	0.5	69	PASS
127	198	10	80	49.8	17390	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	34922	PASS
199	198	5	9	6.9	2413	PASS
275	198	10	60	29.4	10268	PASS
365	198	1	100	4.1	1430	PASS
441	442	0.01	24	15.4	5077	PASS
442	198	50	100	94.5	32997	PASS
443	442	15	24	19.9	6579	PASS