


Data Path : Z:\HPCHEM1\BNA G\Data\BG031218\
 Data File : BG033101.D
 Acq On : 12 Mar 2018 23:06
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 09 15:10:14 2018

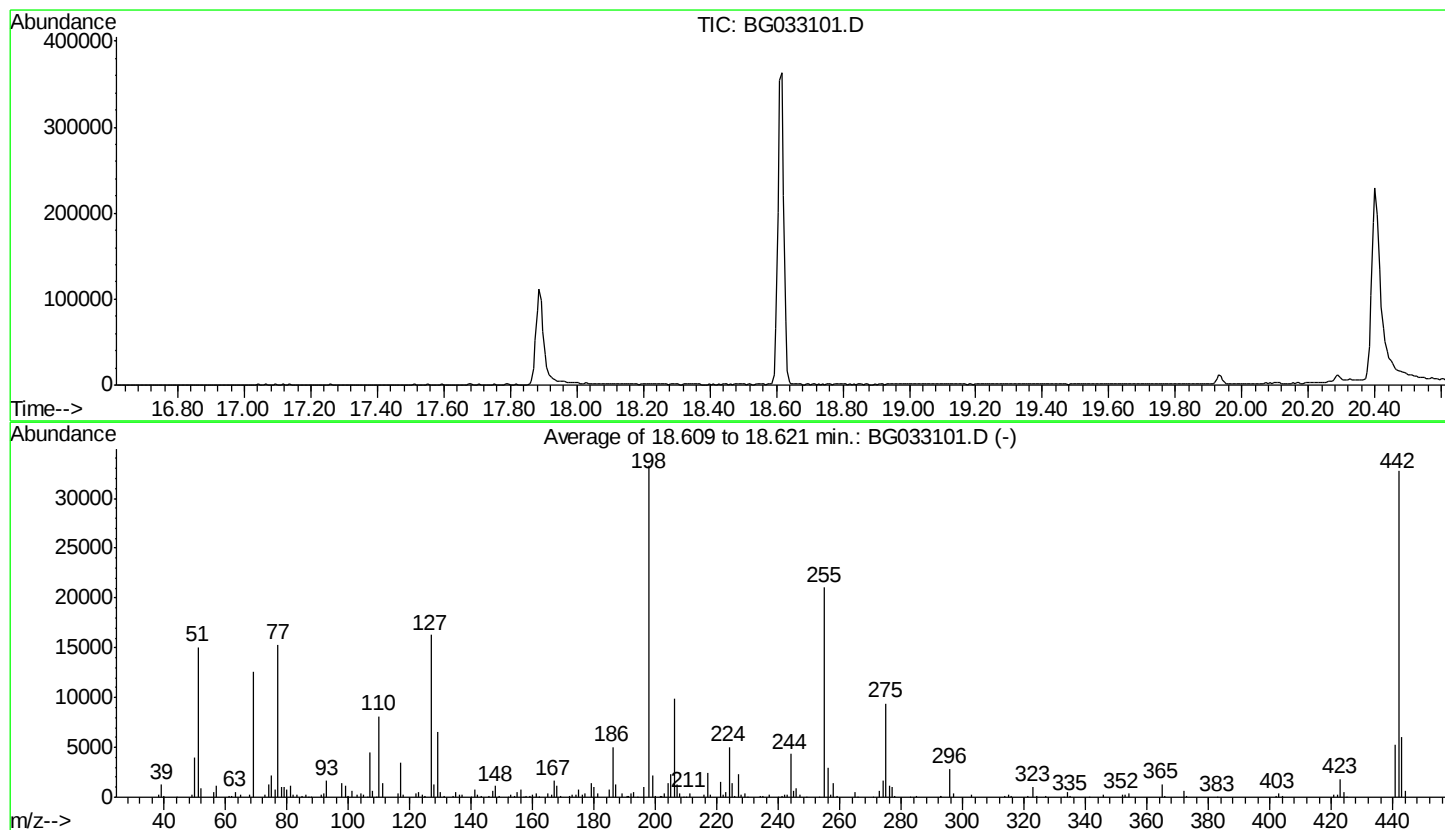

AutoFind: Scans 2608, 2609, 2610; Background Corrected with Scan 2601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.2	15056	PASS
68	69	0.00	2	1.6	199	PASS
69	198	0.00	100	37.7	12564	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.0	16303	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	33290	PASS
199	198	5	9	6.5	2156	PASS
275	198	10	60	28.3	9416	PASS
365	198	1	100	4.0	1344	PASS
441	442	0.01	24	16.0	5249	PASS
442	198	50	100	98.6	32813	PASS
443	442	15	24	18.4	6031	PASS