

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG031219\
 Data File : BG039887.D
 Acq On : 12 Mar 2019 23:31
 Operator : JU/SJ
 Sample : K1824-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP-27

Quant Time: Mar 13 05:50:35 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 13 05:34:05 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.15	152	42401	20.00	ng	0.00
21) Naphthalene-d8	10.97	136	180133	20.00	ng	0.00
39) Acenaphthene-d10	14.77	164	117093	20.00	ng	0.00
64) Phenanthrene-d10	17.52	188	291062	20.00	ng	0.00
76) Chrysene-d12	21.81	240	316355	20.00	ng	0.00
87) Perylene-d12	25.18	264	312585	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.70	112	291614	117.33	ng	0.00
7) Phenol-d6	7.30	99	417243	112.59	ng	0.00
23) Nitrobenzene-d5	9.33	82	251003	75.36	ng	0.00
42) 2,4,6-Tribromophenol	16.27	330	151375	110.91	ng	0.00
45) 2-Fluorobiphenyl	13.40	172	535077	65.06	ng	0.00
79) Terphenyl-d14	20.11	244	952882	66.32	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.33	70	32114	12.039	ng	Qvalue # 69
50) Dimethylphthalate	14.22	163	48131	4.916	ng	100
57) 2,4-Dinitrotoluene	14.77	165	14761	5.061	ng	# 20
67) 4-Bromophenyl-phenylether	16.26	248	12320	3.782	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG031219\
Data File : BG039887.D
Acq On : 12 Mar 2019 23:31
Operator : JU/SJ
Sample : K1824-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-27

Quant Time: Mar 13 05:50:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 13 05:34:05 2019
Response via : Initial Calibration

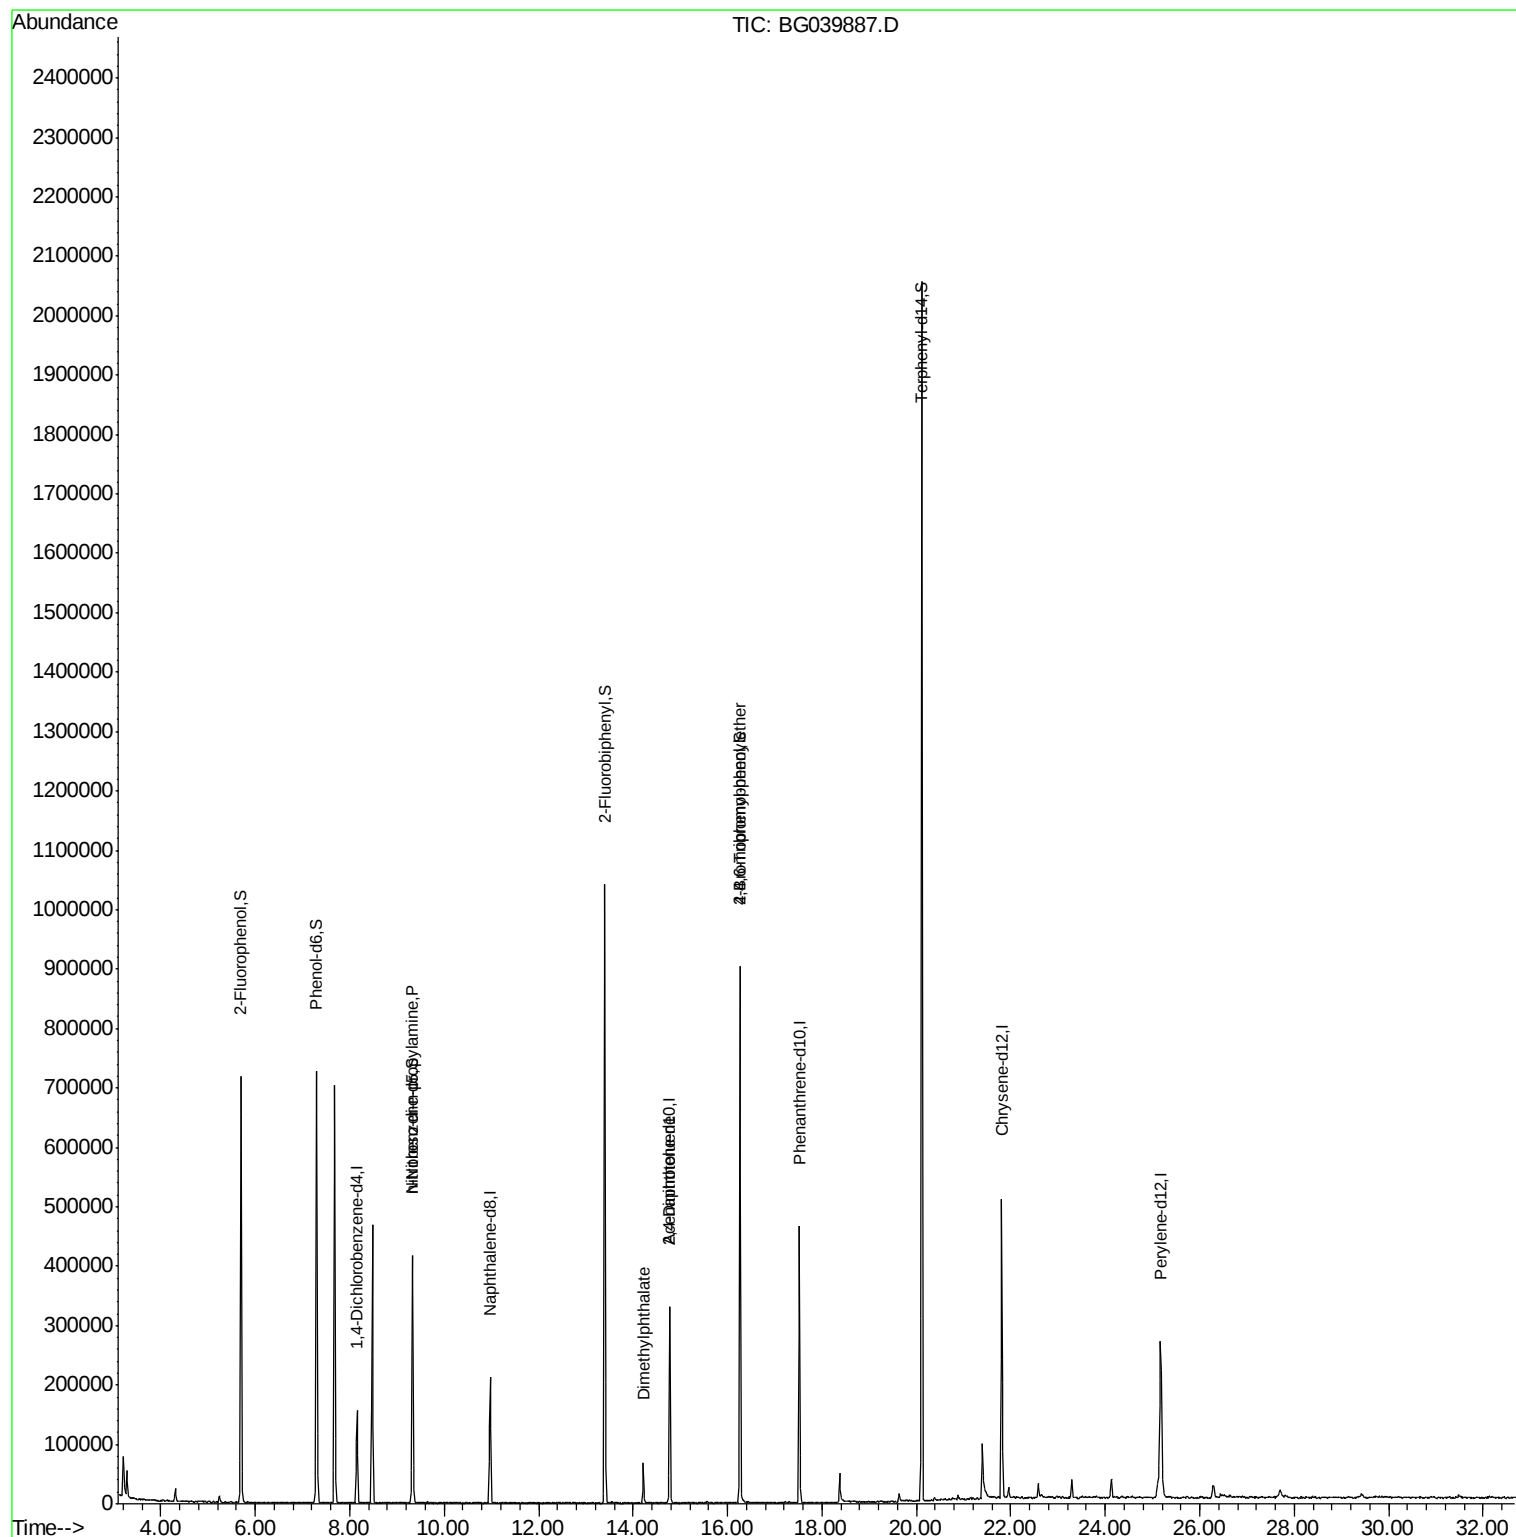




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.15 min Scan# 862
Delta R.T. 0.00 min
Lab File: BG039887.D
Acq: 12 Mar 2019 23:31

Instrument :
BNA_G
ClientSampled :
TP-27

Tgt Ion:152 Resp: 42401
Ion Ratio Lower Upper
152 100
150 166.7 123.7 185.5
115 62.3 45.9 68.9

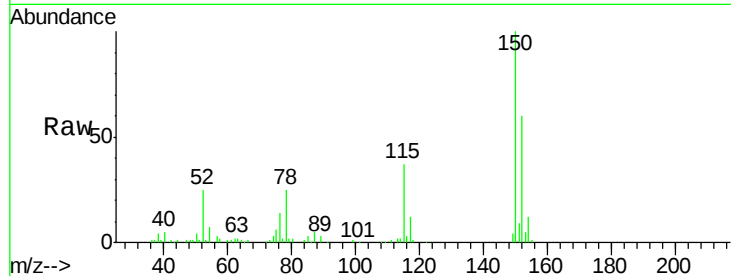


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

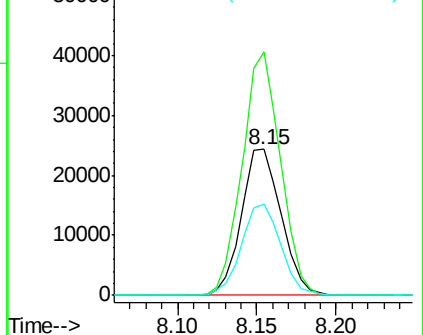



#5

2-Fluorophenol
Concen: 117.331 ng
RT: 5.70 min Scan# 444
Delta R.T. -0.00 min
Lab File: BG039887.D
Acq: 12 Mar 2019 23:31

Tgt Ion:112 Resp: 291614
Ion Ratio Lower Upper
112 100
64 69.1 57.8 86.8
63 37.4 29.8 44.6



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

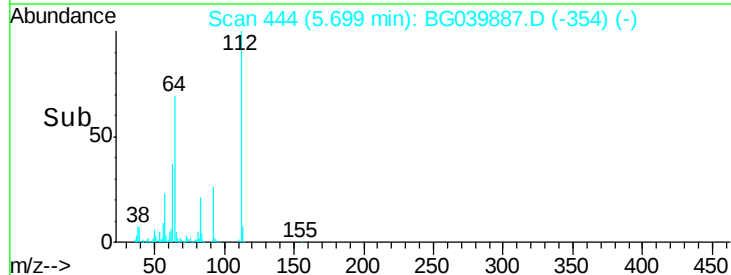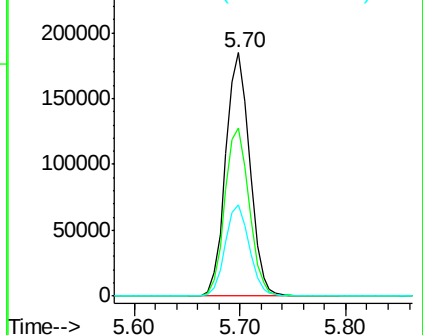



#7

Phenol-d6

Concen: 112.590 ng

RT: 7.30 min Scan# 716

Delta R.T. 0.00 min

Lab File: BG039887.D

Acq: 12 Mar 2019 23:31

Instrument :

BNA_G

ClientSampleId :

TP-27


Tgt Ion: 99 Resp: 417243

Ion Ratio Lower Upper




99 100

42 19.9 18.2 27.2

71 36.7 28.0 42.0

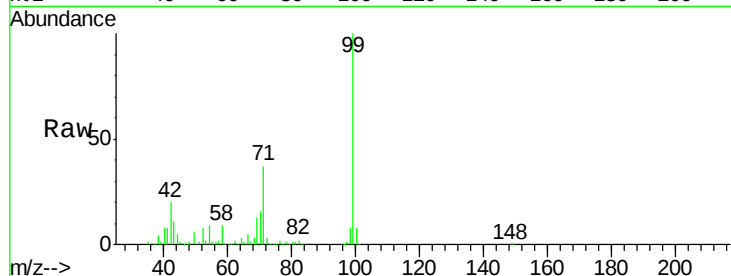

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

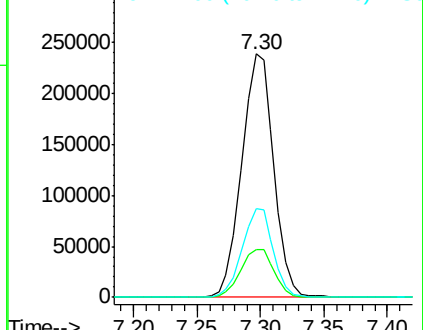

#19

n-Nitroso-di-n-propylamine

Concen: 12.039 ng

RT: 9.33 min Scan# 1062

Delta R.T. 0.38 min

Lab File: BG039887.D

Acq: 12 Mar 2019 23:31

Tgt Ion: 70 Resp: 32114


Ion Ratio Lower Upper

70 100



42 49.9 60.4 90.6#

101 0.0 7.5 11.3#

130 3.0 16.9 25.3#



Abundance Ion 70.00 (69.70 to 70.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 101.00 (100.70 to 101.70): BGC
Ion 130.00 (129.70 to 130.70): BGC

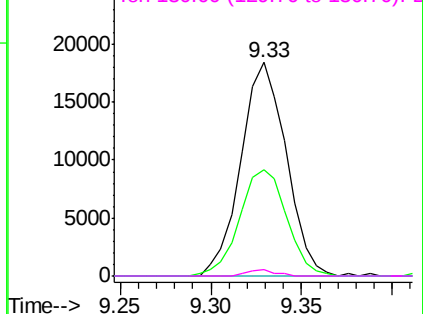







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.97 min Scan# 1342
Delta R.T. 0.00 min
Lab File: BG039887.D
Acq: 12 Mar 2019 23:31

Instrument :
BNA_G
ClientSampleId :
TP-27

Tgt Ion:	136	Resp:	180133
Ion	Ratio	Lower	Upper
136	100		
137	11.5	9.1	13.7
54	11.2	9.4	14.2
68	6.9	4.2	6.4#




Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

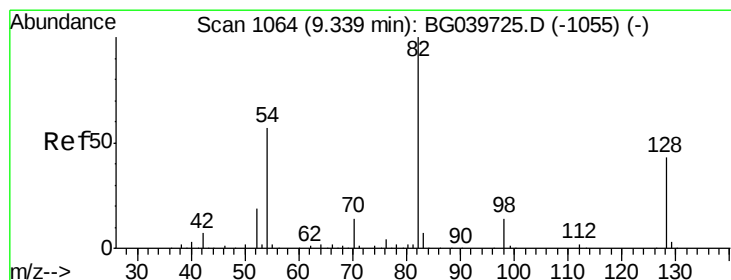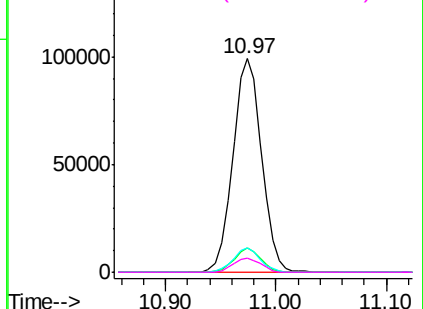




#23
Nitrobenzene-d5
Concen: 75.362 ng
RT: 9.33 min Scan# 1062
Delta R.T. 0.00 min
Lab File: BG039887.D
Acq: 12 Mar 2019 23:31

Tgt Ion:	82	Resp:	251003
Ion	Ratio	Lower	Upper
82	100		
128	42.6	31.3	46.9
54	58.2	50.9	76.3



Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

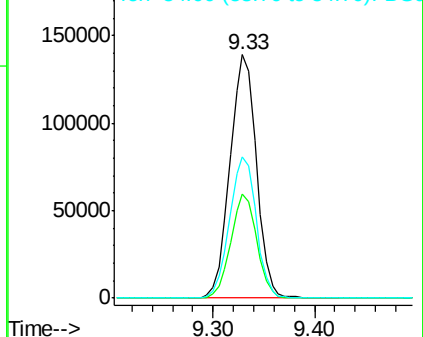

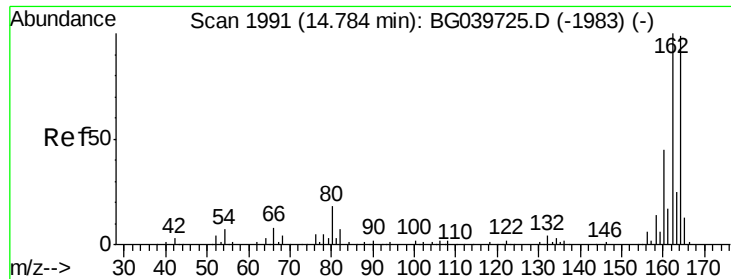

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.77 min Scan# 1989

Delta R.T. -0.01 min

Lab File: BG039887.D

Acq: 12 Mar 2019 23:31

Instrument :

BNA_G

ClientSampleId :

TP-27


Tgt Ion:164 Resp: 117093

Ion Ratio Lower Upper

164 100

162 103.6 81.6 122.4




160 43.8 34.2 51.2



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

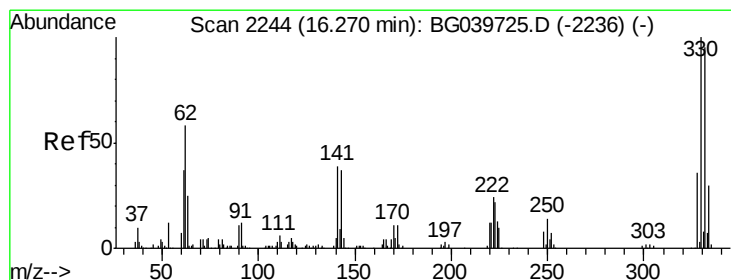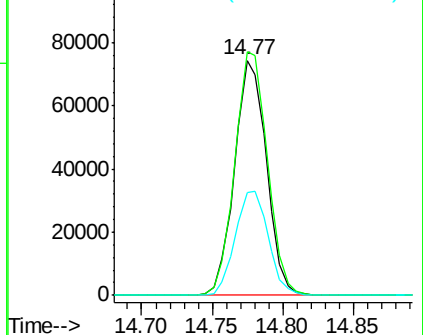

#42

2,4,6-Tribromophenol

Concen: 110.913 ng

RT: 16.27 min Scan# 2243

Delta R.T. 0.00 min

Lab File: BG039887.D

Acq: 12 Mar 2019 23:31


Tgt Ion:330 Resp: 151375

Ion Ratio Lower Upper

330 100

332 96.4 75.7 113.5



141 42.6 35.6 53.4



Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E




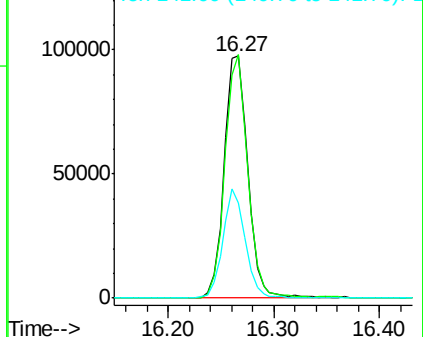




#45
 2-Fluorobiphenyl
 Concen: 65.064 ng
 RT: 13.40 min Scan# 1755
 Delta R.T. 0.00 min
 Lab File: BG039887.D
 Acq: 12 Mar 2019 23:31




Instrument :
 BNA_G
 ClientSampleId :
 TP-27

Tgt Ion:172 Resp: 535077
 Ion Ratio Lower Upper
 172 100
 171 36.7 30.8 46.2
 170 24.2 20.2 30.4

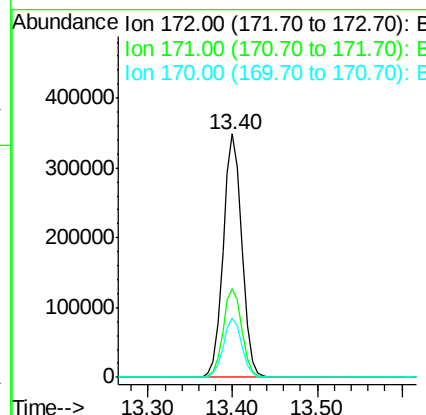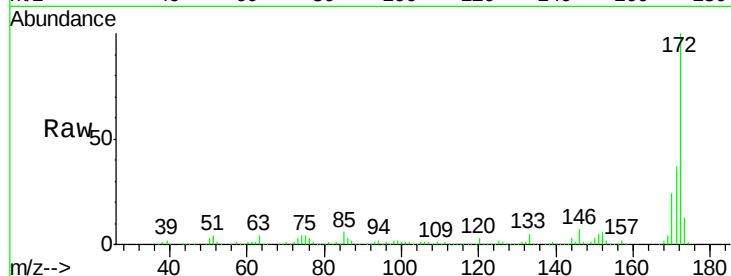

#50
 Dimethylphthalate
 Concen: 4.916 ng
 RT: 14.22 min Scan# 1895
 Delta R.T. -0.01 min
 Lab File: BG039887.D
 Acq: 12 Mar 2019 23:31

Tgt Ion:163 Resp: 48131
 Ion Ratio Lower Upper
 163 100
 194 4.4 3.6 5.4
 164 10.3 8.4 12.6



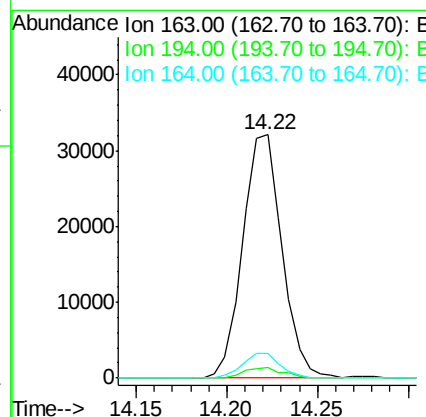
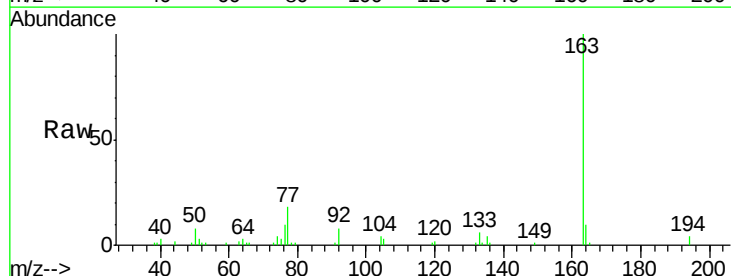




#57
 2,4-Dinitrotoluene
 Concen: 5.061 ng
 RT: 14.77 min Scan# 1989
 Delta R.T. -0.36 min
 Lab File: BG039887.D
 Acq: 12 Mar 2019 23:31




Instrument :
 BNA_G
 ClientSampleId :
 TP-27


Tgt Ion:	165	Resp:	14761
Ion	Ratio	Lower	Upper
165	100		
63	1.8	41.0	61.6#
89	2.5	64.6	96.8#
182	0.0	2.0	3.0#

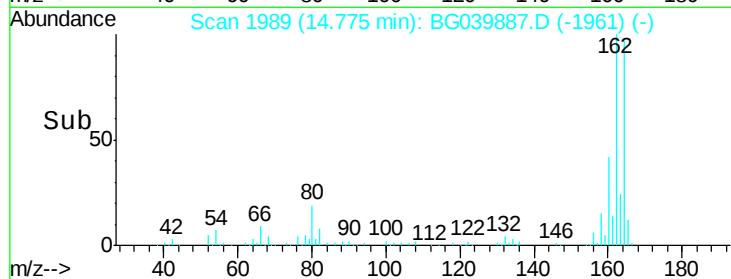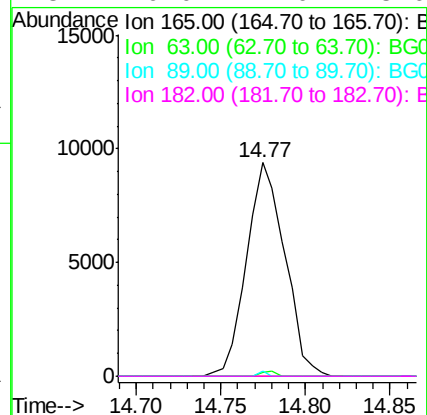

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.52 min Scan# 2457
 Delta R.T. 0.00 min
 Lab File: BG039887.D
 Acq: 12 Mar 2019 23:31

Tgt Ion:	188	Resp:	291062
Ion	Ratio	Lower	Upper
188	100		
94	8.2	6.9	10.3
80	8.7	8.1	12.1

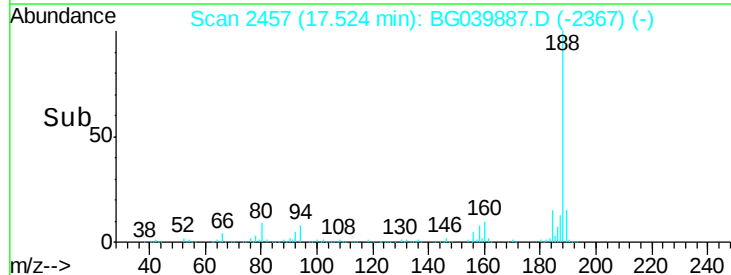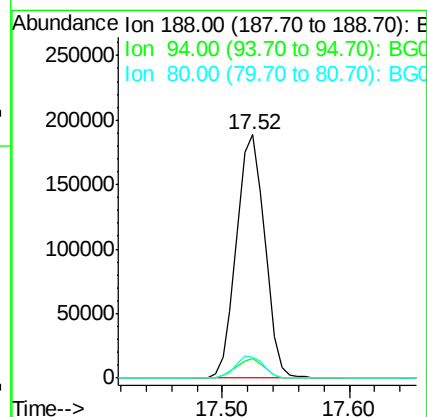


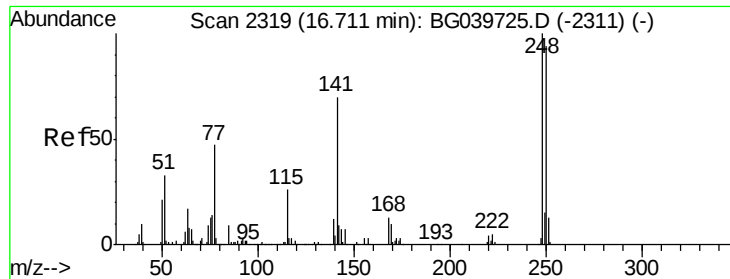




#67
 4-Bromophenyl-phenylether
 Concen: 3.782 ng
 RT: 16.26 min Scan# 2242
 Delta R.T. -0.45 min
 Lab File: BG039887.D
 Acq: 12 Mar 2019 23:31

Instrument :
 BNA_G
 ClientSampleId :
 TP-27

Tgt Ion:248 Resp: 12320
 Ion Ratio Lower Upper
 248 100
 250 187.8 77.6 116.4#
 141 517.5 63.9 95.9#

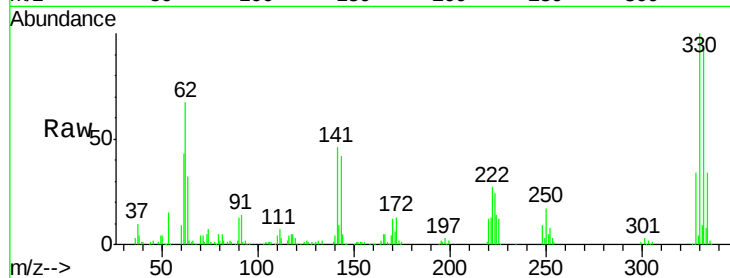


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

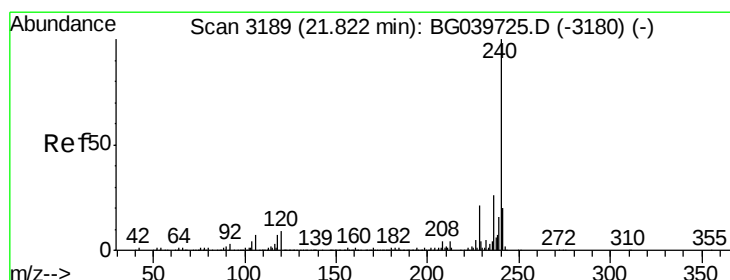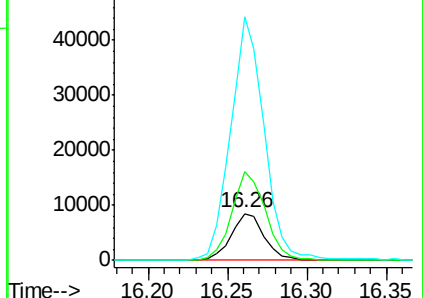
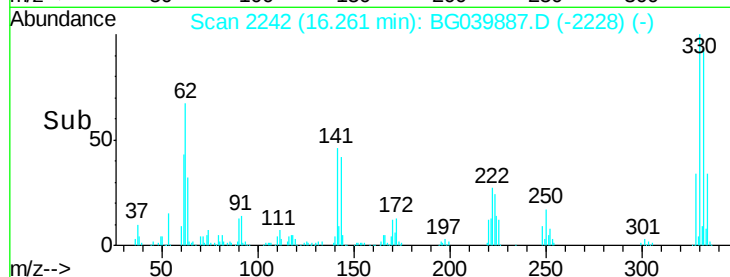



#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.81 min Scan# 3186
 Delta R.T. -0.01 min
 Lab File: BG039887.D
 Acq: 12 Mar 2019 23:31

Tgt Ion:240 Resp: 316355
 Ion Ratio Lower Upper
 240 100
 120 8.6 7.0 10.6
 236 26.4 21.0 31.4

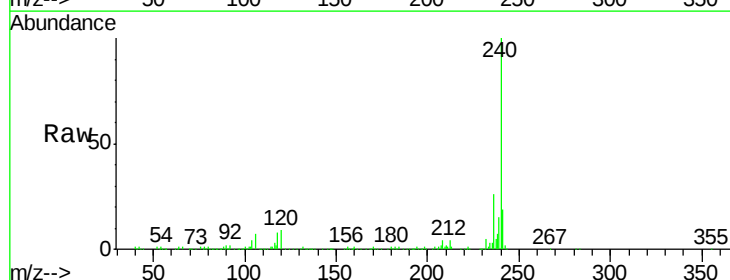

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

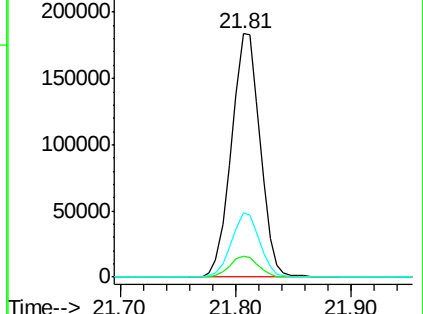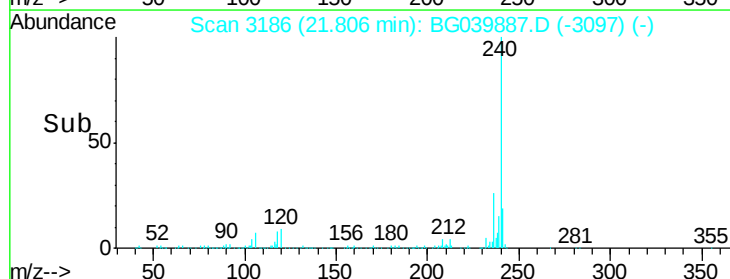

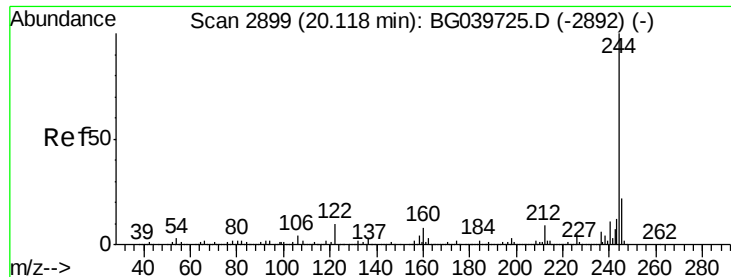

#79

Terphenyl-d14

Concen: 66.320 ng

RT: 20.11 min Scan# 2898

Delta R.T. 0.00 min

Lab File: BG039887.D

Acq: 12 Mar 2019 23:31

Instrument :

BNA_G

ClientSampleId :

TP-27


Tgt Ion:244 Resp: 952882

Ion Ratio Lower Upper

244 100

212 8.6 7.3 10.9




122 9.6 8.4 12.6

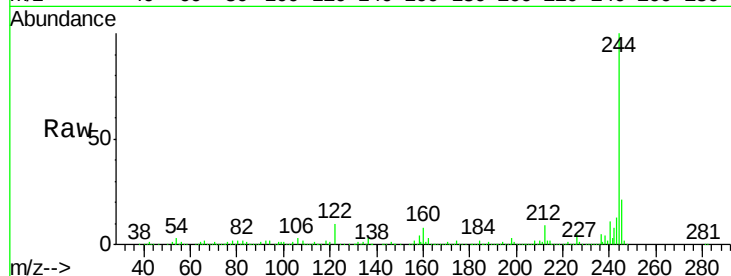

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

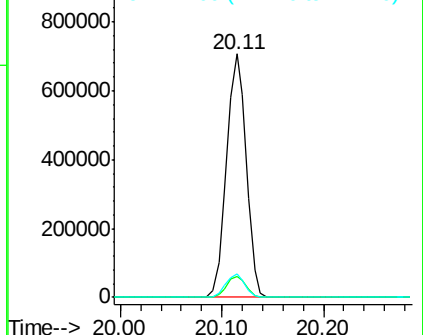

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.18 min Scan# 3760

Delta R.T. -0.01 min

Lab File: BG039887.D

Acq: 12 Mar 2019 23:31


Tgt Ion:264 Resp: 312585

Ion Ratio Lower Upper

264 100

260 25.4 18.2 27.4

265 20.6 18.5 27.7



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

