

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG031219\
 Data File : BG039890.D
 Acq On : 13 Mar 2019 2:10
 Operator : JU/SJ
 Sample : K1687-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 HR-06-031119-B

Quant Time: Mar 13 07:09:54 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG030419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 13 05:34:05 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	41868	20.00	ng	0.00
21) Naphthalene-d8	10.97	136	165141	20.00	ng	0.00
39) Acenaphthene-d10	14.78	164	114422	20.00	ng	0.00
64) Phenanthrene-d10	17.52	188	294587	20.00	ng	0.00
76) Chrysene-d12	21.81	240	327709	20.00	ng	0.00
87) Perylene-d12	25.17	264	316568	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.70	112	320929	130.77	ng	0.00
7) Phenol-d6	7.30	99	401892	109.83	ng	0.00
23) Nitrobenzene-d5	9.33	82	329156	107.80	ng	0.00
42) 2,4,6-Tribromophenol	16.26	330	217978	163.44	ng	0.00
45) 2-Fluorobiphenyl	13.40	172	767442	95.50	ng	0.00
79) Terphenyl-d14	20.12	244	1449308	97.38	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG031219\
Data File : BG039890.D
Acq On : 13 Mar 2019 2:10
Operator : JU/SJ
Sample : K1687-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
HR-06-031119-B

Quant Time: Mar 13 07:09:54 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG030419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 13 05:34:05 2019
Response via : Initial Calibration

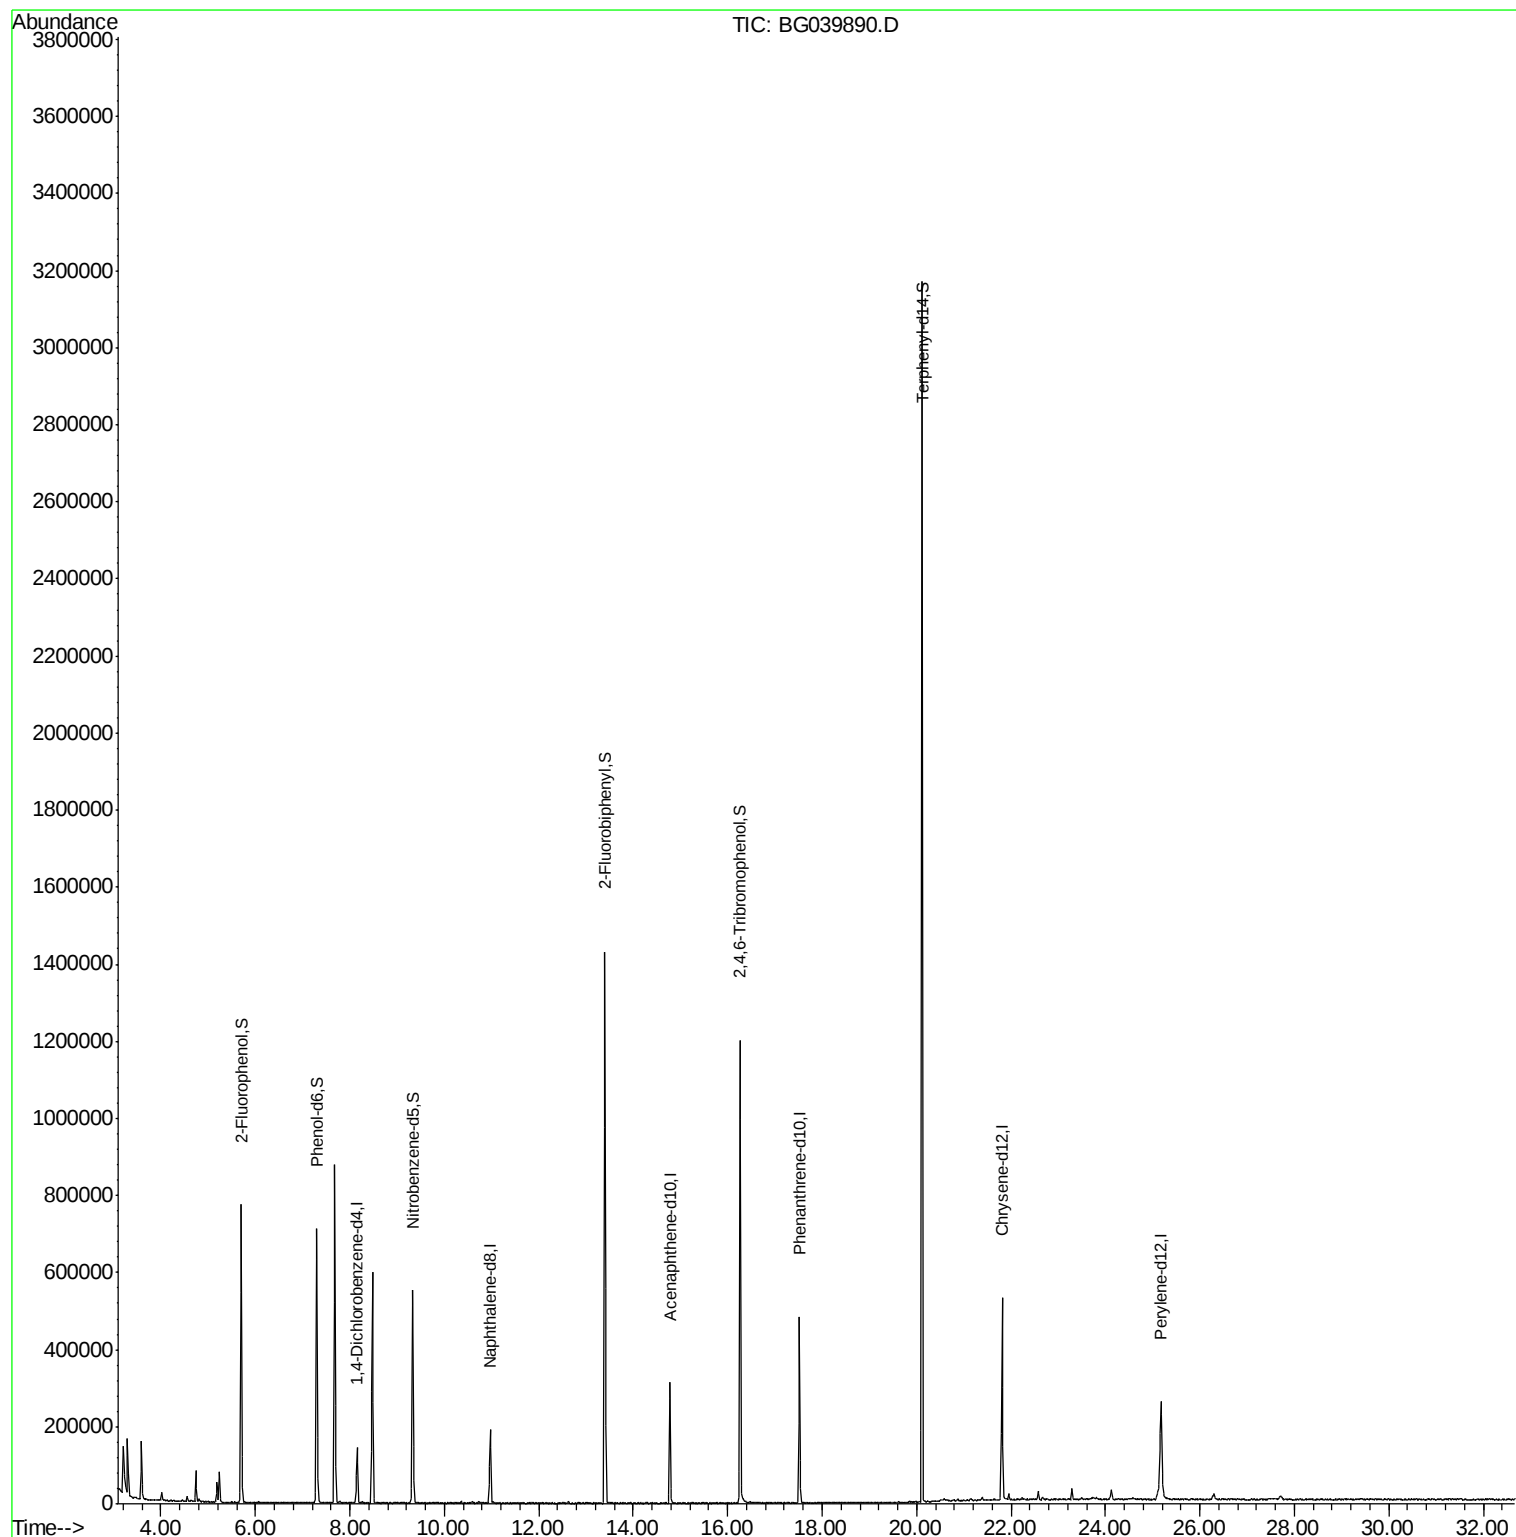




#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.16 min Scan# 863
Delta R.T. 0.00 min
Lab File: BG039890.D
Acq: 13 Mar 2019 2:10

Instrument :
BNA_G
ClientSampleId :
HR-06-031119-B

Tot Ion	Ratio	Lower	Upper
152	100		
150	143.7	123.7	185.5
115	54.9	45.9	68.9



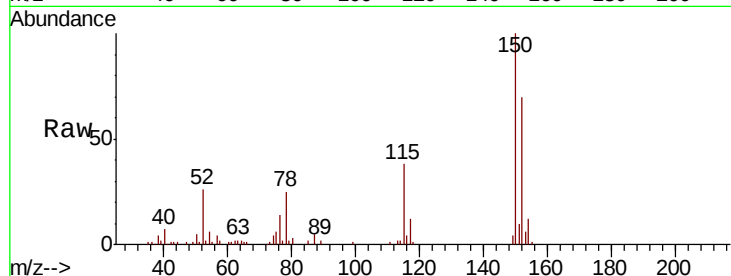


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

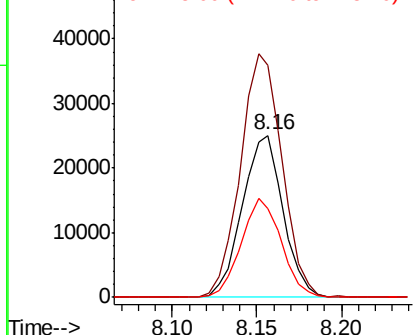

#5

2-Fluorophenol
Concen: 130.770 ng
RT: 5.70 min Scan# 445
Delta R.T. 0.00 min
Lab File: BG039890.D
Acq: 13 Mar 2019 2:10

Tgt Ion	Ratio	Lower	Upper
112	100		
64	69.6	57.8	86.8
63	37.6	29.8	44.6






Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

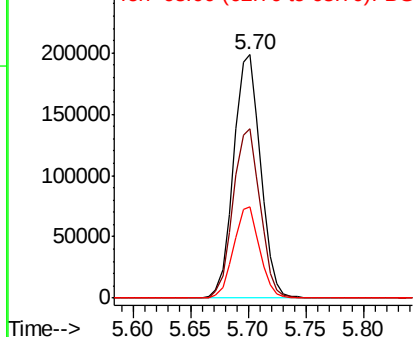



#7

Phenol-d6

Concen: 109.828 ng

RT: 7.30 min Scan# 717

Delta R.T. 0.00 min

Lab File: BG039890.D

Acq: 13 Mar 2019 2:10

Instrument :

BNA_G

ClientSampleId :

HR-06-031119-B


Tot Ion: 99 Resp: 401892

Ion Ratio Lower Upper




99 100

42 18.9 18.2 27.2

71 35.6 28.0 42.0

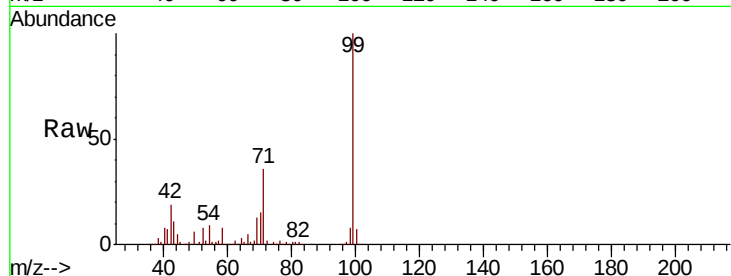

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

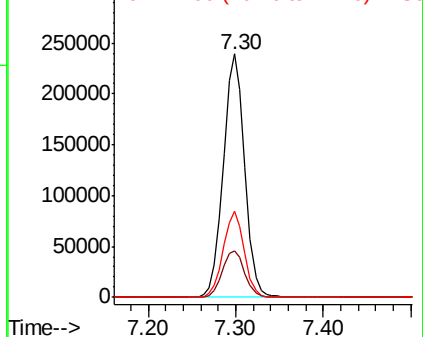

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.97 min Scan# 1342

Delta R.T. -0.00 min

Lab File: BG039890.D

Acq: 13 Mar 2019 2:10

Tgt Ion: 136 Resp: 165141


Ion Ratio Lower Upper

136 100



137 11.2 9.1 13.7


54 10.7 9.4 14.2

68 5.4 4.2 6.4



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC




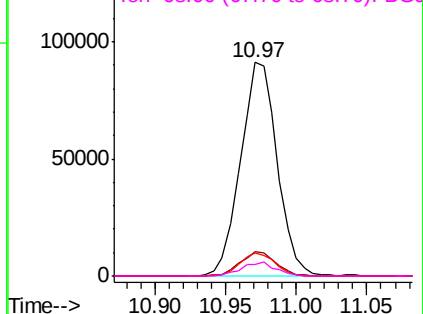


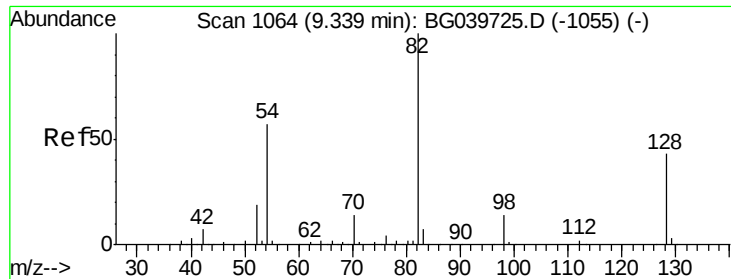

#23
Nitrobenzene-d5
Concen: 107.799 ng
RT: 9.33 min Scan# 1063
Delta R.T. 0.00 min
Lab File: BG039890.D
Acq: 13 Mar 2019 2:10




Instrument :
BNA_G
ClientSampleId :
HR-06-031119-B


Tot Ion: 82 Resp: 329156
Ion Ratio Lower Upper
82 100
128 43.7 31.3 46.9
54 60.1 50.9 76.3

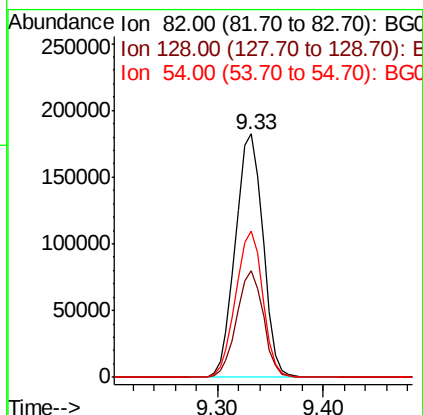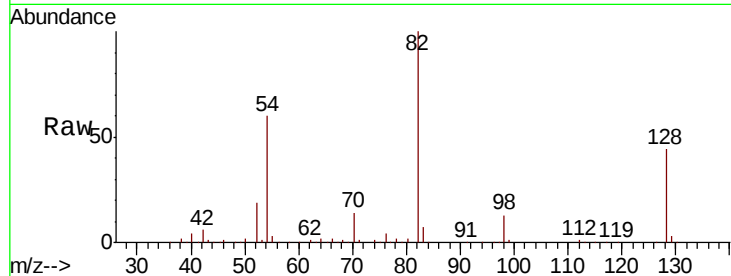

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.78 min Scan# 1990
Delta R.T. -0.00 min
Lab File: BG039890.D
Acq: 13 Mar 2019 2:10

Tgt Ion:164 Resp: 114422
Ion Ratio Lower Upper
164 100
162 100.4 81.6 122.4
160 42.7 34.2 51.2

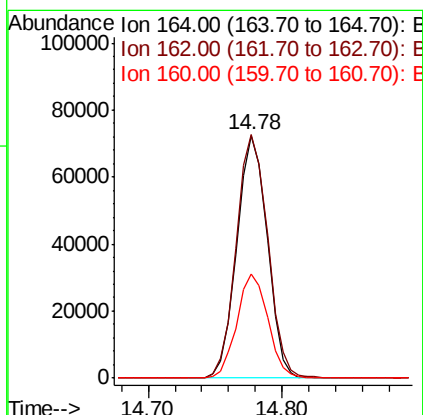


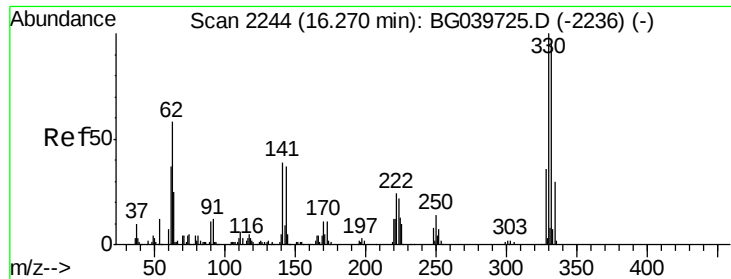

#42
 2,4,6-Tribromophenol
 Concen: 163.442 ng
 RT: 16.26 min Scan# 2243
 Delta R.T. -0.00 min
 Lab File: BG039890.D
 Acq: 13 Mar 2019 2:10

Instrument :
 BNA_G
 ClientSampleId :
 HR-06-031119-B

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.1	75.7	113.5
141	41.7	35.6	53.4



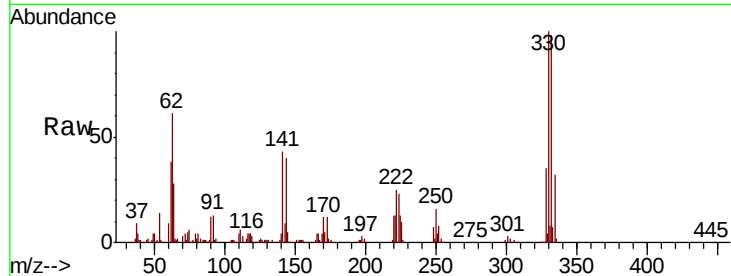


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

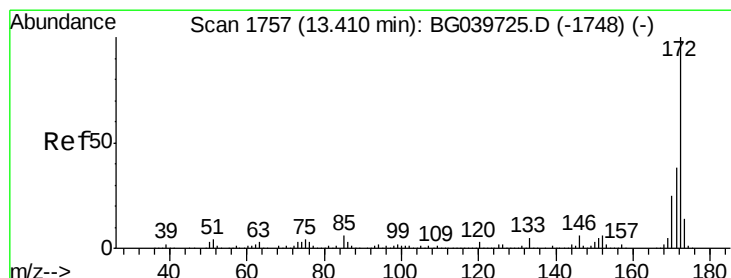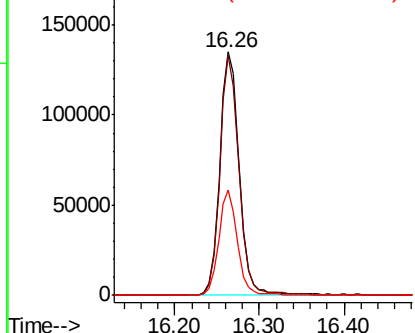

#45
 2-Fluorobiphenyl
 Concen: 95.498 ng
 RT: 13.40 min Scan# 1756
 Delta R.T. 0.00 min
 Lab File: BG039890.D
 Acq: 13 Mar 2019 2:10

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.3	30.8	46.2
170	25.2	20.2	30.4






Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

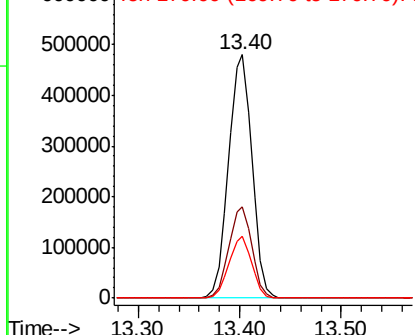



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.52 min Scan# 2457

Delta R.T. -0.00 min

Lab File: BG039890.D

Acq: 13 Mar 2019 2:10

Instrument :

BNA_G

ClientSampleId :

HR-06-031119-B


Tot Ion:188 Resp: 294587

Ion Ratio Lower Upper

188 100

94 7.5 6.9 10.3




80 8.7 8.1 12.1



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG

Ion 80.00 (79.70 to 80.70): BG

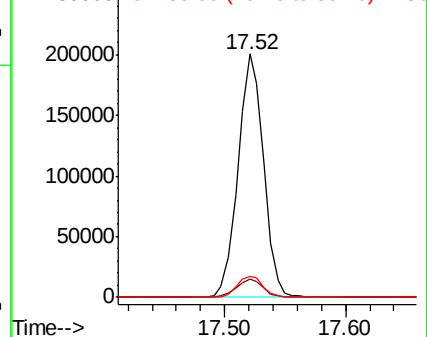

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.81 min Scan# 3187

Delta R.T. -0.00 min

Lab File: BG039890.D

Acq: 13 Mar 2019 2:10


Tgt Ion:240 Resp: 327709

Ion Ratio Lower Upper

240 100

120 7.9 7.0 10.6



236 26.3 21.0 31.4




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

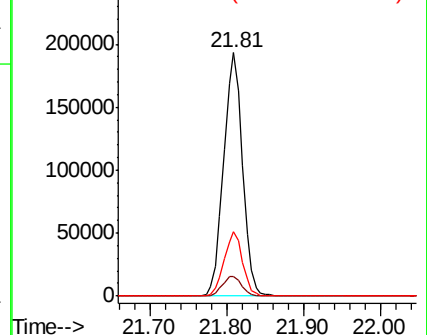

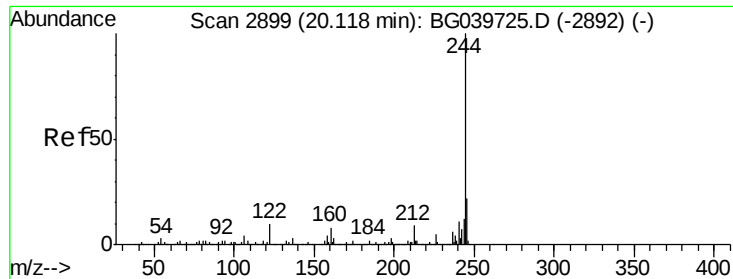

#79

Terphenyl-d14

Concen: 97.376 ng

RT: 20.12 min Scan# 2899

Delta R.T. 0.00 min

Lab File: BG039890.D

Acq: 13 Mar 2019 2:10

Instrument :

BNA_G

ClientSampleId :

HR-06-031119-B


Tot Ion:244 Resp: 1449308

Ion Ratio Lower Upper

244 100

212 9.4 7.3 10.9




122 9.5 8.4 12.6

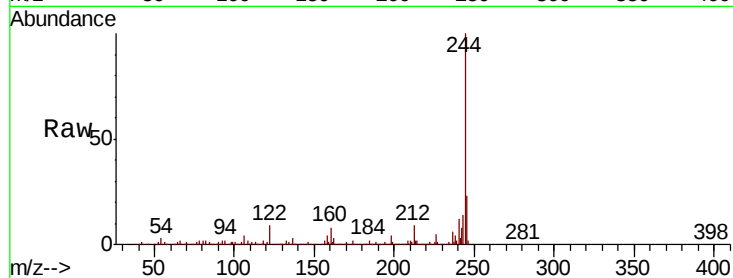

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

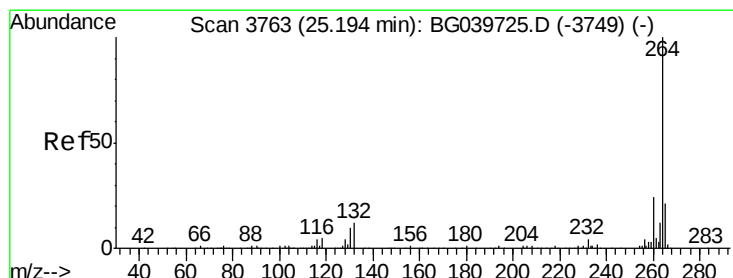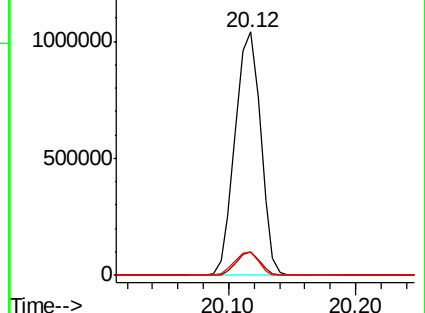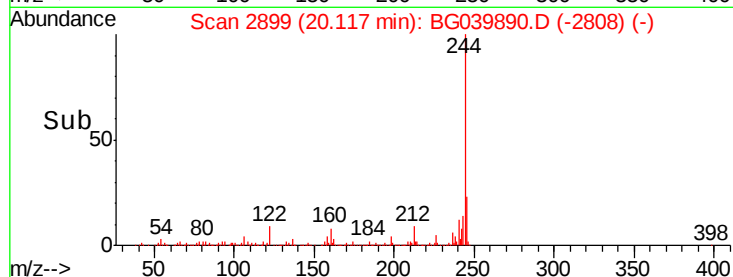

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.17 min Scan# 3760

Delta R.T. -0.01 min

Lab File: BG039890.D

Acq: 13 Mar 2019 2:10


Tgt Ion:264 Resp: 316568

Ion Ratio Lower Upper

264 100

260 23.9 18.2 27.4

265 20.8 18.5 27.7

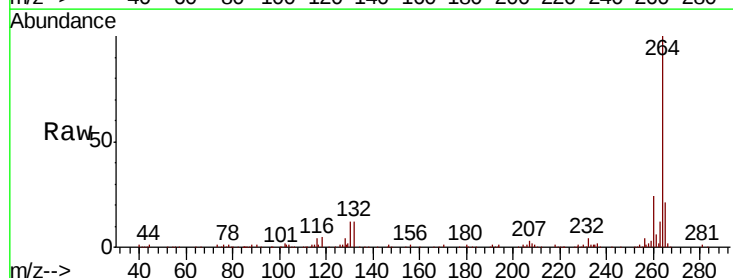

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

