

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG031219\
 Data File : BG039900.D
 Acq On : 13 Mar 2019 8:44
 Operator : JU/SJ
 Sample : PB117850BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB117850BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.200	15	19	28	rBV3	15732	32777	1.29%	0.268%
2	5.696	437	444	460	rBV	588443	939085	36.84%	7.673%
3	7.294	708	716	732	rBV	594281	1037571	40.70%	8.477%
4	7.676	774	781	794	rVB	545724	977321	38.34%	7.985%
5	8.152	856	862	871	rVB	141728	241393	9.47%	1.972%
6	8.475	909	917	926	rVB	400329	698838	27.41%	5.710%
7	9.327	1054	1062	1074	rBV	331513	593089	23.26%	4.846%
8	10.972	1335	1342	1352	rBV	187162	335553	13.16%	2.742%
9	13.398	1748	1755	1765	rBV	975722	1487097	58.33%	12.150%
10	14.778	1983	1990	2000	rBV2	307139	501708	19.68%	4.099%
11	16.264	2236	2243	2254	rBV	367718	624845	24.51%	5.105%
12	17.521	2450	2457	2467	rVB2	453000	679998	26.67%	5.556%
13	20.112	2892	2898	2905	rBV	1970230	2549352	100.00%	20.829%
14	21.810	3179	3187	3197	rBV	477425	831642	32.62%	6.795%
15	25.176	3747	3760	3775	rBV	212275	708904	27.81%	5.792%




Sum of corrected areas: 12239173

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG031219\
Data File : BG039900.D
Acq On : 13 Mar 2019 8:44
Operator : JU/SJ
Sample : PB117850BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB117850BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG030419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

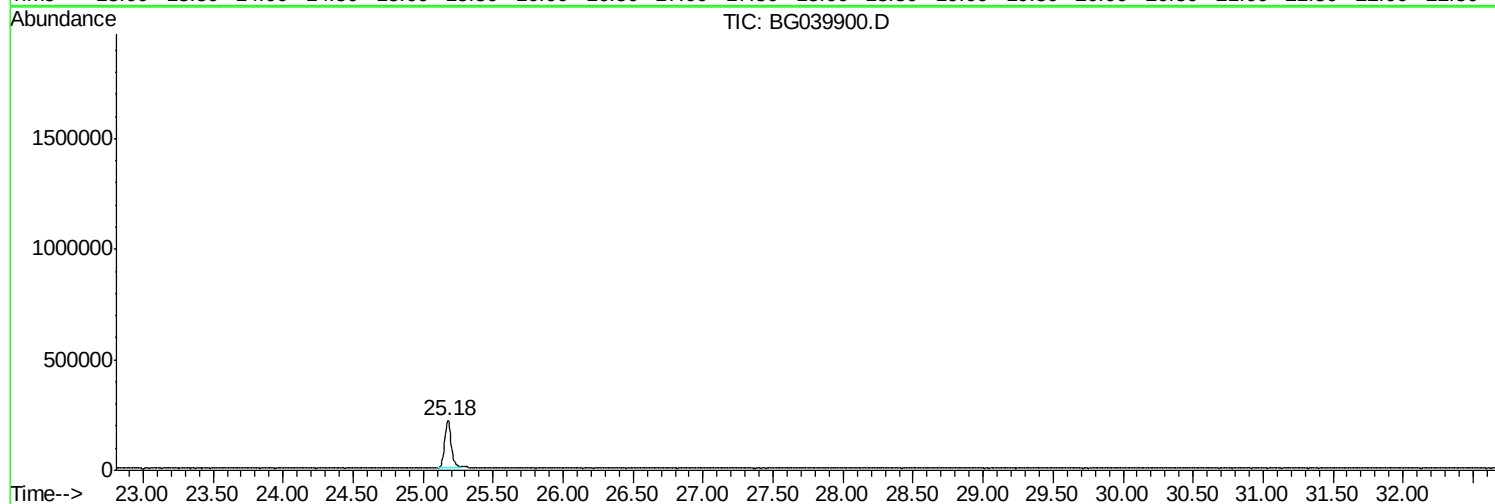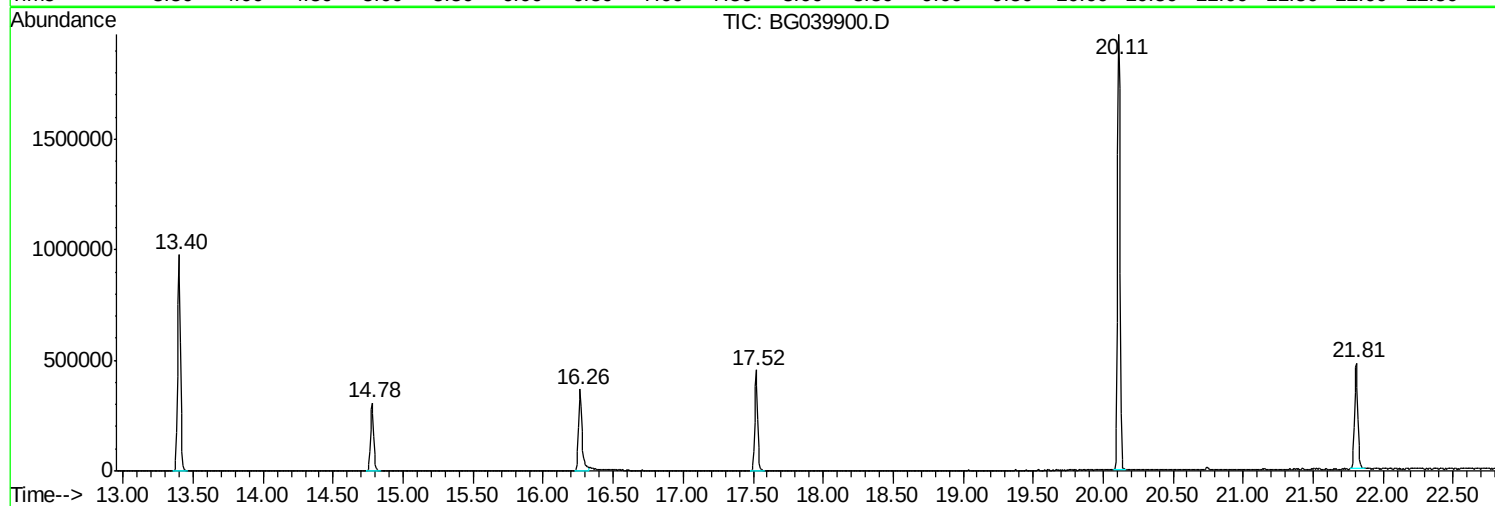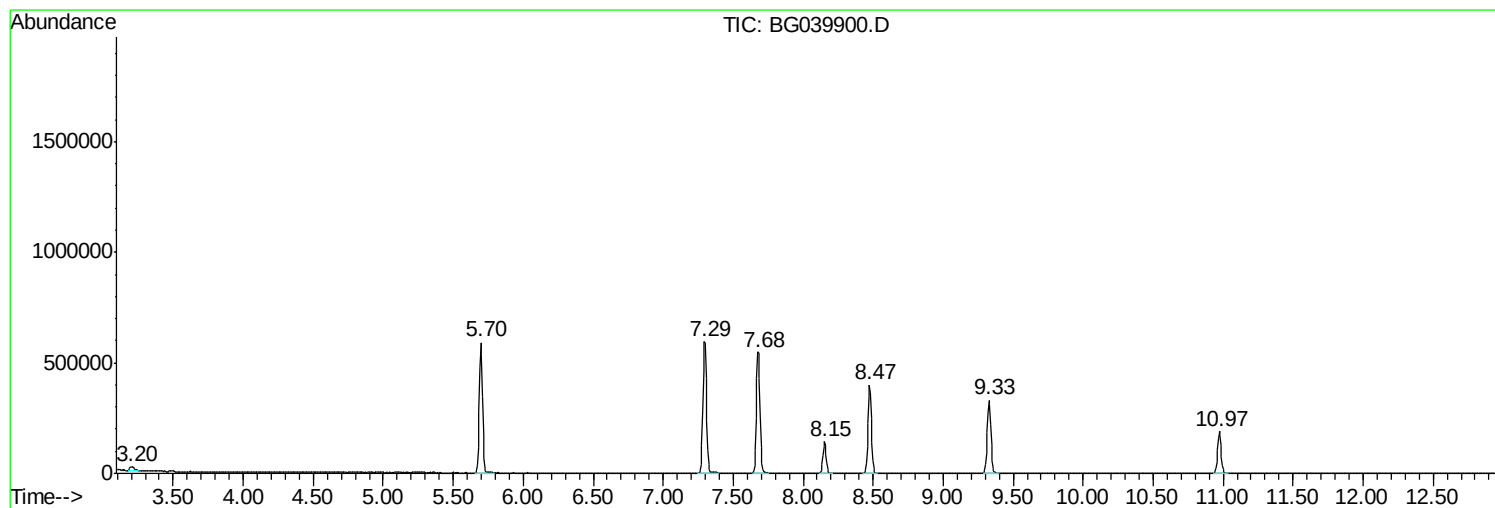

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG031219\
Data File : BG039900.D
Acq On : 13 Mar 2019 8:44
Operator : JU/SJ
Sample : PB117850BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB117850BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG030419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.68 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.68	80.97 ng	977321	1,4-Dichlorobenzene-d4	8.15

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	25
3		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	17
4		5-Aminoindole	132	C8H8N2	005192-03-0	12
5		Tranlycypromine-propionyl	189	C12H15NO	1000123-86-3	12

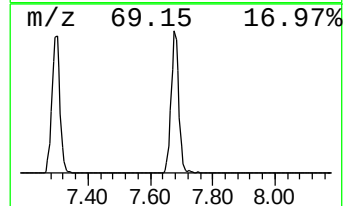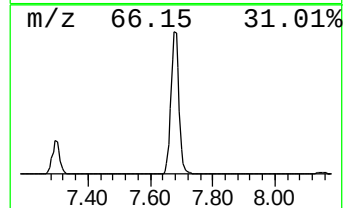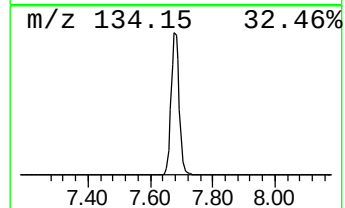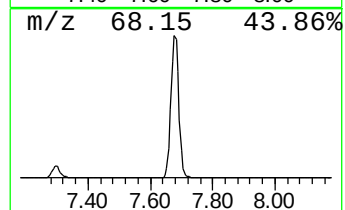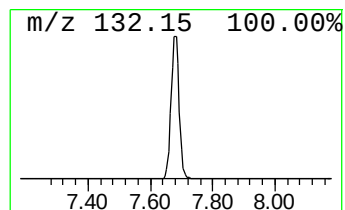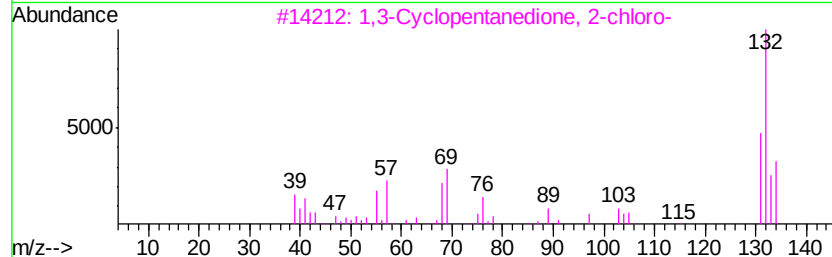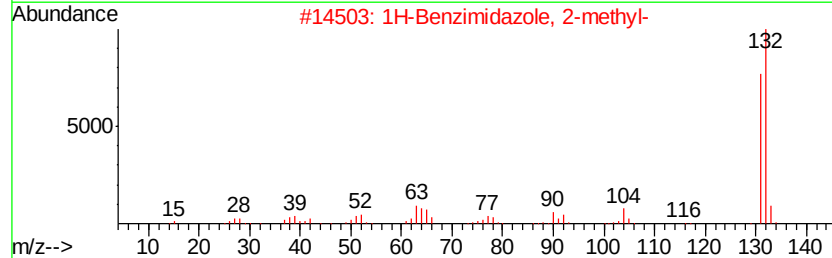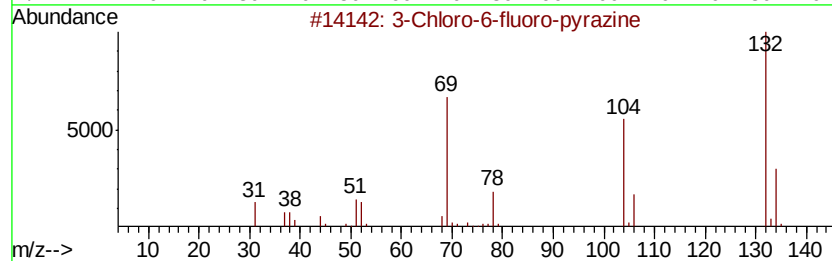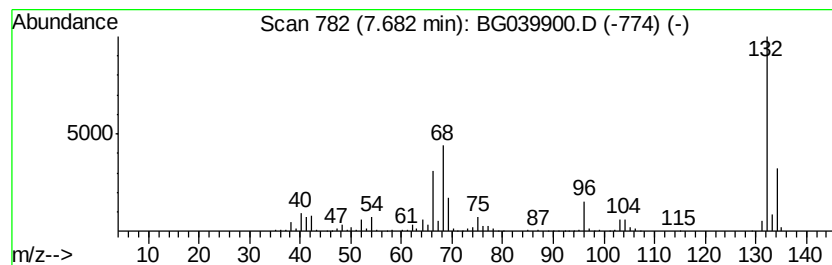

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG031219\
Data File : BG039900.D
Acq On : 13 Mar 2019 8:44
Operator : JU/SJ
Sample : PB117850BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB117850BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.68	7.68	81.0	ng	977321	1	8.15	241393	20.0