


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG031219\
 Data File : BG039888.D
 Acq On : 13 Mar 2019 00:50
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 04 14:38:15 2019

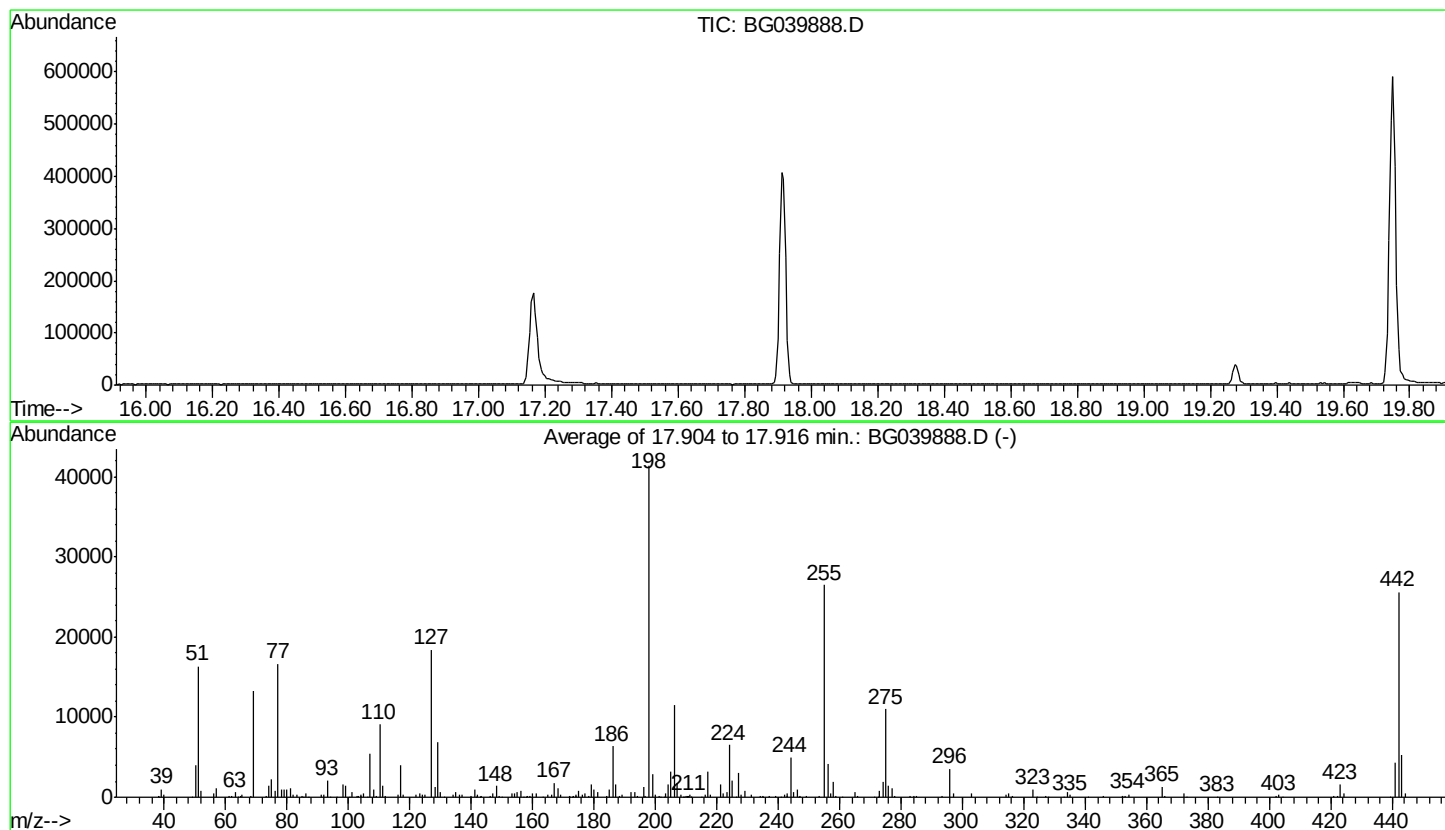

AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2516

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.4	16311	PASS
68	69	0.00	2	0.9	120	PASS
69	198	0.00	100	32.0	13252	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.5	18431	PASS
197	198	0.00	2	0.2	92	PASS
198	198	100	100	100.0	41408	PASS
199	198	5	9	7.0	2907	PASS
275	198	10	60	26.5	10969	PASS
365	198	1	100	3.1	1287	PASS
441	198	0.01	100	10.6	4390	PASS
442	198	50	100	61.9	25620	PASS
443	442	15	24	20.6	5283	PASS