
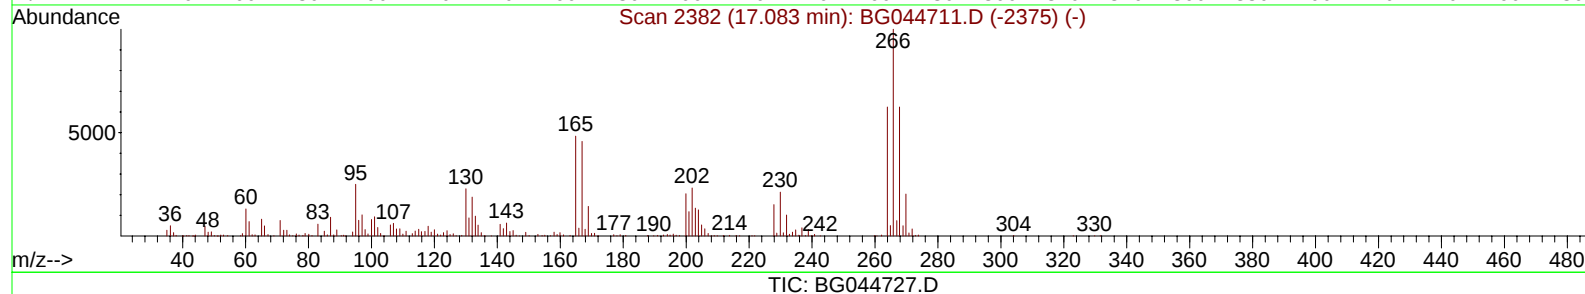
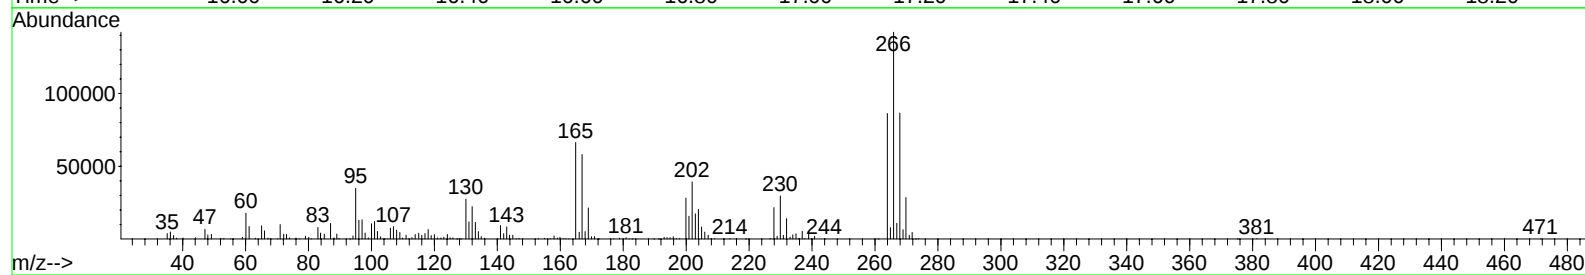


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG031220\
 Data File : BG044727.D
 Acq On : 12 Mar 2020 9:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 13 18:55:19 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG031020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 10 16:27:39 2020
 Response via : Initial Calibration

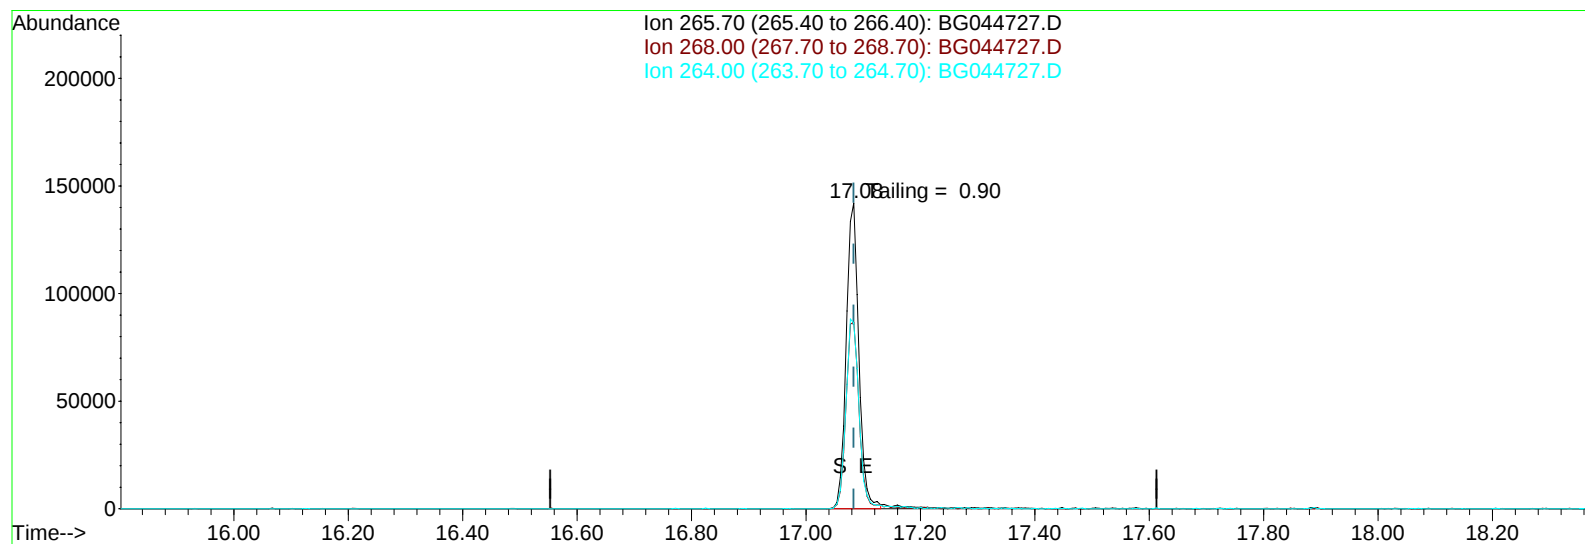

(70) Pentachlorophenol (C)




17.083min (+0.000) 507885.04ng

response 219822

Ion	Exp%	Act%
265.70	100	100
268.00	62.40	60.98
264.00	62.40	60.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG031220\
 Data File : BG044727.D
 Acq On : 12 Mar 2020 9:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 13 18:55:19 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG031020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 10 16:27:39 2020
 Response via : Initial Calibration

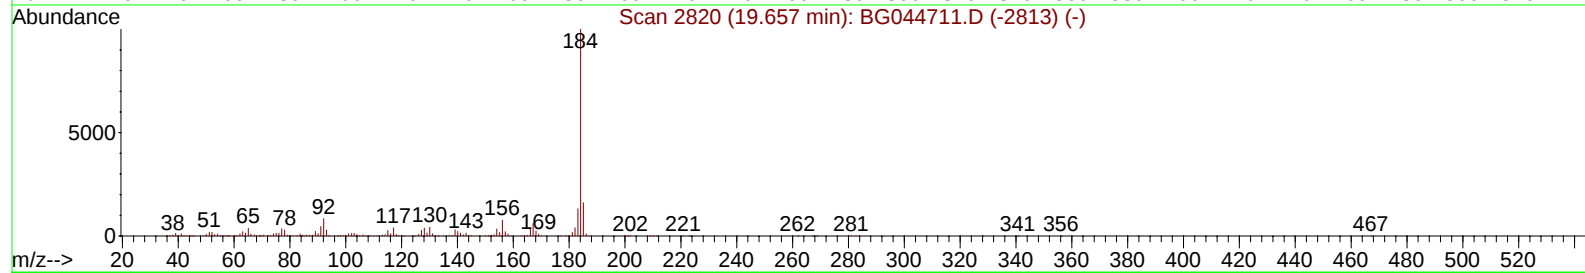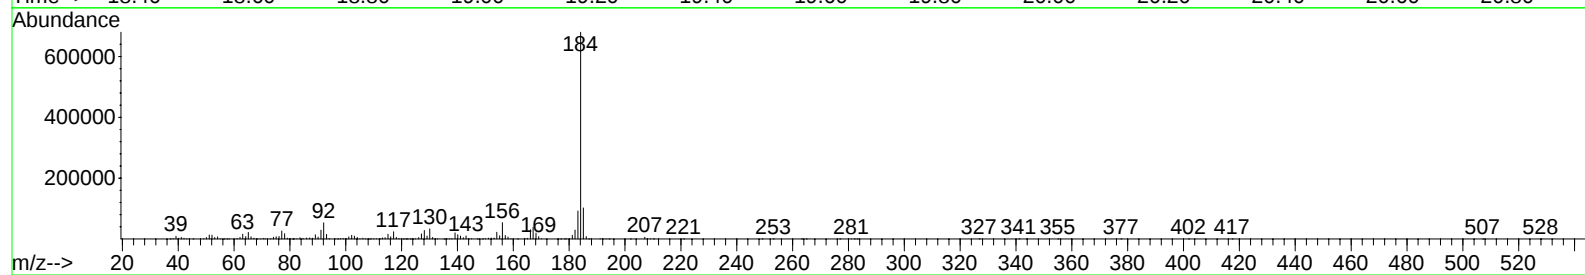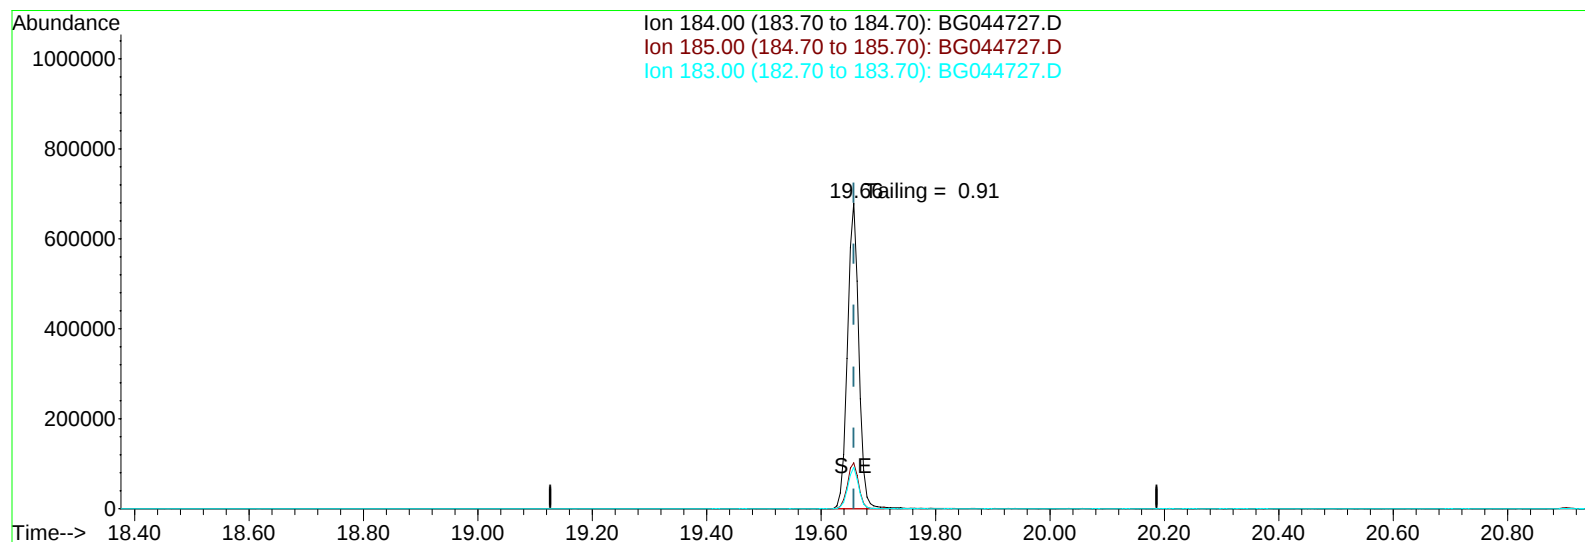

(77) Benzidine

19.657min (+0.000) 535202.18ng

response 938238

Ion	Exp%	Act%
184.00	100	100
185.00	16.10	15.02
183.00	13.20	13.57
0.00	0.00	0.00