
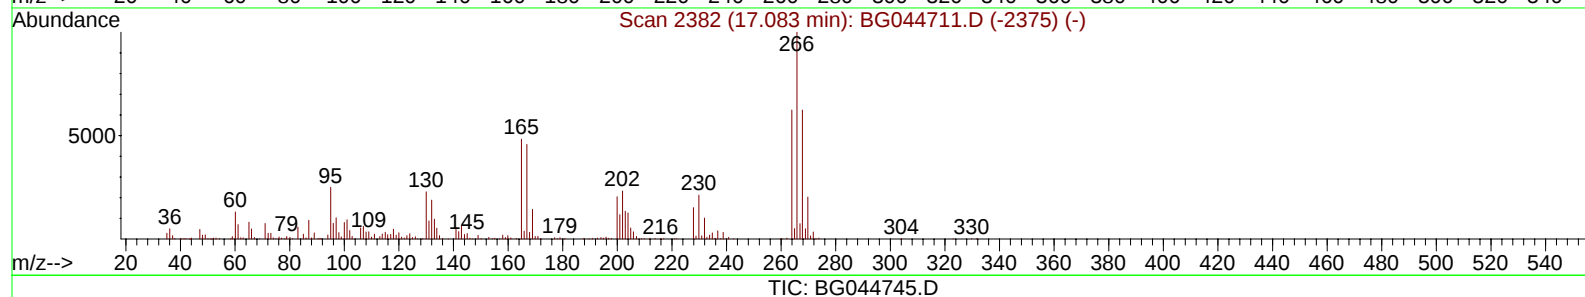
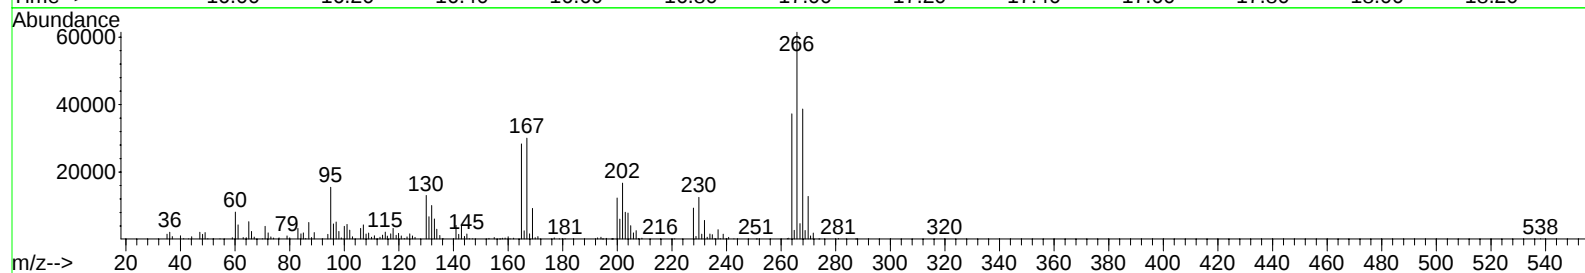


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG031220\
Data File : BG044745.D
Acq On : 12 Mar 2020 22:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 13 18:56:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG031020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 10 16:27:39 2020
Response via : Initial Calibration

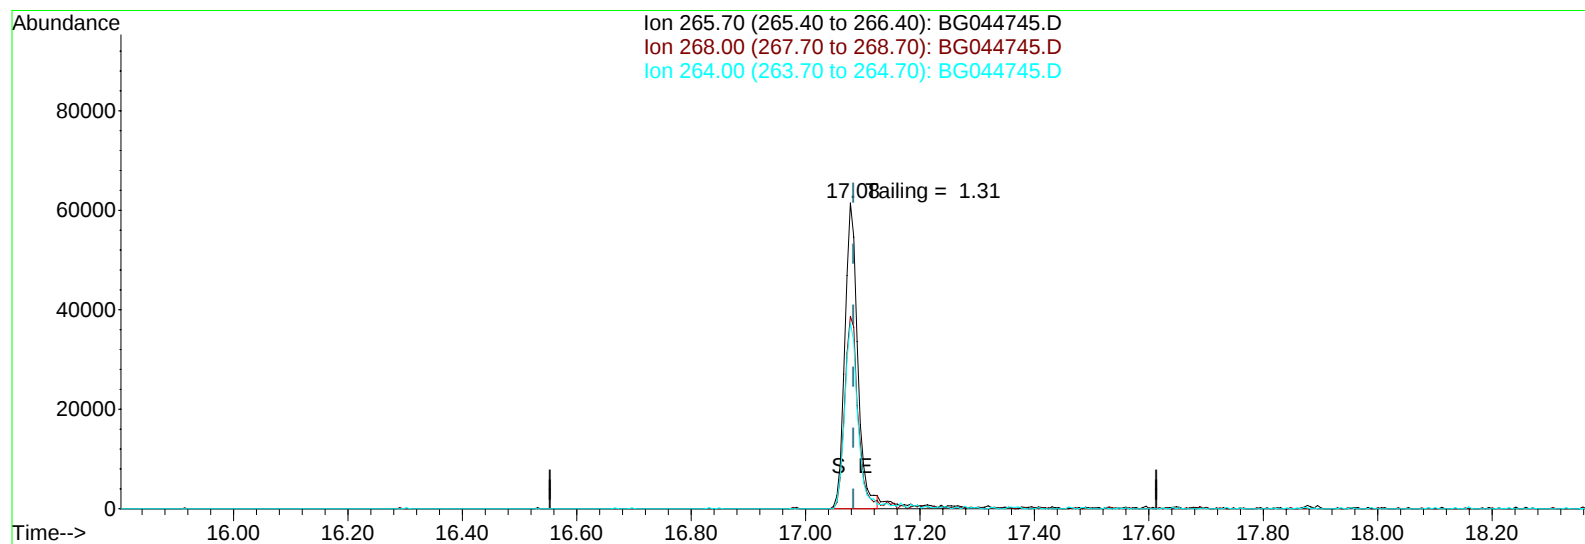

TIC: BG044745.D

(70) Pentachlorophenol (C)




17.078min (-0.005) 166575.40ng

response 99444

Ion	Exp%	Act%
265.70	100	100
268.00	62.40	62.97
264.00	62.40	60.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG031220\
 Data File : BG044745.D
 Acq On : 12 Mar 2020 22:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 13 18:56:46 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG031020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 10 16:27:39 2020
 Response via : Initial Calibration

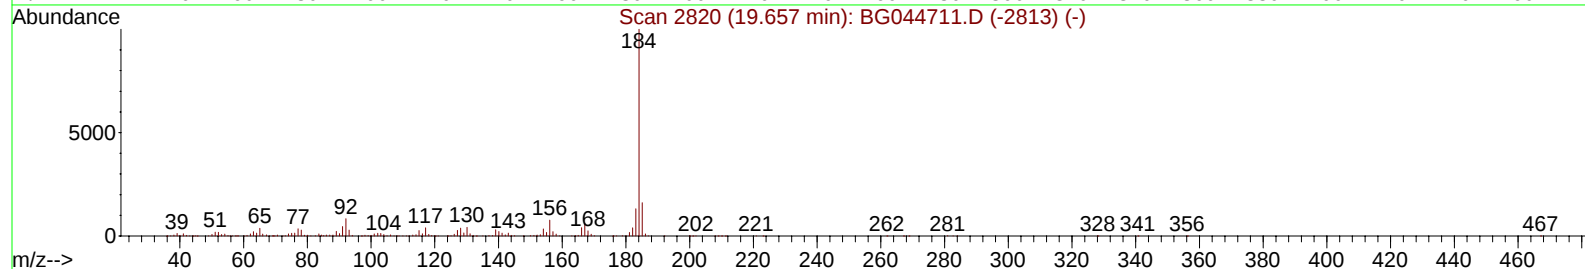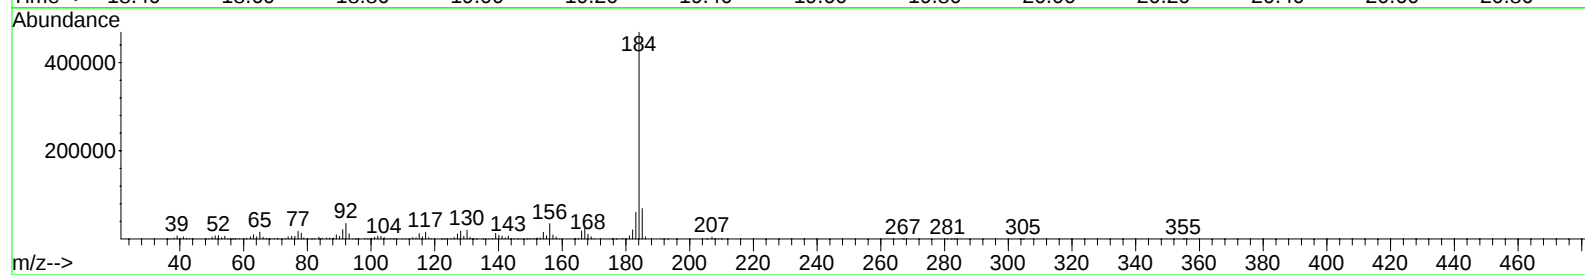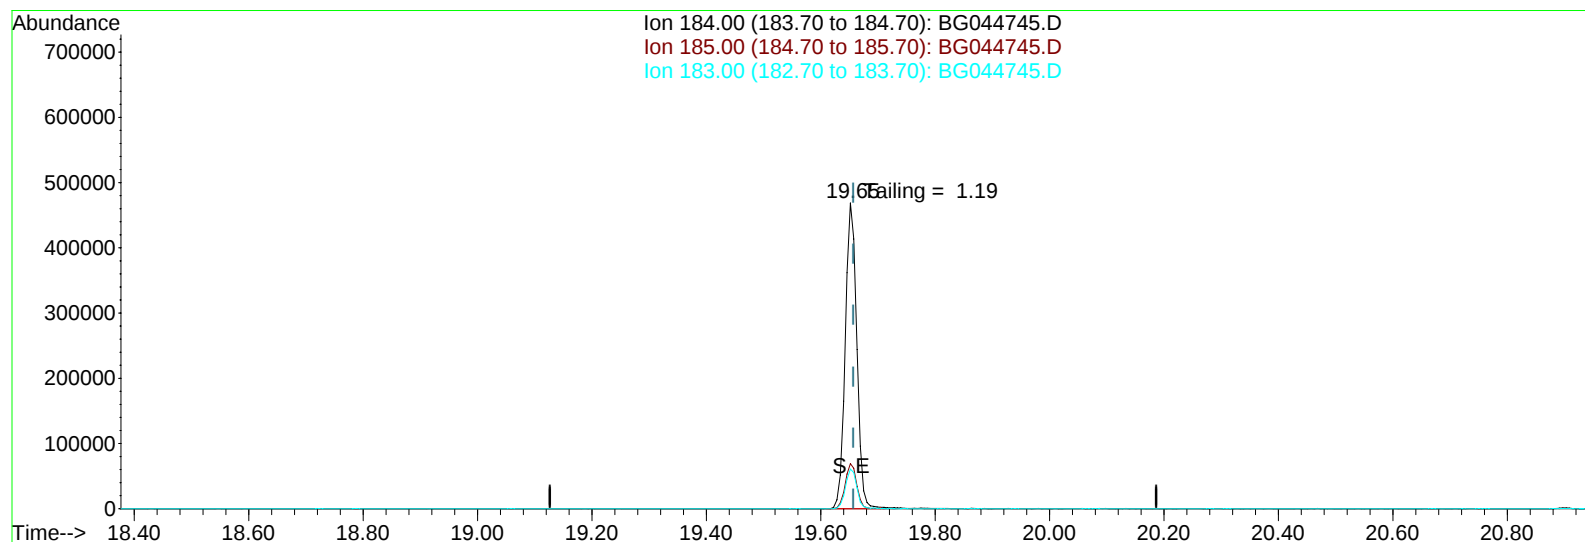

TIC: BG044745.D

(77) Benzidine

19.652min (-0.005) 364191.87ng

response 662094

Ion	Exp%	Act%
184.00	100	100
185.00	16.10	14.75
183.00	13.20	12.96
0.00	0.00	0.00