


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG031220\
 Data File : BG044727.D
 Acq On : 12 Mar 2020 9:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 10 16:27:39 2020

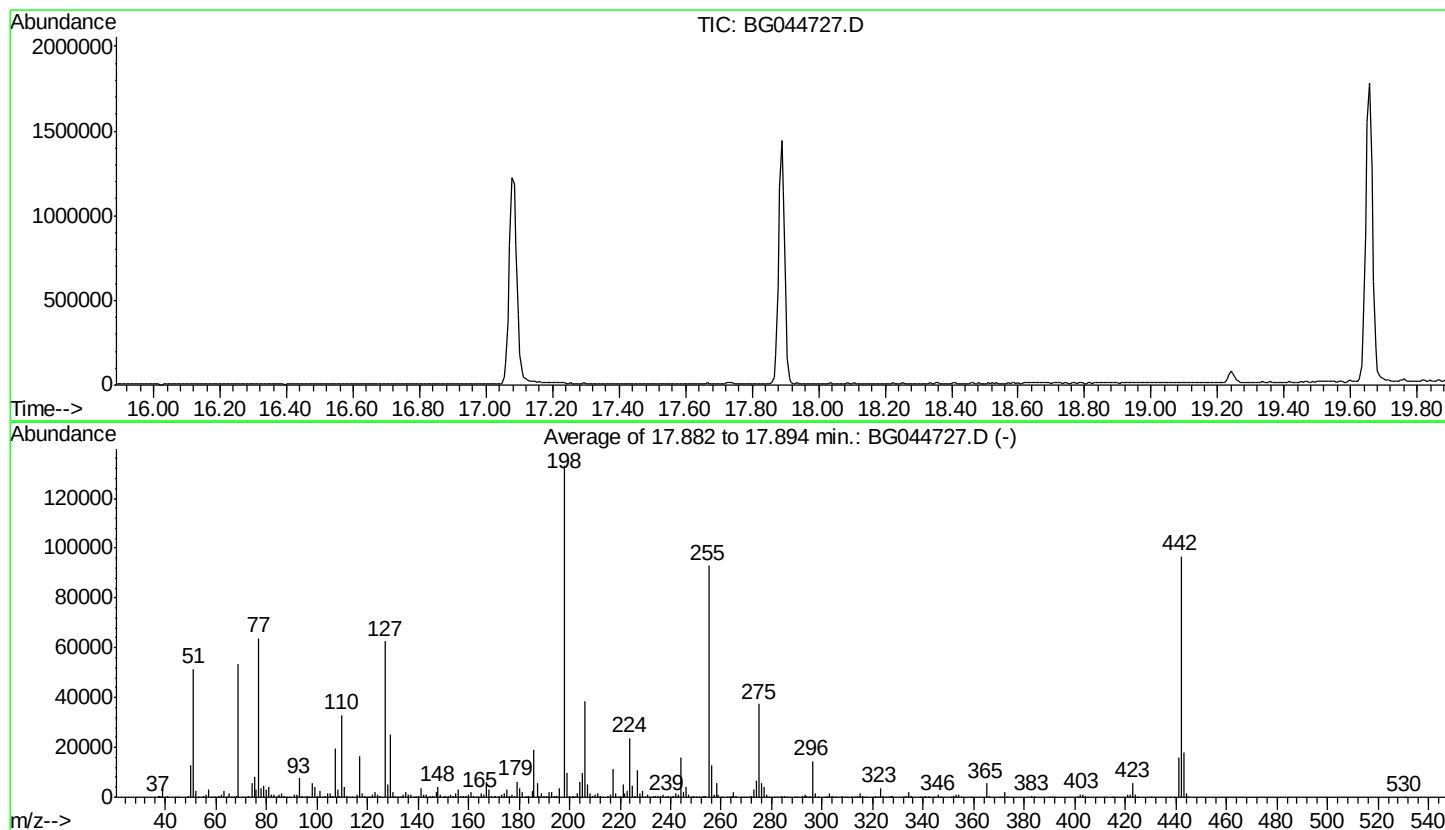

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2511

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	51610	PASS
68	69	0.00	2	0.7	348	PASS
69	198	0.00	100	40.1	53360	PASS
70	69	0.00	2	0.3	174	PASS
127	198	10	80	47.1	62653	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	133130	PASS
199	198	5	9	7.5	9978	PASS
275	198	10	60	28.2	37493	PASS
365	198	1	100	4.2	5529	PASS
441	198	0.01	100	12.0	15998	PASS
442	198	50	100	72.7	96762	PASS
443	442	15	24	18.7	18122	PASS