


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG031220\
 Data File : BG044745.D
 Acq On : 12 Mar 2020 22:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 10 16:27:39 2020

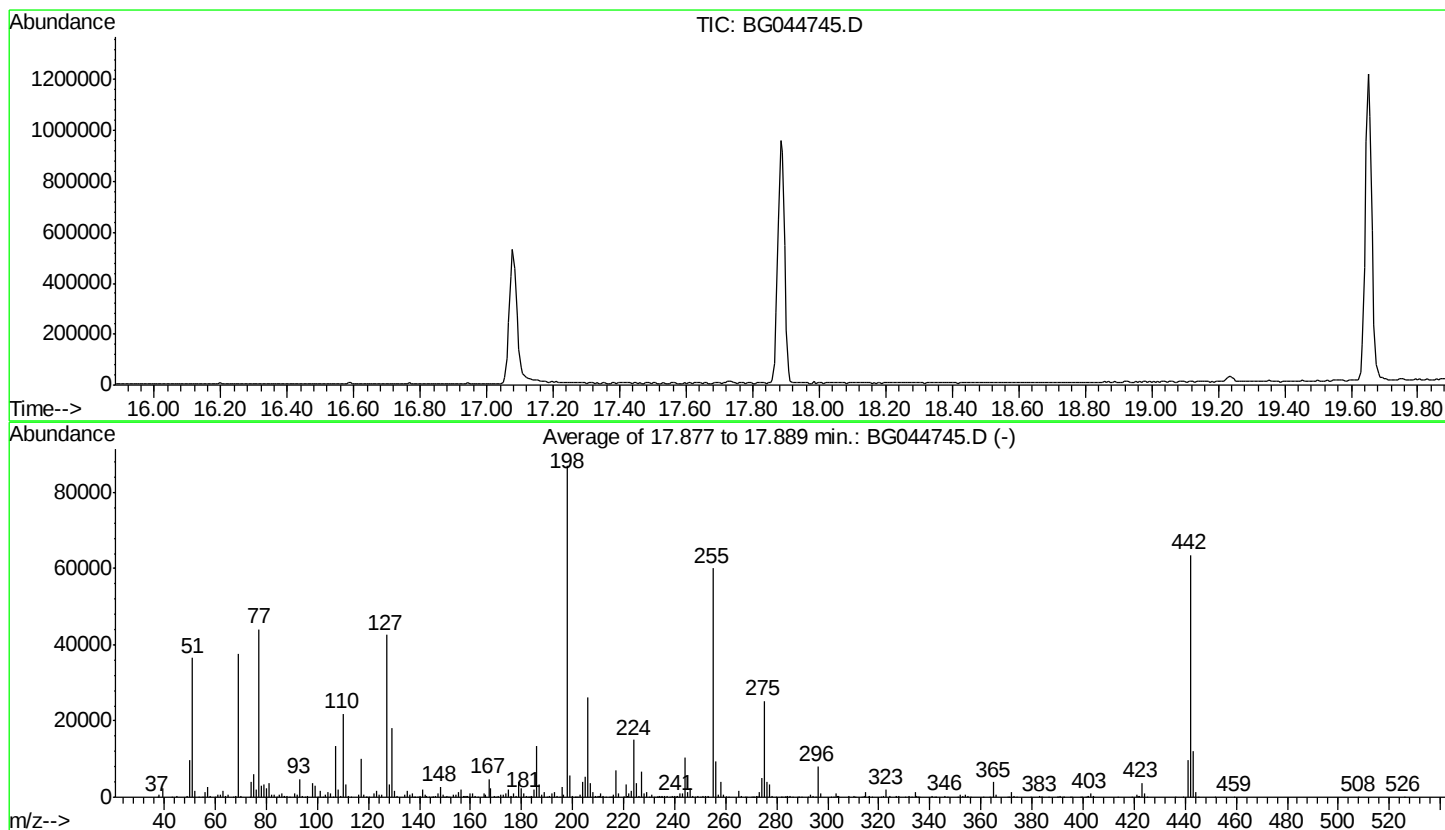

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2511

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.0	36552	PASS
68	69	0.00	2	0.6	220	PASS
69	198	0.00	100	43.1	37472	PASS
70	69	0.00	2	0.6	207	PASS
127	198	10	80	49.0	42610	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	87021	PASS
199	198	5	9	6.6	5702	PASS
275	198	10	60	29.0	25256	PASS
365	198	1	100	4.6	3964	PASS
441	198	0.01	100	11.1	9654	PASS
442	198	50	100	73.0	63504	PASS
443	442	15	24	19.3	12251	PASS