

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG031317\
 Data File : BG026222.D
 Acq On : 13 Mar 2017 21:46
 Operator : SJ/MA
 Sample : I2217-22
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CB2Z1

Quant Time: Mar 15 06:54:26 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG030317-PAH.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 15 06:53:58 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	83378	20.00	ng/ul	0.00
2) Naphthalene-d8	10.86	136	414953	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.66	164	255358	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.39	188	587278	20.00	ng/ul	0.00
18) Chrysene-d12	21.64	240	598825	20.00	ng/ul	0.00
23) Perylene-d12	24.82	264	578308	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 2,4-Dichlorophenol-d3	10.47	165	75729	12.32	ng/uL	0.00
7) Acenaphthylene-d8	14.35	160	451051	20.72	ng/ul	0.00
10) Fluorene-d10	15.64	176	328523	20.68	ng/ul	0.00
15) Anthracene-d10	17.49	188	467171	17.90	ng/ul	0.00
19) Pyrene-d10	19.76	212	512383	16.77	ng/ul	0.00
26) Benzo(a)pyrene-d12	24.60	264	459815	18.44	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
14) Phenanthrene	17.44	178	115038	3.70	ng/ul	98
17) Fluoranthene	19.43	202	196459	6.08	ng/ul	96
20) Pyrene	19.79	202	188184	4.94	ng/ul	99
21) Benzo(a)anthracene	21.61	228	110163	3.31	ng/ul	98
22) Chrysene	21.68	228	106206	3.42	ng/ul	97
24) Benzo(b)fluoranthene	23.87	252	42307	1.29	ng/ul	95
25) Benzo(k)fluoranthene	23.87	252	42418	1.35	ng/ul	96
27) Benzo(a)pyrene	24.67	252	100996	3.31	ng/ul	95
28) Indeno(1,2,3-cd)pyrene	28.44	276	71878	2.11	ng/ul	95
30) Benzo(g,h,i)perylene	29.56	276	30163	1.04	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG031317\
Data File : BG026222.D
Acq On : 13 Mar 2017 21:46
Operator : SJ/MA
Sample : I2217-22
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CB2Z1

Quant Time: Mar 15 06:54:26 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG030317-PAH.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 15 06:53:58 2017
Response via : Initial Calibration

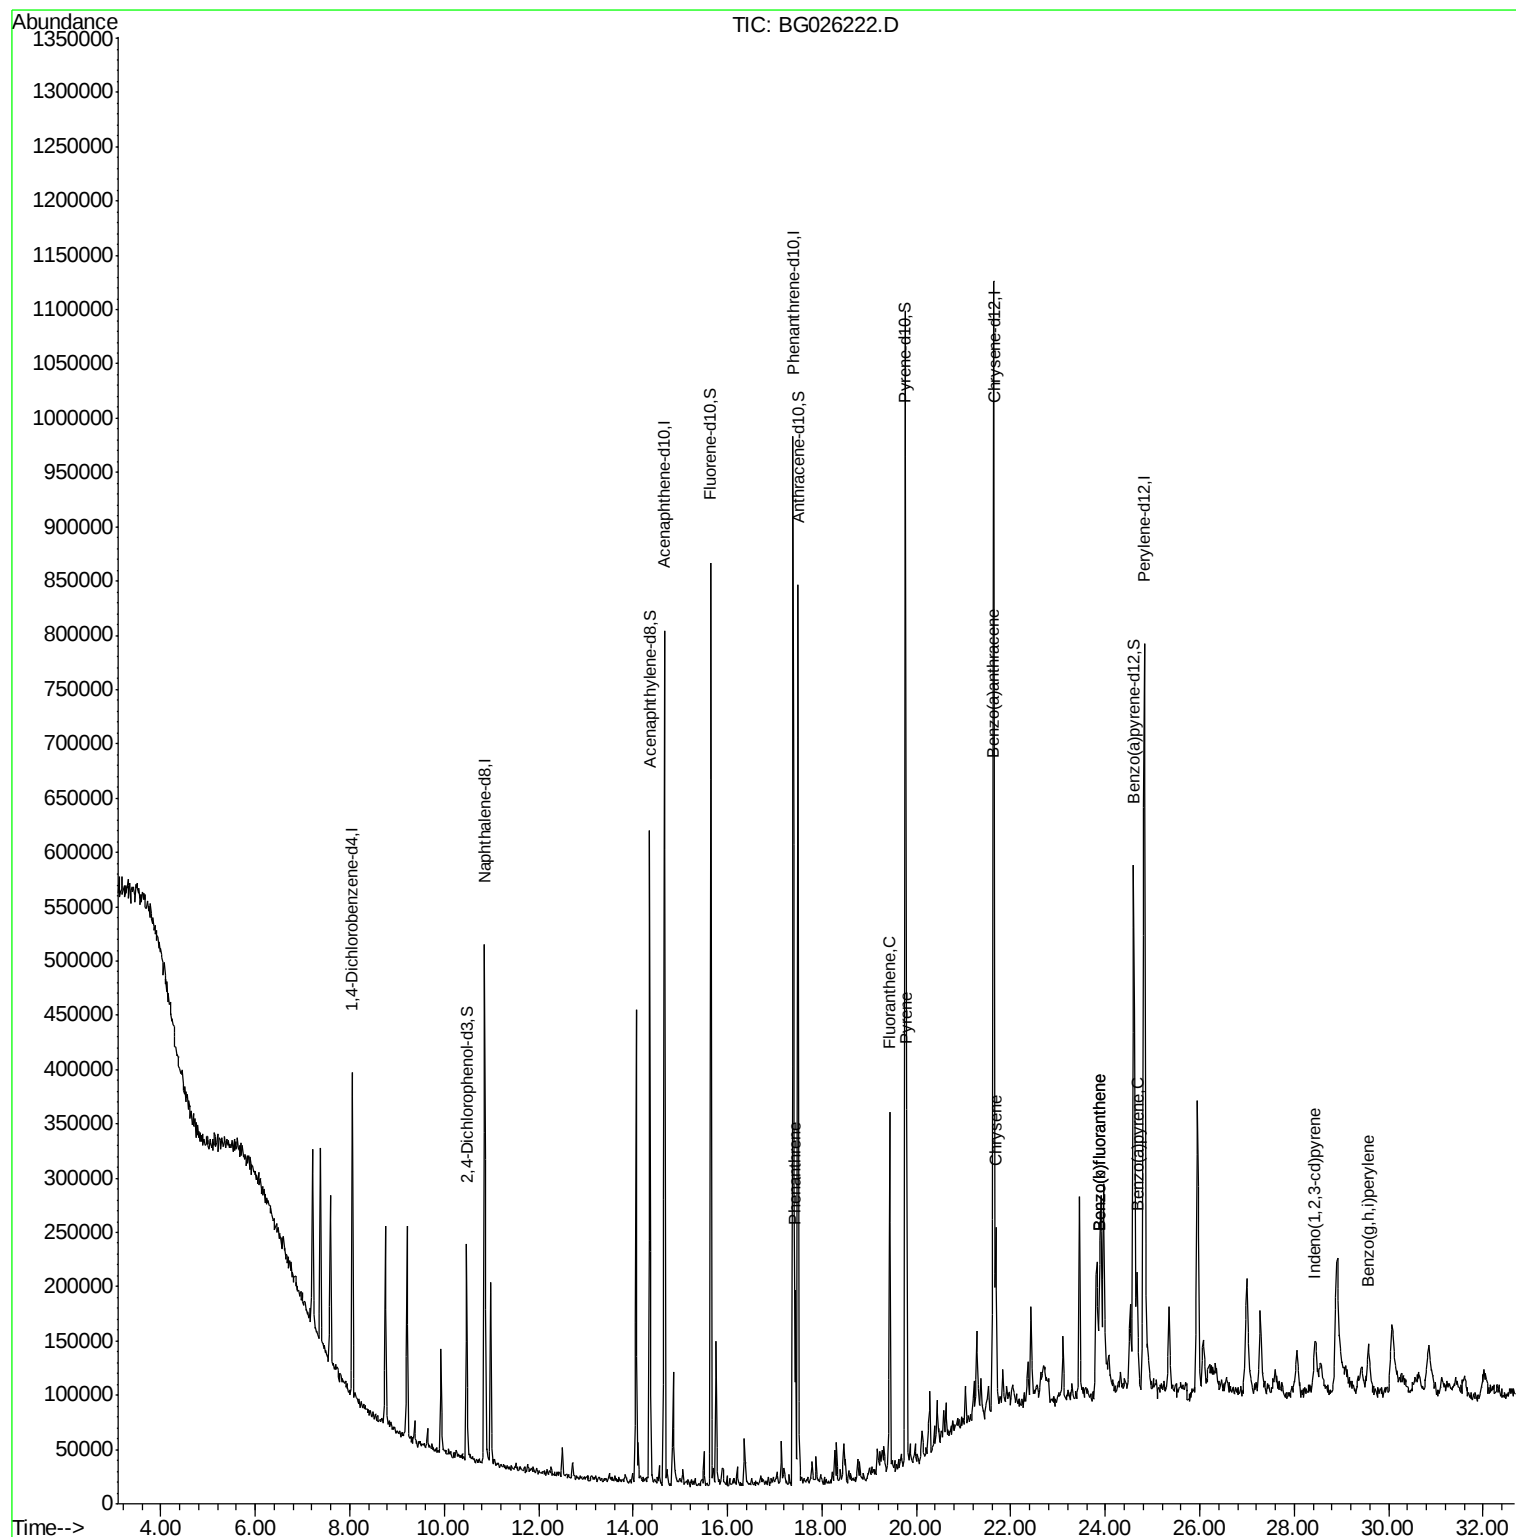

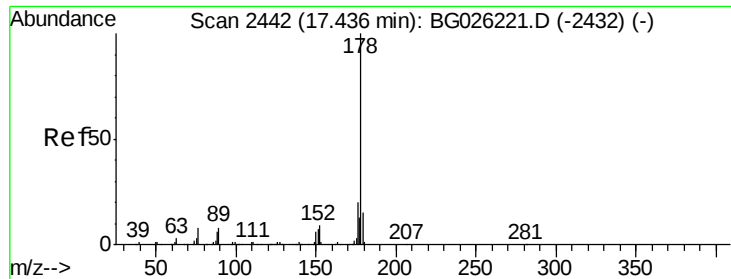

#14

Phenanthrene

Concen: 3.70 ng/ul

RT: 17.44 min Scan# 2442

Delta R.T. 0.00 min

Lab File: BG026222.D

Acq: 13 Mar 2017 21:46

Instrument :

BNA_G

ClientSampleId :

CB2Z1


Tgt Ion:178 Resp: 115038

Ion Ratio Lower Upper

178 100

179 14.3 12.2 18.4


176 19.7 16.4 24.6

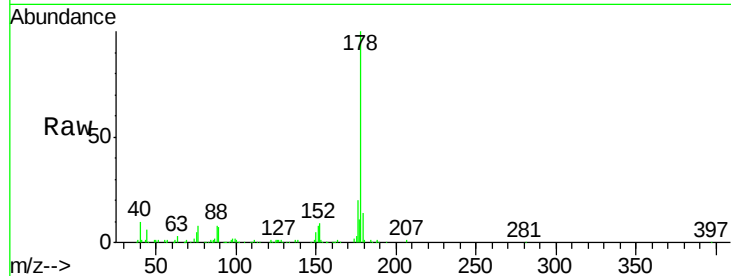



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

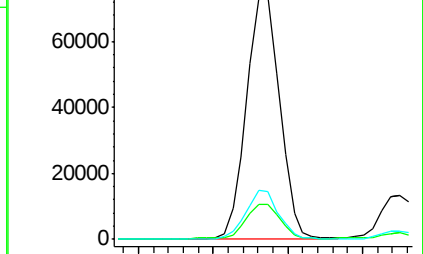

Time-->



#17

Fluoranthene

Concen: 6.08 ng/ul

RT: 19.43 min Scan# 2782

Delta R.T. 0.00 min

Lab File: BG026222.D

Acq: 13 Mar 2017 21:46


Tgt Ion:202 Resp: 196459

Ion Ratio Lower Upper

202 100

101 10.0 9.8 14.8


100 8.6 7.5 11.3




Abundance Ion 202.00 (201.70 to 202.70): E


Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

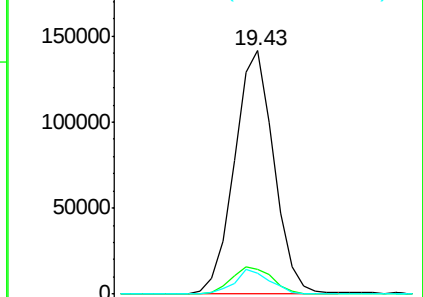

Time-->









#20
 Pyrene
 Concen: 4.94 ng/ul
 RT: 19.79 min Scan# 2843
 Delta R.T. 0.00 min
 Lab File: BG026222.D
 Acq: 13 Mar 2017 21:46




Instrument :
 BNA_G
 ClientSampleId :
 CB2Z1


Tgt Ion	Ratio	Lower	Upper
202	100		
101	13.6	11.2	16.8
100	11.4	9.8	14.6

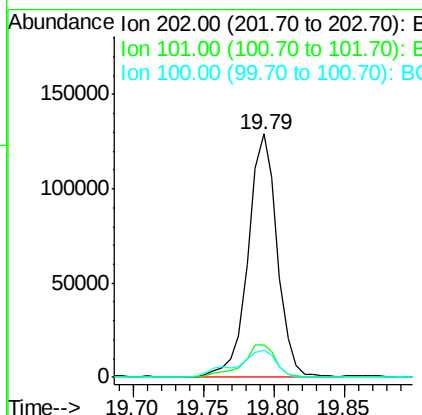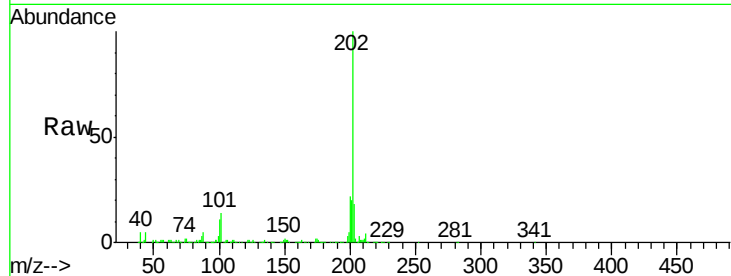

#21
 Benzo(a)anthracene
 Concen: 3.31 ng/ul
 RT: 21.61 min Scan# 3153
 Delta R.T. -0.01 min
 Lab File: BG026222.D
 Acq: 13 Mar 2017 21:46

Tgt Ion	Ratio	Lower	Upper
228	100		
229	19.0	15.9	23.9
226	28.5	22.1	33.1

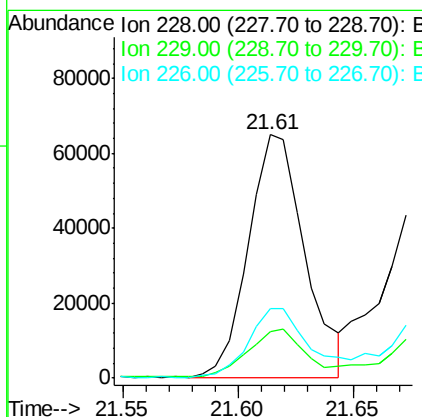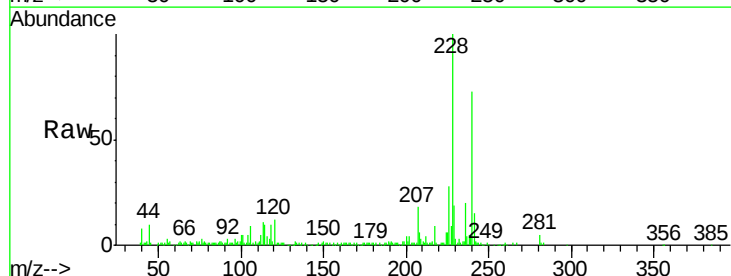



#22

Chrysene

Concen: 3.42 ng/ul

RT: 21.68 min Scan# 3164

Delta R.T. -0.01 min

Lab File: BG026222.D

Acq: 13 Mar 2017 21:46

Instrument :

BNA_G

ClientSampleId :

CB2Z1


Tgt Ion:228 Resp: 106206

Ion Ratio Lower Upper

228 100

226 29.6 25.0 37.6




229 19.6 16.6 25.0



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

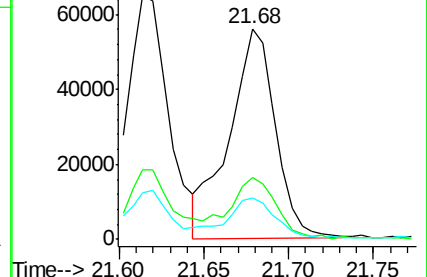

#24

Benzo(b)fluoranthene

Concen: 1.29 ng/ul

RT: 23.87 min Scan# 3537

Delta R.T. 0.06 min

Lab File: BG026222.D

Acq: 13 Mar 2017 21:46


Tgt Ion:252 Resp: 42307

Ion Ratio Lower Upper

252 100

253 19.0 17.8 26.6



125 11.3 9.4 14.0




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

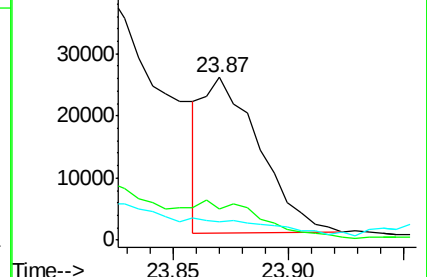



#25

Benzo(k)fluoranthene

Concen: 1.35 ng/ul

RT: 23.87 min Scan# 3537

Delta R.T. -0.01 min

Lab File: BG026222.D

Acq: 13 Mar 2017 21:46

Instrument :

BNA_G

ClientSampleId :

CB2Z1


Tgt Ion:252 Resp: 42418

Ion Ratio Lower Upper

252 100

253 19.0 17.4 26.2




125 11.3 8.8 13.2



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

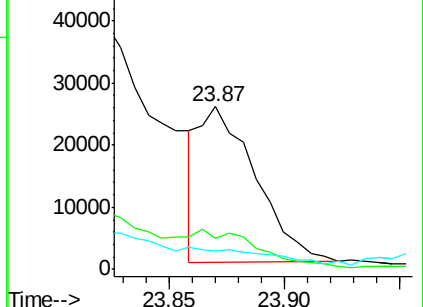

#27

Benzo(a)pyrene

Concen: 3.31 ng/ul

RT: 24.67 min Scan# 3673

Delta R.T. -0.01 min

Lab File: BG026222.D

Acq: 13 Mar 2017 21:46


Tgt Ion:252 Resp: 100996

Ion Ratio Lower Upper

252 100

253 18.6 17.1 25.7



125 13.1 9.4 14.2




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

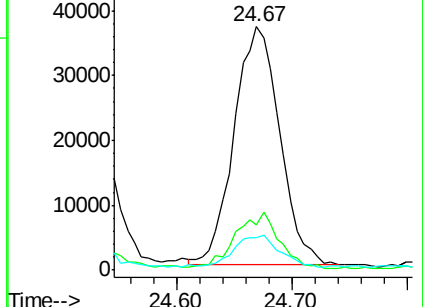

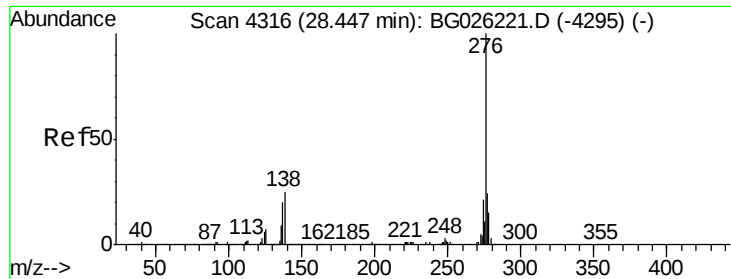

#28

Indeno(1,2,3-cd)pyrene

Concen: 2.11 ng/ul

RT: 28.44 min Scan# 4314

Delta R.T. -0.01 min

Lab File: BG026222.D

Acq: 13 Mar 2017 21:46

Instrument :

BNA_G

ClientSampleId :

CB2Z1


Tgt Ion:276 Resp: 71878

Ion Ratio Lower Upper

276 100

138 25.2 17.8 26.6




277 22.7 19.4 29.0

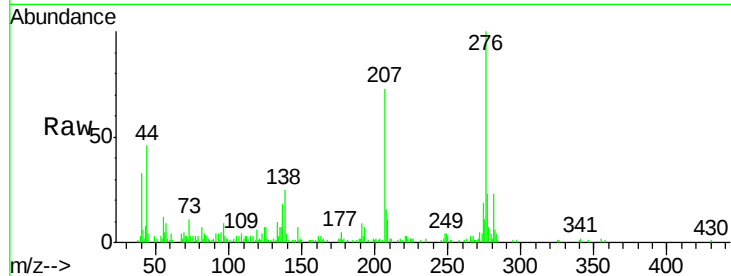

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

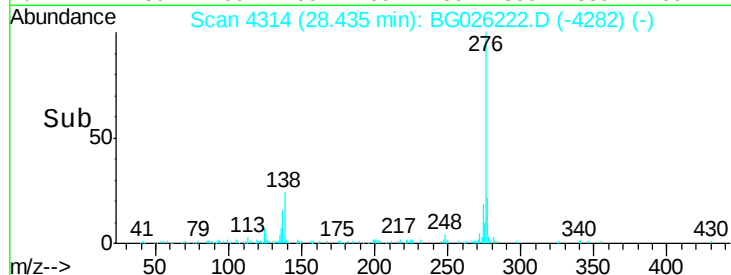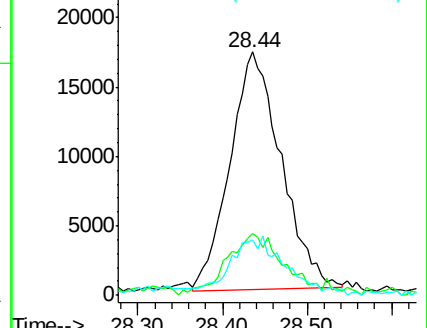

#30

Benzo(g,h,i)perylene

Concen: 1.04 ng/ul

RT: 29.56 min Scan# 4505

Delta R.T. -0.02 min

Lab File: BG026222.D

Acq: 13 Mar 2017 21:46


Tgt Ion:276 Resp: 30163

Ion Ratio Lower Upper

276 100

138 22.6 19.0 28.4

277 25.2 19.7 29.5



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

