


Data Path : Z:\HPCHEM1\BNA G\Data\BG031318\
 Data File : BG033114.D
 Acq On : 13 Mar 2018 10:50
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 14 13:59:34 2018

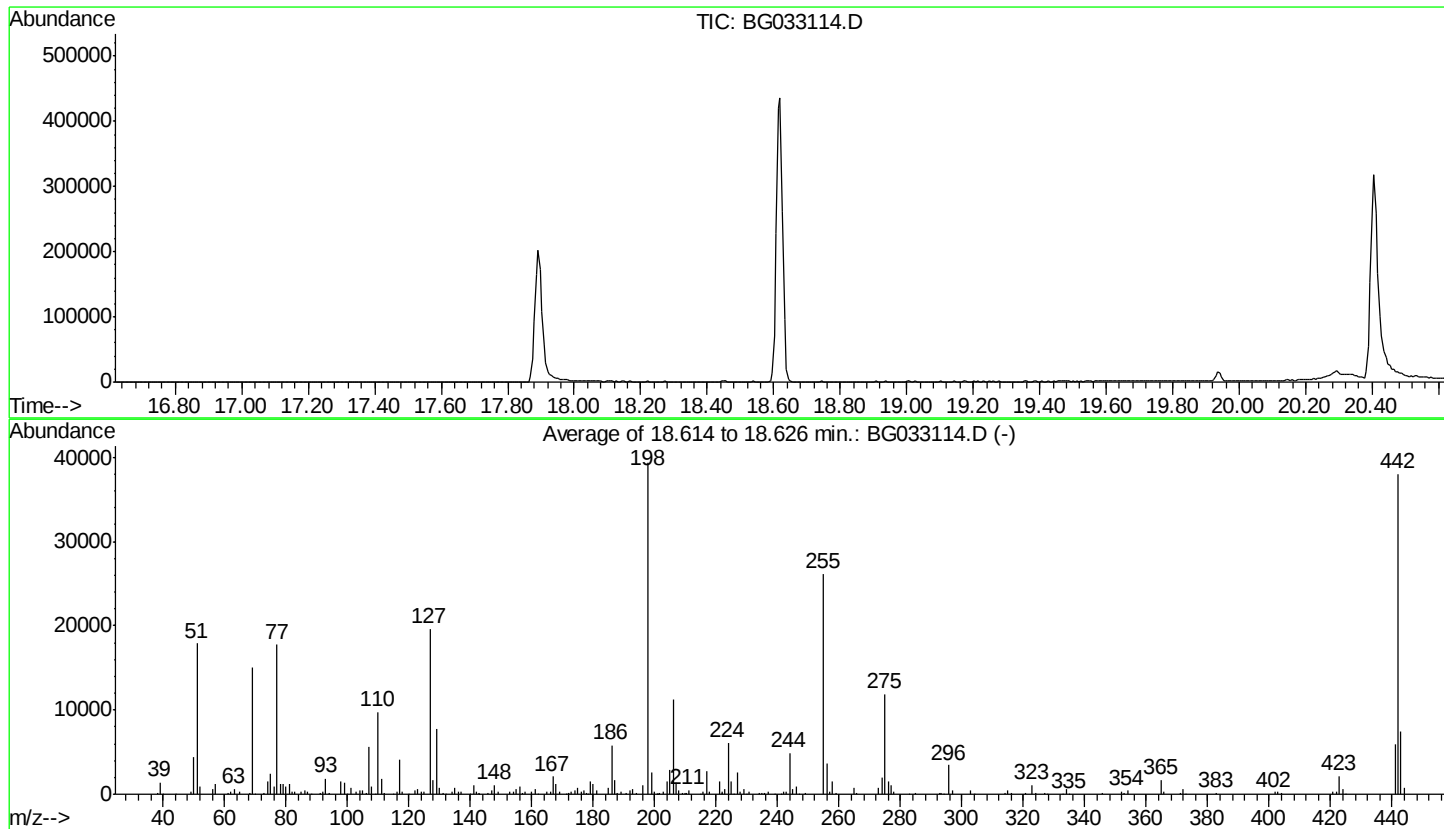

AutoFind: Scans 2609, 2610, 2611; Background Corrected with Scan 2602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.5	17915	PASS
68	69	0.00	2	0.7	98	PASS
69	198	0.00	100	38.1	15009	PASS
70	69	0.00	2	0.4	60	PASS
127	198	10	80	49.9	19624	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	39360	PASS
199	198	5	9	6.6	2598	PASS
275	198	10	60	30.1	11866	PASS
365	198	1	100	4.4	1742	PASS
441	442	0.01	24	15.8	5991	PASS
442	198	50	100	96.6	38013	PASS
443	442	15	24	19.7	7474	PASS