
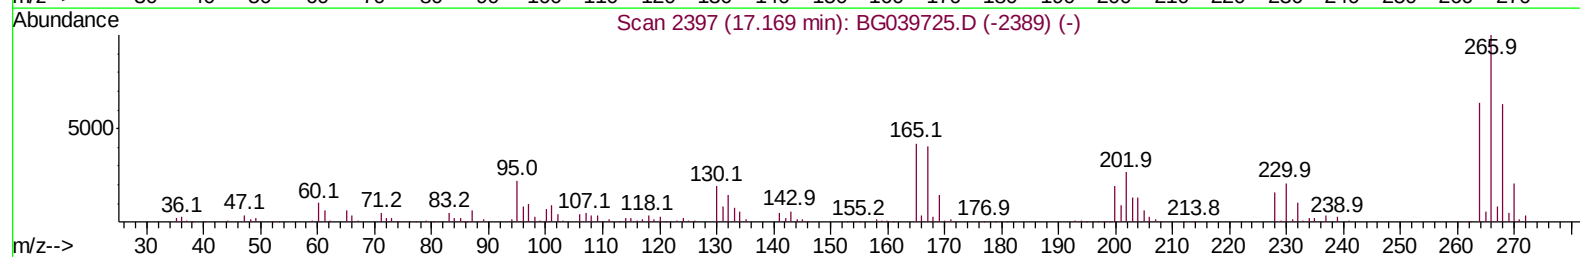
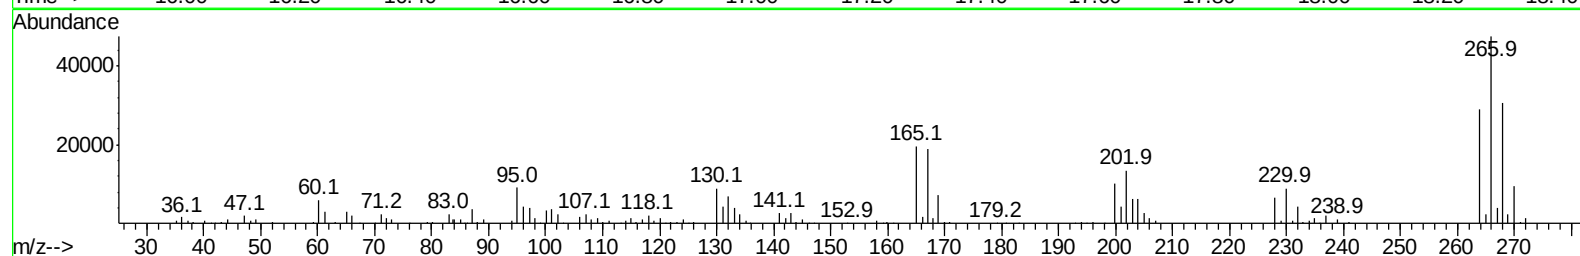


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG031319\
Data File : BG039904.D
Acq On : 13 Mar 2019 16:06
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 14 05:06:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG030419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 04 14:38:15 2019
Response via : Initial Calibration

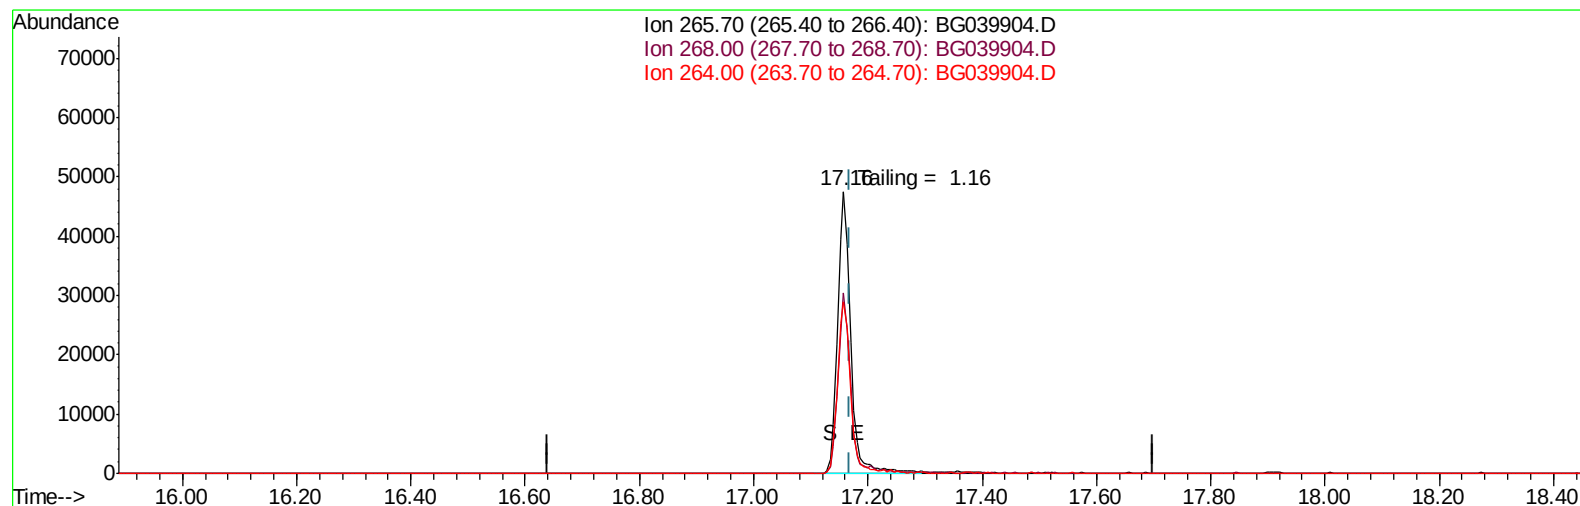

TIC: BG039904.D

(70) Pentachlorophenol (C)




17.158min (-0.012) 28472.88ng

response 73650

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.24
264.00	65.10	60.94
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG031319\
 Data File : BG039904.D
 Acq On : 13 Mar 2019 16:06
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 14 05:06:06 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG030419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 04 14:38:15 2019
 Response via : Initial Calibration

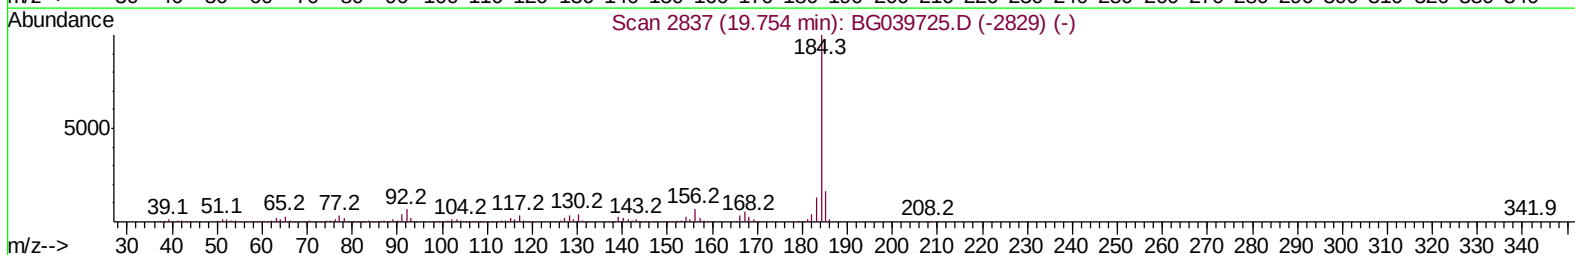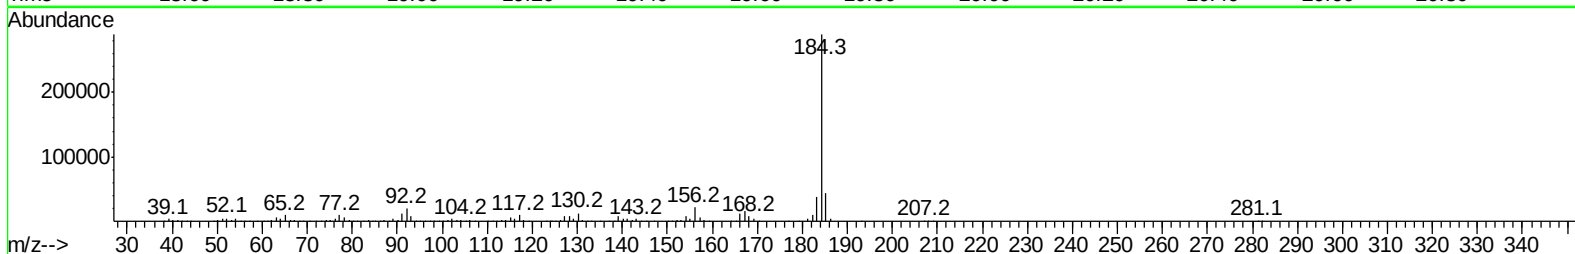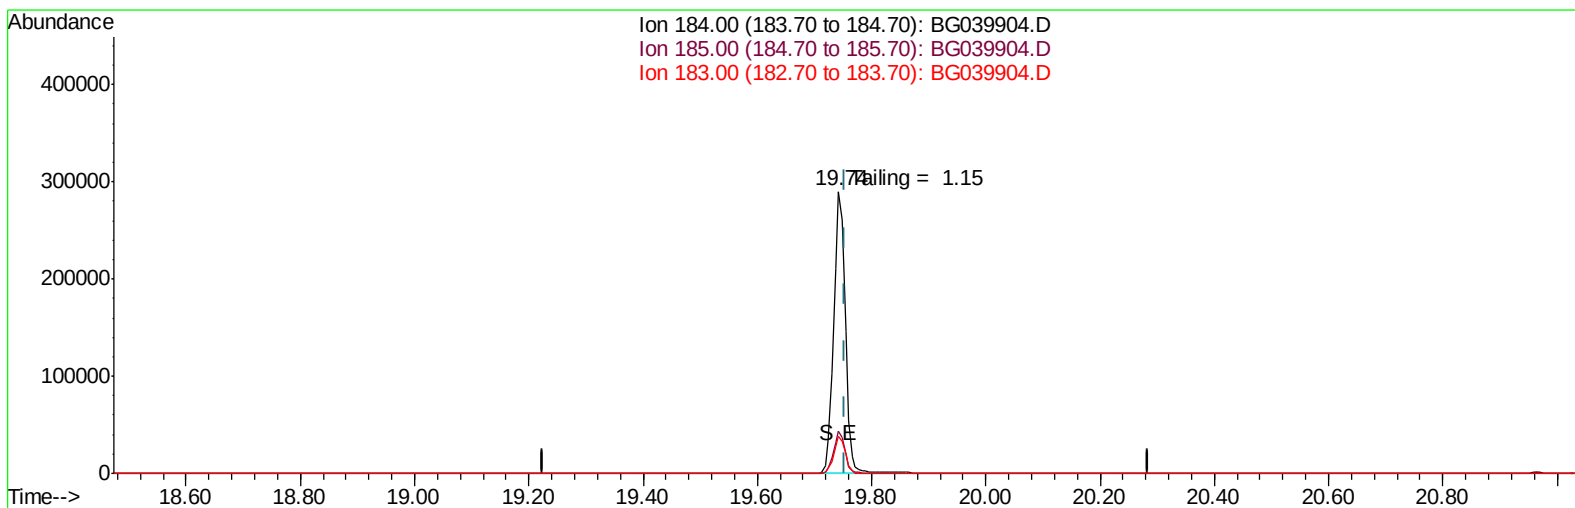

TIC: BG039904.D

(77) Benzidine

19.742min (-0.012) 37661.15ng

response 408724

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.88
183.00	13.20	13.20
0.00	0.00	0.00