

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG031319\
 Data File : BG039907.D
 Acq On : 13 Mar 2019 18:04
 Operator : JU/SJ
 Sample : PB117884BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB117884BL

Quant Time: Mar 14 04:31:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG030419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 04 14:38:15 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.14	152	38349	20.00	ng	-0.03
21) Naphthalene-d8	10.97	136	156805	20.00	ng	-0.02
39) Acenaphthene-d10	14.77	164	104018	20.00	ng	-0.02
64) Phenanthrene-d10	17.51	188	266888	20.00	ng	-0.02
76) Chrysene-d12	21.80	240	302315	20.00	ng	-0.03
87) Perylene-d12	25.16	264	300002	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.69	112	271136	120.62	ng	-0.02
7) Phenol-d6	7.29	99	377551	112.64	ng	-0.02
23) Nitrobenzene-d5	9.32	82	225606	77.81	ng	-0.02
42) 2,4,6-Tribromophenol	16.26	330	151996	125.37	ng	-0.02
45) 2-Fluorobiphenyl	13.40	172	570387	78.08	ng	-0.02
79) Terphenyl-d14	20.11	244	1028612	74.92	ng	-0.01


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG031319\
Data File : BG039907.D
Acq On : 13 Mar 2019 18:04
Operator : JU/SJ
Sample : PB117884BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB117884BL

Quant Time: Mar 14 04:31:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG030419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 04 14:38:15 2019
Response via : Initial Calibration

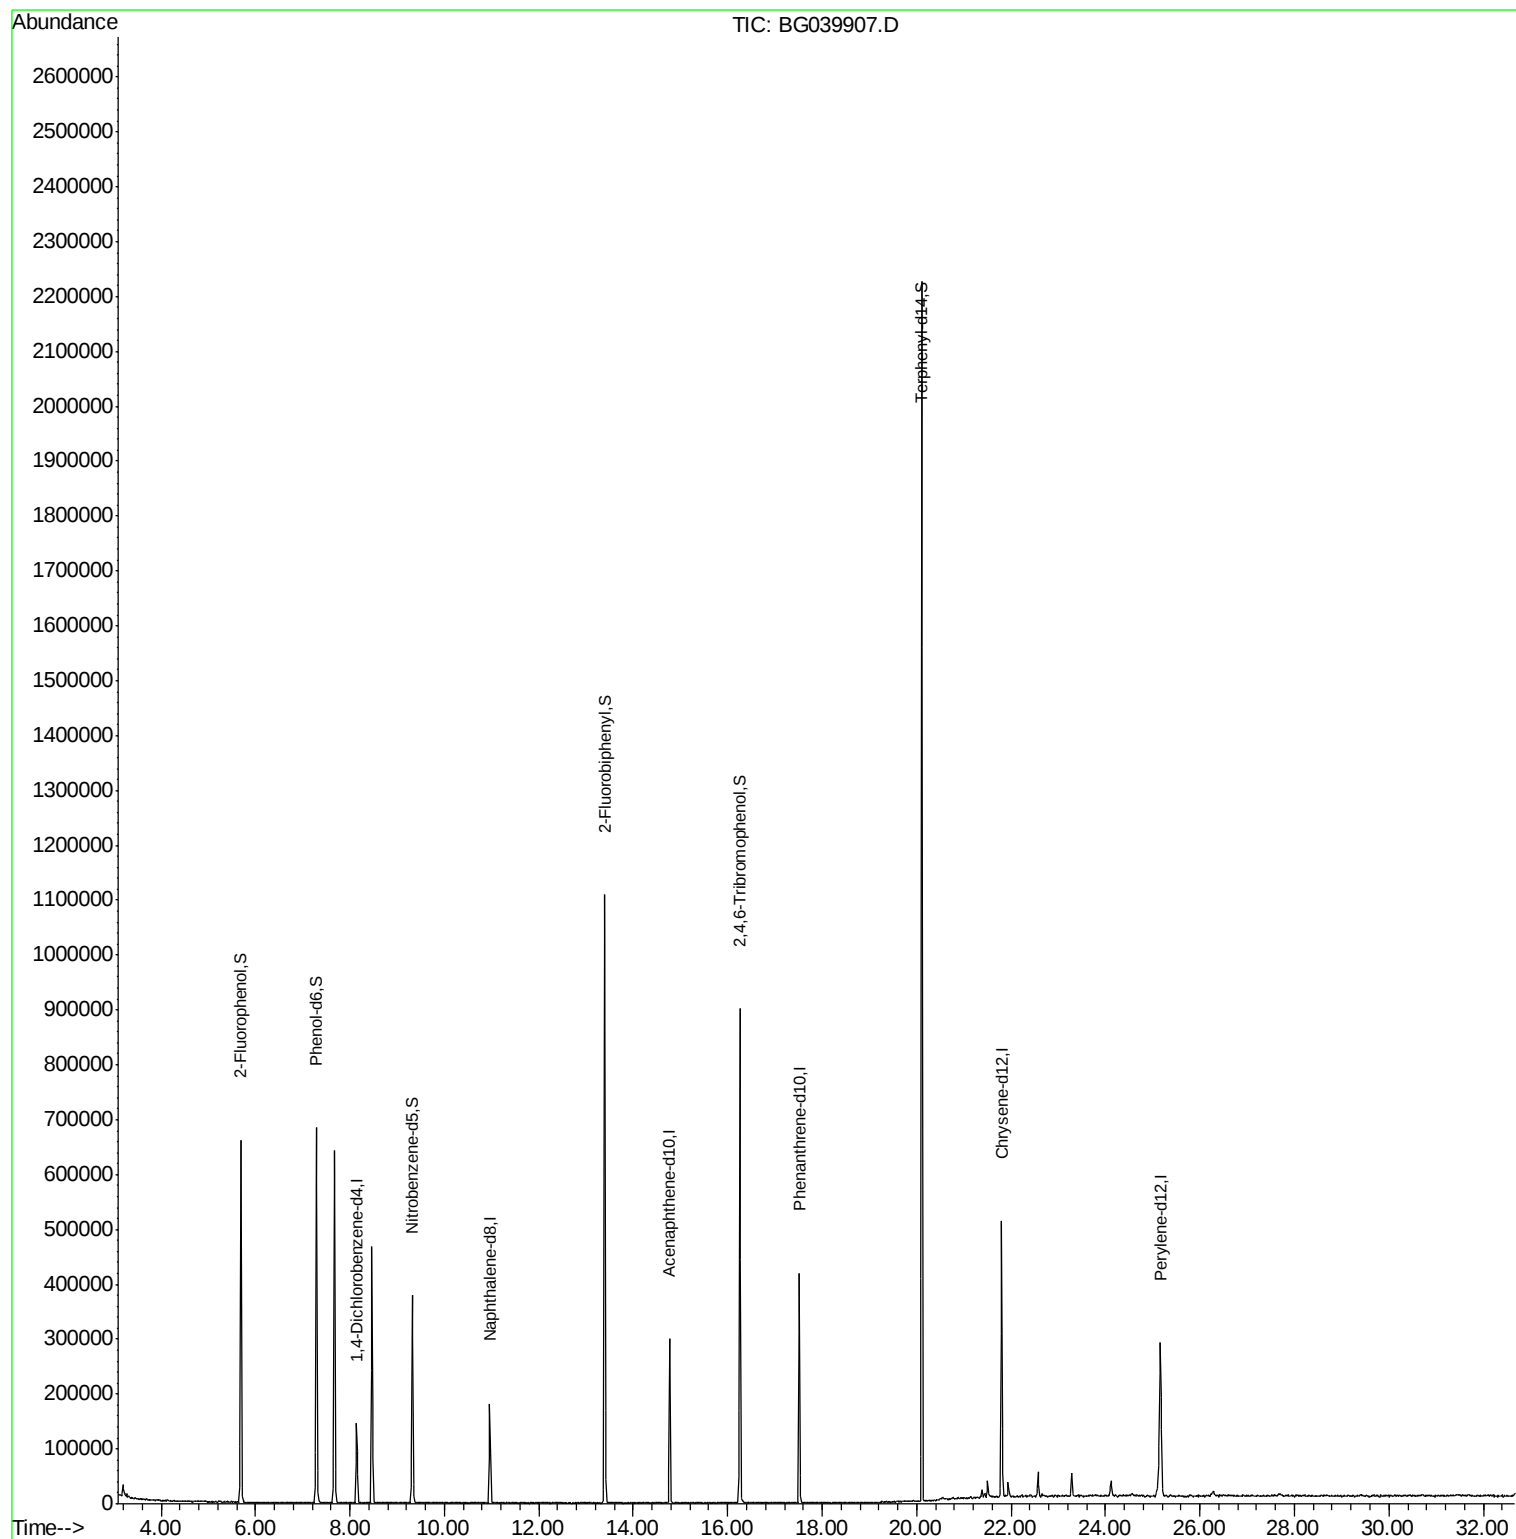




#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.14 min Scan# 861
Delta R.T. -0.03 min
Lab File: BG039907.D
Acq: 13 Mar 2019 18:04

Instrument :
BNA_G
ClientSampleId :
PB117884BL

Tot Ion	Ratio	Lower	Upper
152	100		
150	162.2	123.7	185.5
115	63.5	45.9	68.9



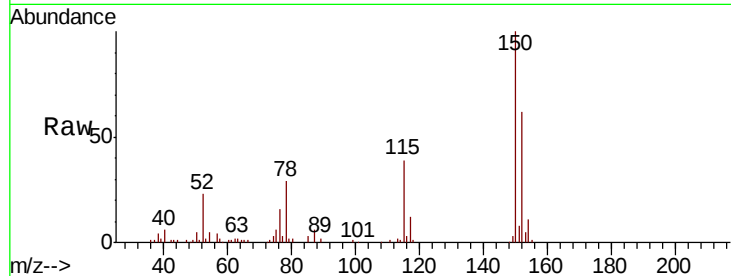


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

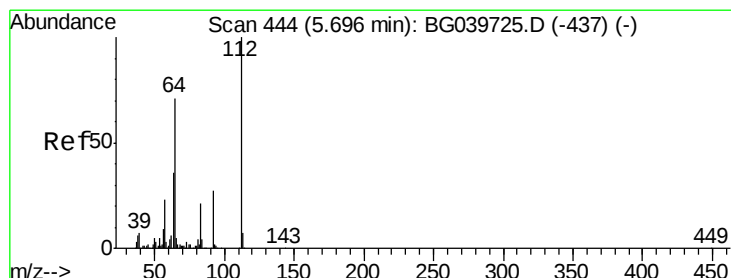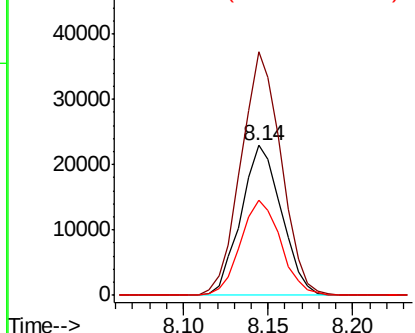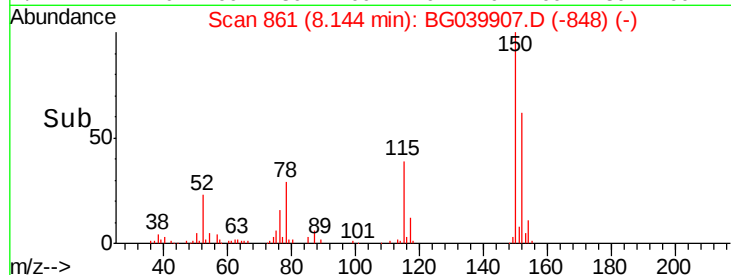

#5

2-Fluorophenol
Concen: 120.619 ng
RT: 5.69 min Scan# 443
Delta R.T. -0.02 min
Lab File: BG039907.D
Acq: 13 Mar 2019 18:04

Tgt Ion	Ratio	Lower	Upper
112	100		
64	70.9	57.8	86.8
63	36.9	29.8	44.6


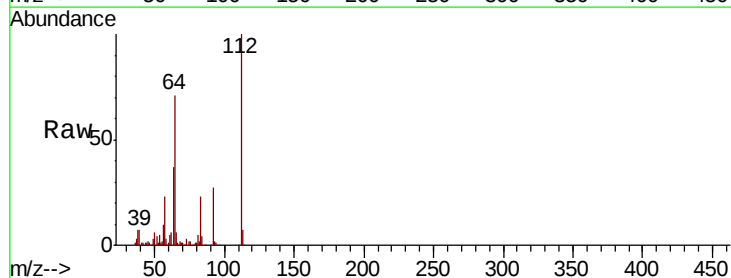


Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG0

Ion 63.00 (62.70 to 63.70): BG0

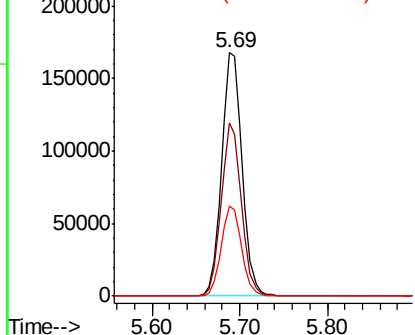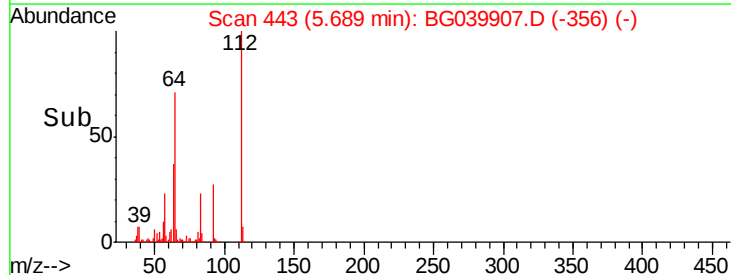



#7

Phenol-d6

Concen: 112.644 ng

RT: 7.29 min Scan# 716

Delta R.T. -0.02 min

Lab File: BG039907.D

Acq: 13 Mar 2019 18:04

Instrument :

BNA_G

ClientSampleId :

PB117884BL


Tot Ion: 99 Resp: 377551

Ion Ratio Lower Upper




99 100

42 21.2 18.2 27.2

71 36.3 28.0 42.0

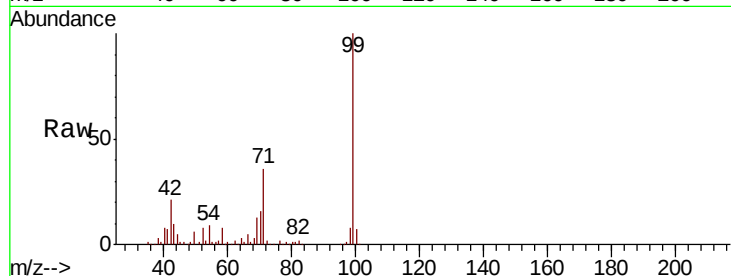

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

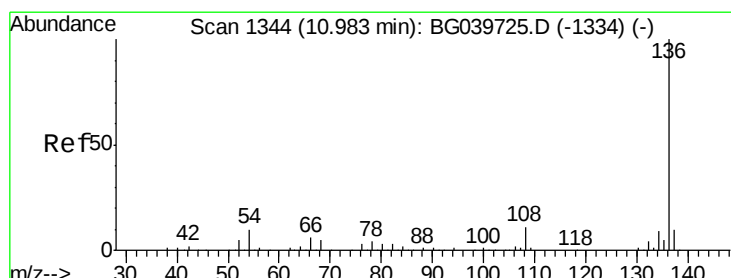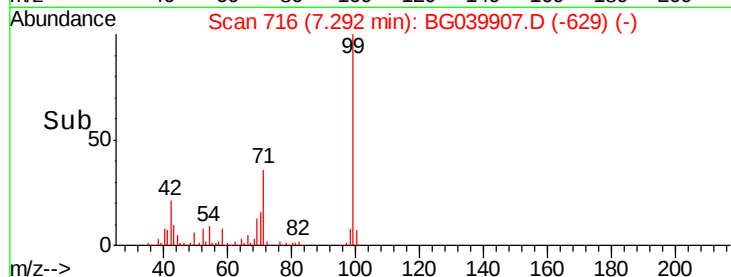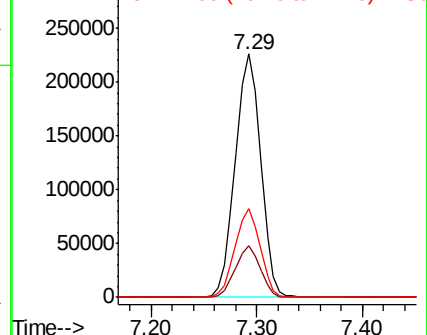

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.97 min Scan# 1342

Delta R.T. -0.02 min

Lab File: BG039907.D

Acq: 13 Mar 2019 18:04

Tgt Ion: 136 Resp: 156805


Ion Ratio Lower Upper

136 100



137 10.1 9.1 13.7


54 9.5 9.4 14.2

68 6.0 4.2 6.4

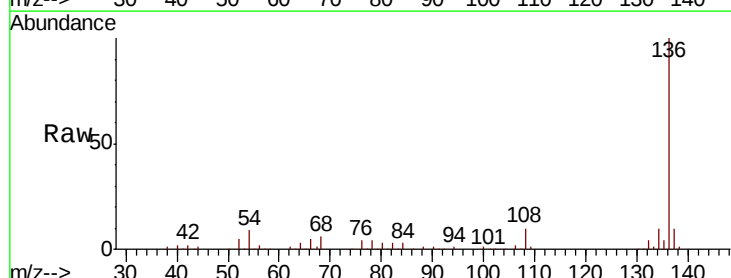

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC


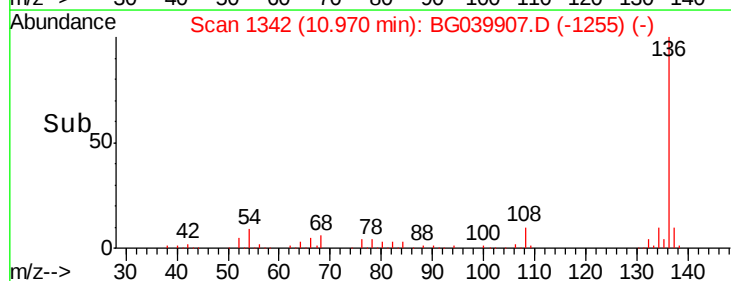
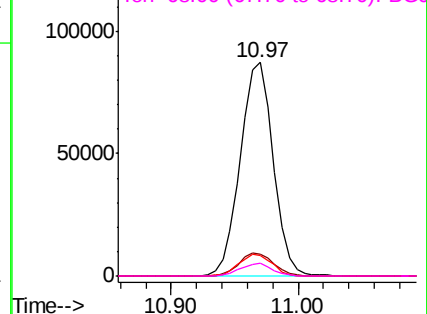


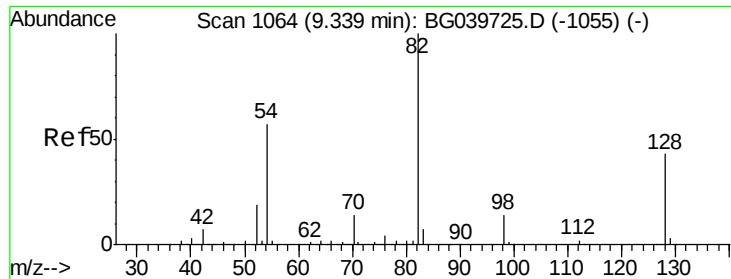

#23
Nitrobenzene-d5
Concen: 77.814 ng
RT: 9.32 min Scan# 1062
Delta R.T. -0.02 min
Lab File: BG039907.D
Acq: 13 Mar 2019 18:04




Instrument :
BNA_G
ClientSampleId :
PB117884BL


Tot Ion: 82 Resp: 225606
Ion Ratio Lower Upper
82 100
128 45.3 31.3 46.9
54 61.8 50.9 76.3

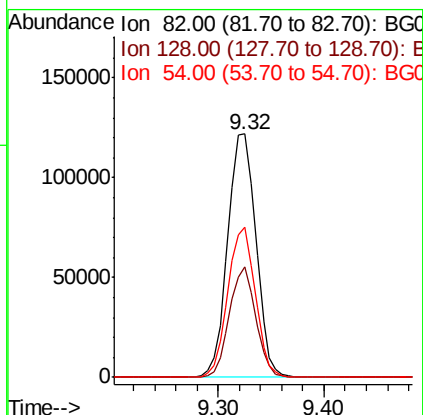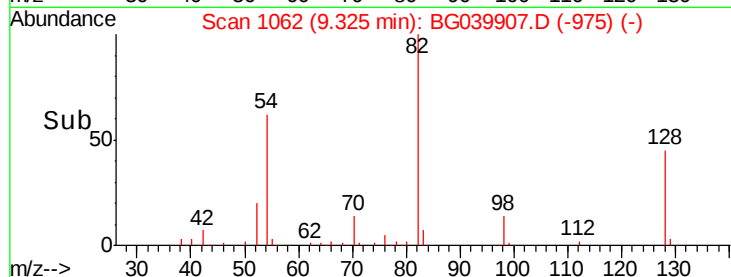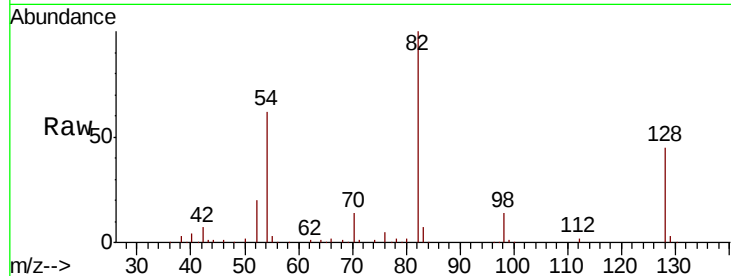

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.77 min Scan# 1989
Delta R.T. -0.02 min
Lab File: BG039907.D
Acq: 13 Mar 2019 18:04

Tgt Ion:164 Resp: 104018
Ion Ratio Lower Upper
164 100
162 97.9 81.6 122.4
160 40.7 34.2 51.2

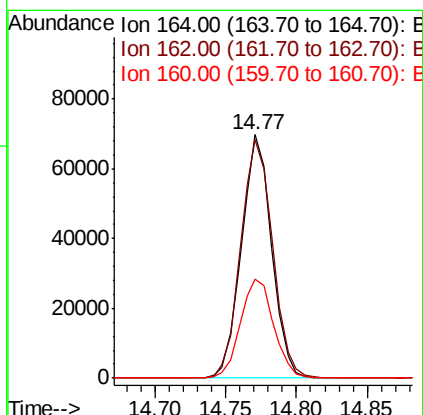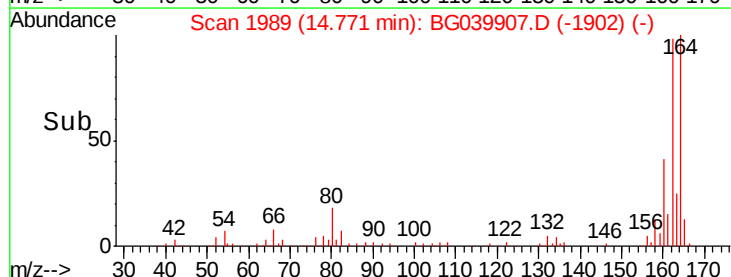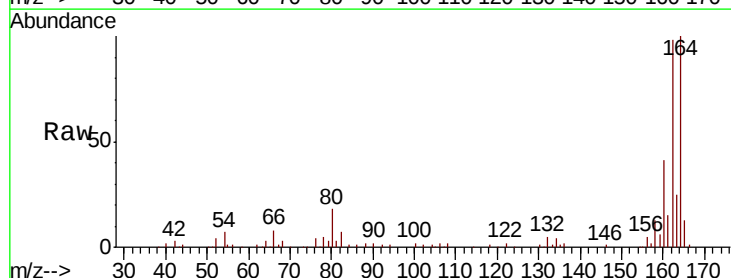


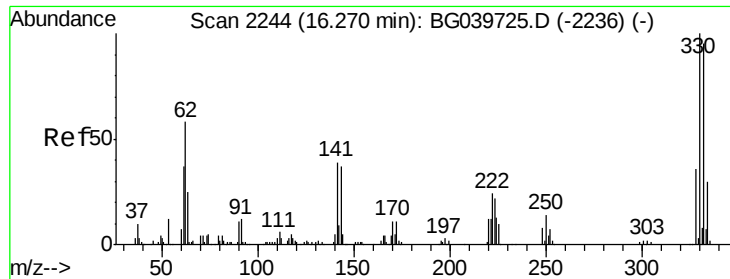

#42
 2,4,6-Tribromophenol
 Concen: 125.367 ng
 RT: 16.26 min Scan# 2242
 Delta R.T. -0.02 min
 Lab File: BG039907.D
 Acq: 13 Mar 2019 18:04

Instrument :
 BNA_G
 ClientSampleId :
 PB117884BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.3	75.7	113.5
141	41.4	35.6	53.4



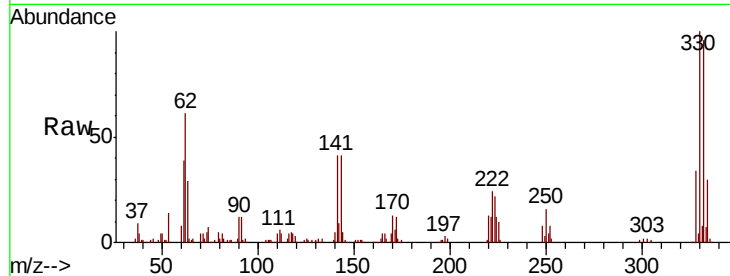


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

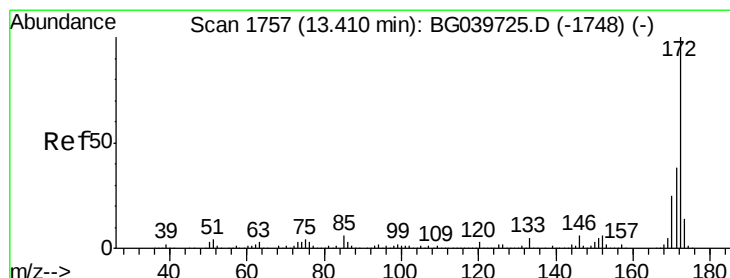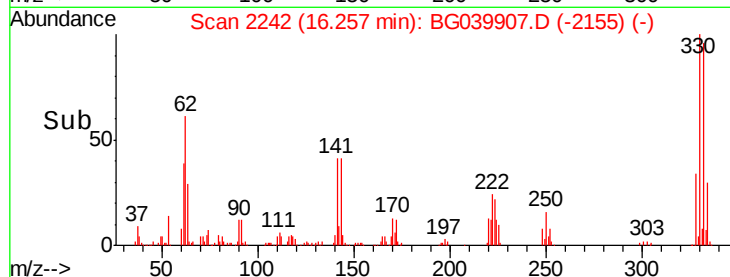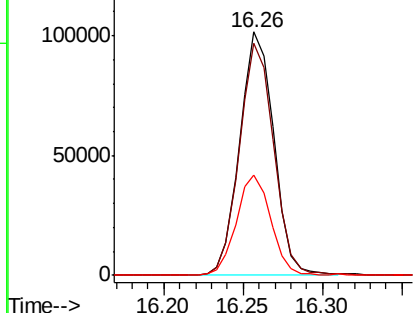

#45
 2-Fluorobiphenyl
 Concen: 78.076 ng
 RT: 13.40 min Scan# 1755
 Delta R.T. -0.02 min
 Lab File: BG039907.D
 Acq: 13 Mar 2019 18:04

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.5	30.8	46.2
170	24.6	20.2	30.4


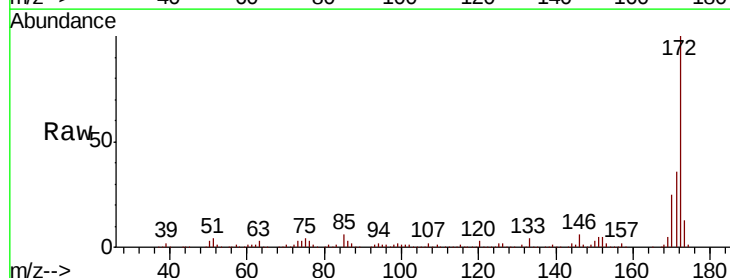


Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E



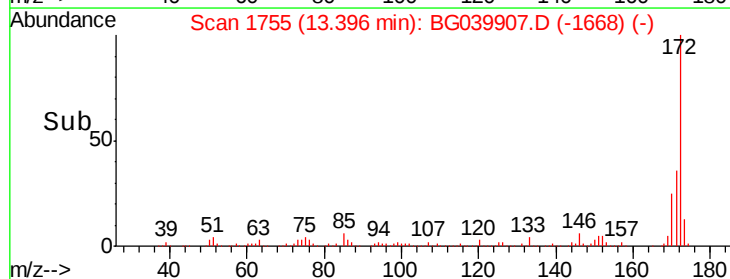
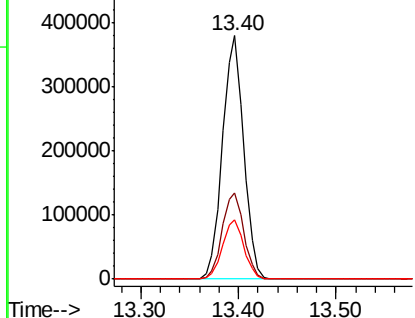




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.51 min Scan# 2456
Delta R.T. -0.02 min
Lab File: BG039907.D
Acq: 13 Mar 2019 18:04




Instrument :
BNA_G
ClientSampleId :
PB117884BL


Tot Ion:188 Resp: 266888
Ion Ratio Lower Upper
188 100
94 7.8 6.9 10.3
80 8.7 8.1 12.1

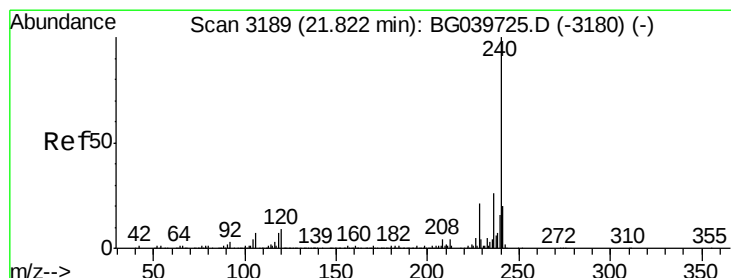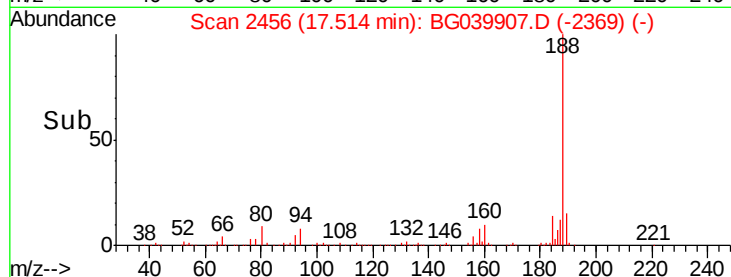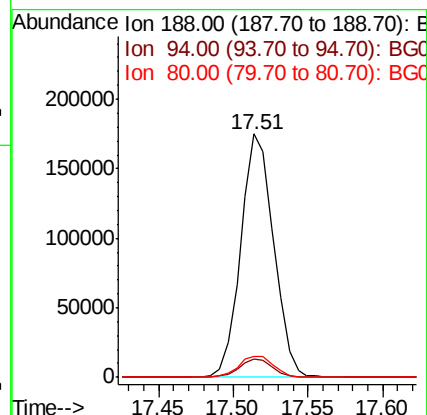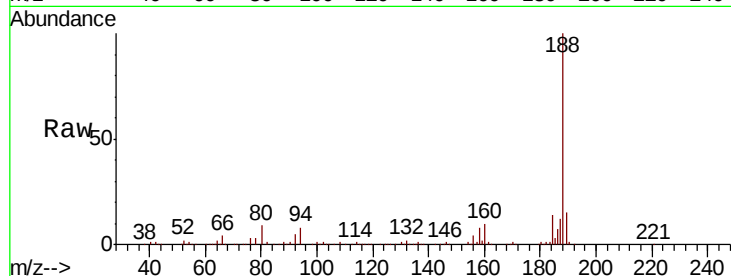

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.80 min Scan# 3186
Delta R.T. -0.03 min
Lab File: BG039907.D
Acq: 13 Mar 2019 18:04

Tgt Ion:240 Resp: 302315
Ion Ratio Lower Upper
240 100
120 8.5 7.0 10.6
236 25.6 21.0 31.4

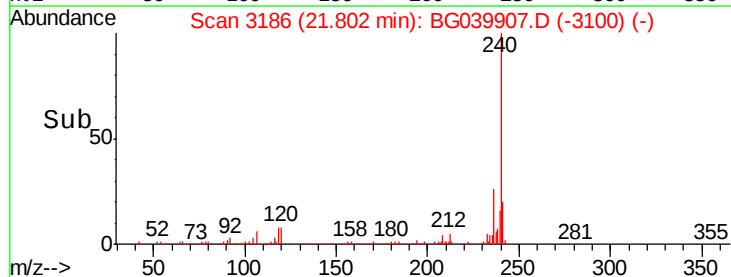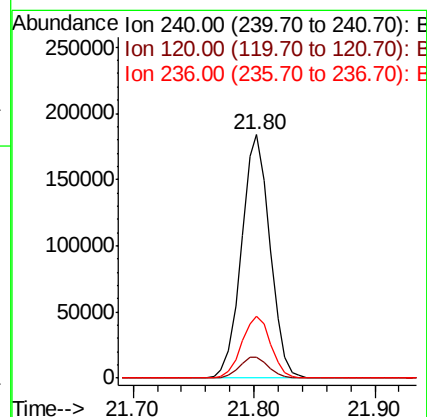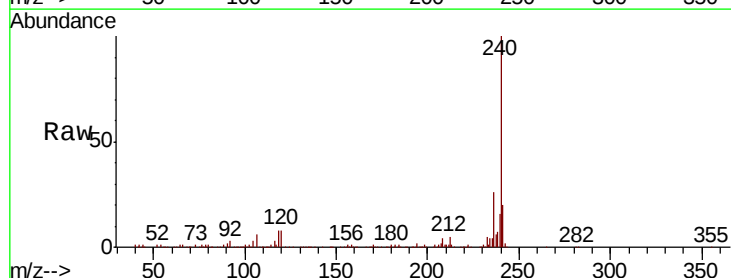

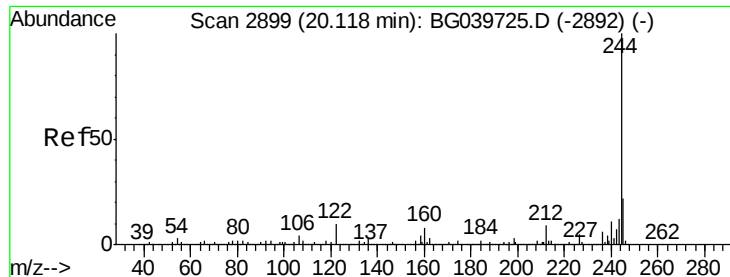

#79

Terphenyl-d14

Concen: 74.915 ng

RT: 20.11 min Scan# 2898

Delta R.T. -0.01 min

Lab File: BG039907.D

Acq: 13 Mar 2019 18:04

Instrument :

BNA_G

ClientSampleId :

PB117884BL


Tot Ion:244 Resp: 1028612

Ion Ratio Lower Upper

244 100

212 8.7 7.3 10.9




122 8.9 8.4 12.6

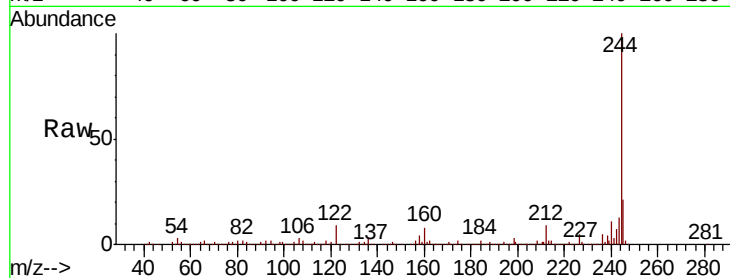

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

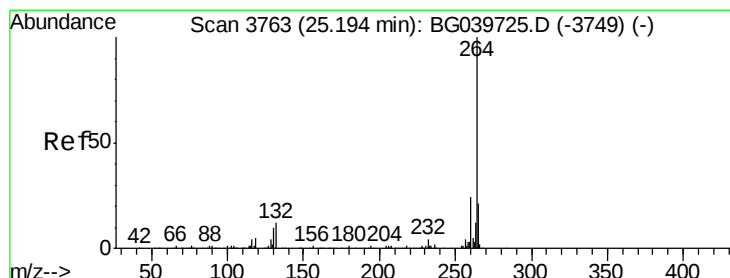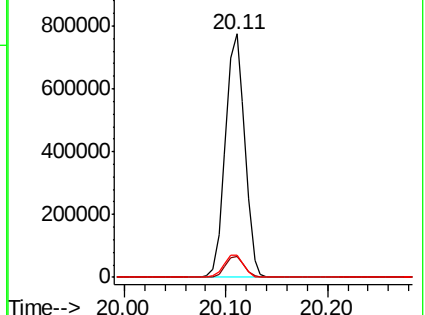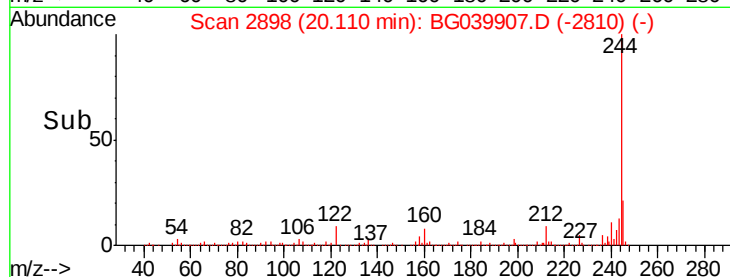

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.16 min Scan# 3758

Delta R.T. -0.04 min

Lab File: BG039907.D

Acq: 13 Mar 2019 18:04


Tgt Ion:264 Resp: 300002

Ion Ratio Lower Upper

264 100

260 25.8 18.2 27.4

265 22.6 18.5 27.7

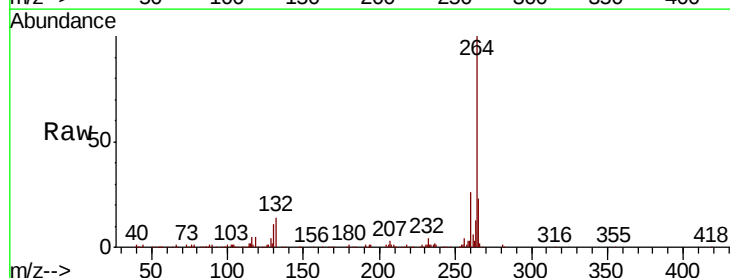

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

