
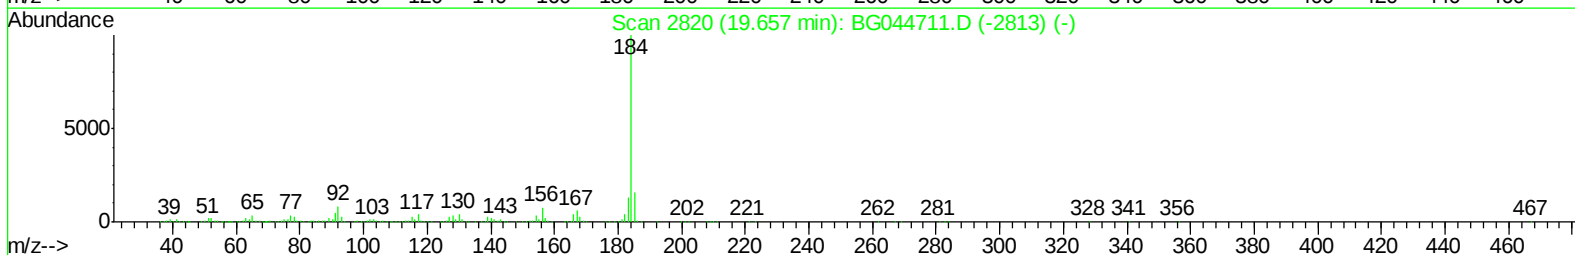
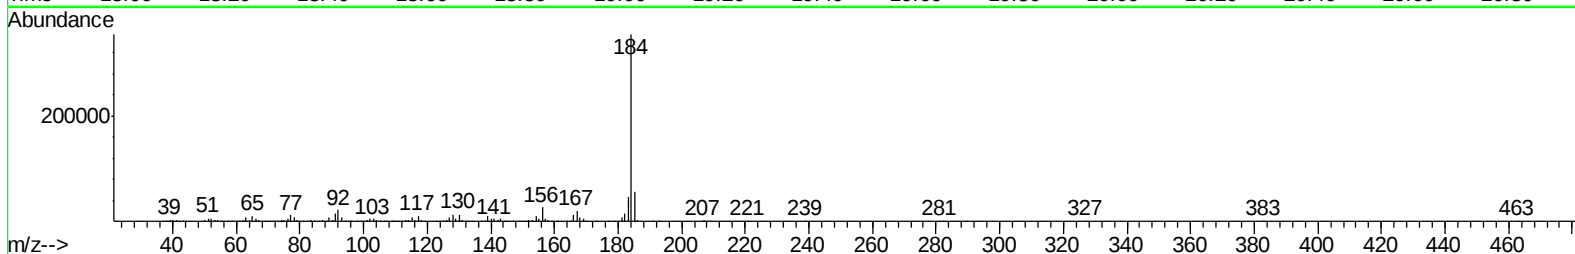


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG031320\
 Data File : BG044799.D
 Acq On : 14 Mar 2020 17:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 16 09:14:03 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 10 16:27:39 2020
 Response via : Initial Calibration

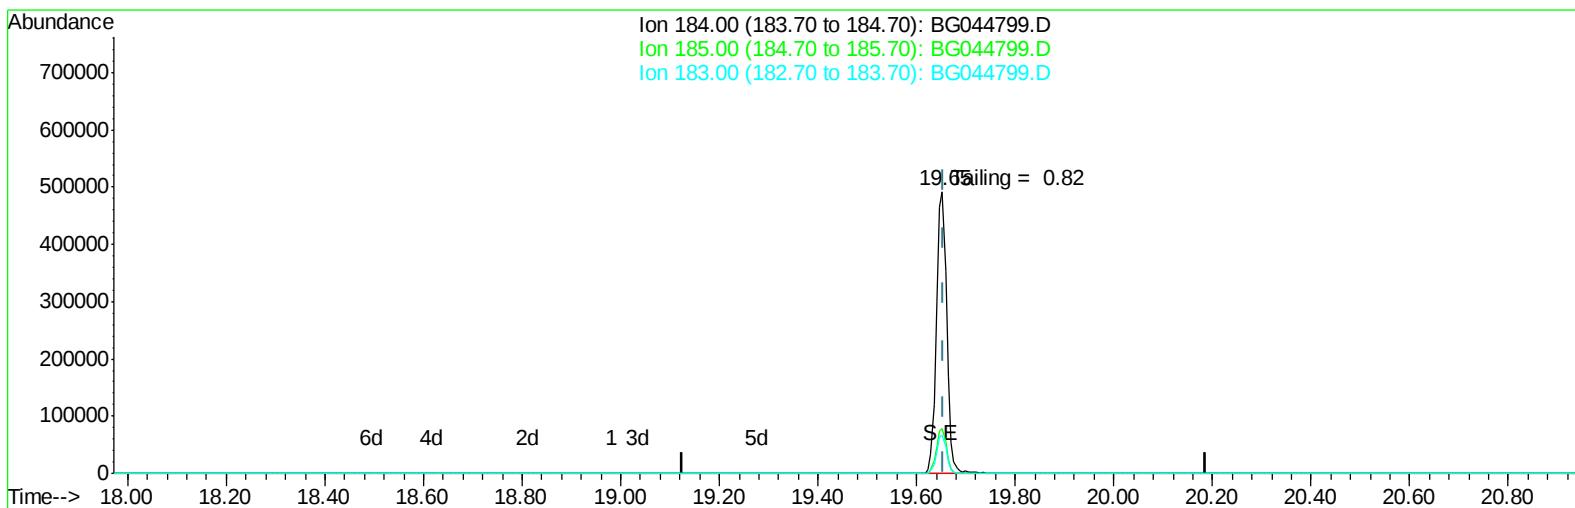

TIC: BG044799.D

(77) Benzidine

18.983min (-0.674) 2.37ng

response 53

Ion	Exp%	Act%
184.00	100	100
185.00	16.10	0.00#
183.00	13.20	0.00#
0.00	0.00	0.00