
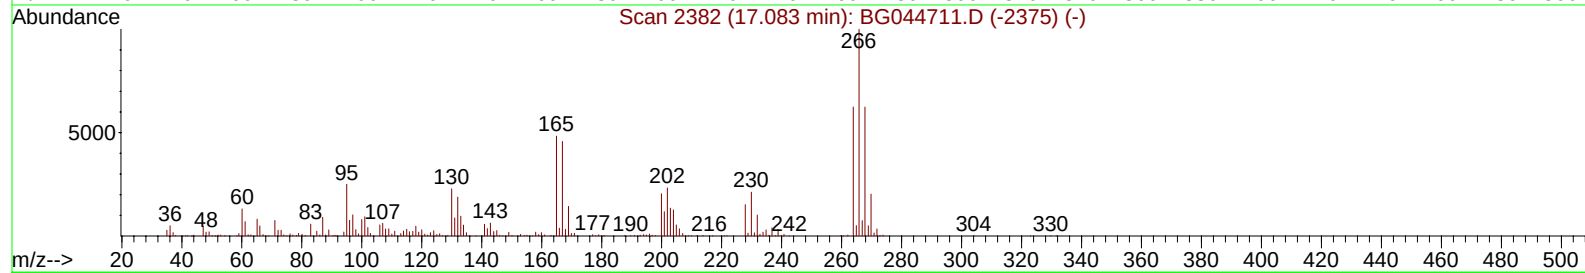
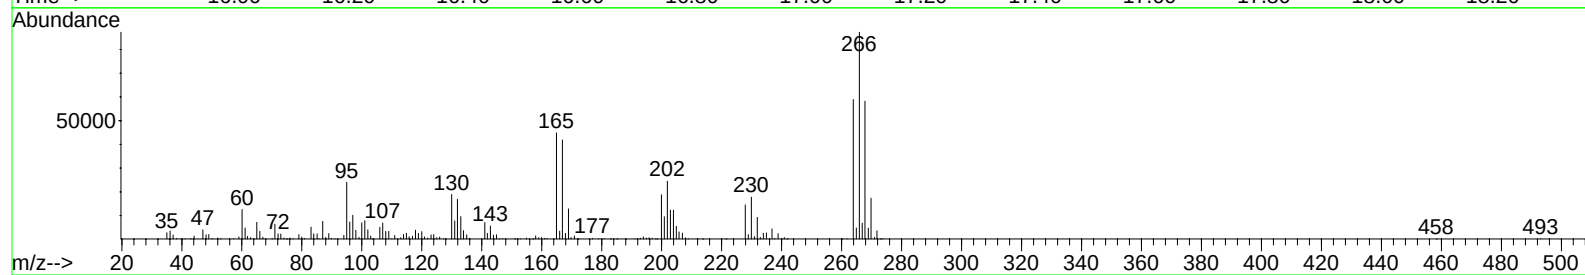


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG031320\
 Data File : BG044763.D
 Acq On : 13 Mar 2020 12:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 13 18:53:44 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG031020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 10 16:27:39 2020
 Response via : Initial Calibration

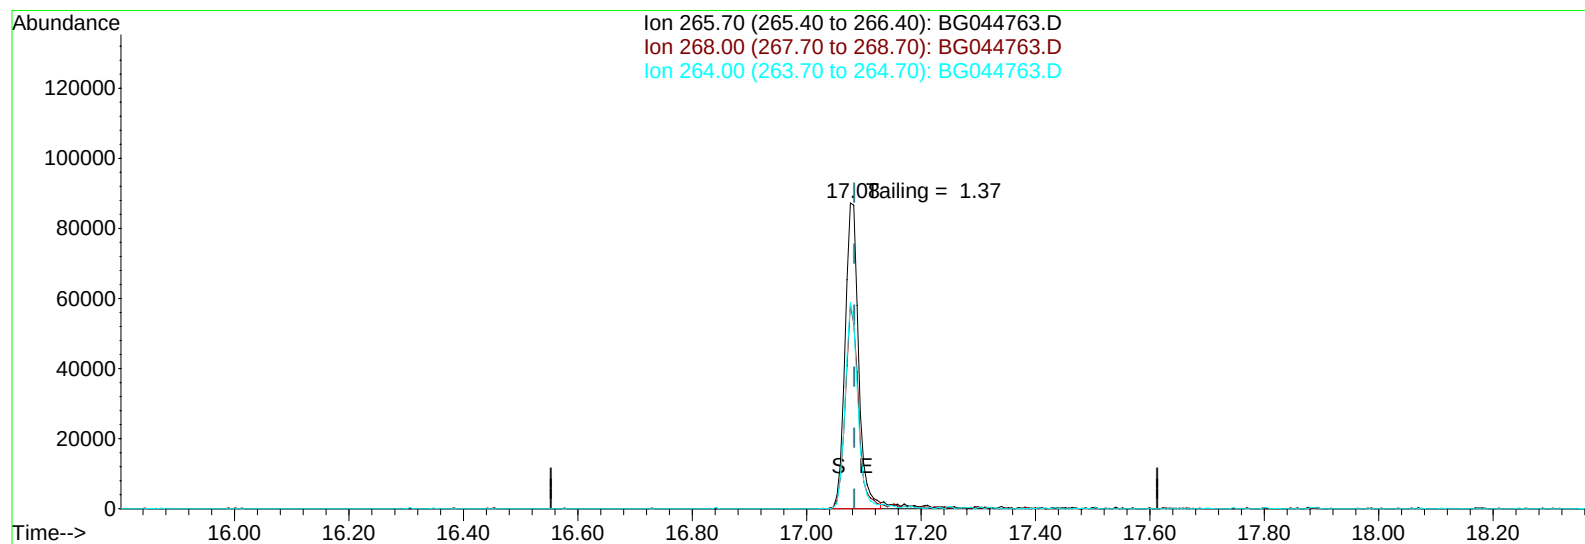

TIC: BG044763.D

(70) Pentachlorophenol (C)




17.076min (-0.007) 221591.61ng

response 145517

Ion	Exp%	Act%
265.70	100	100
268.00	62.40	66.70
264.00	62.40	67.44
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG031320\  
Data File : BG044763.D  
Acq On    : 13 Mar 2020 12:10  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Mar 13 18:53:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG031020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 10 16:27:39 2020
Response via : Initial Calibration

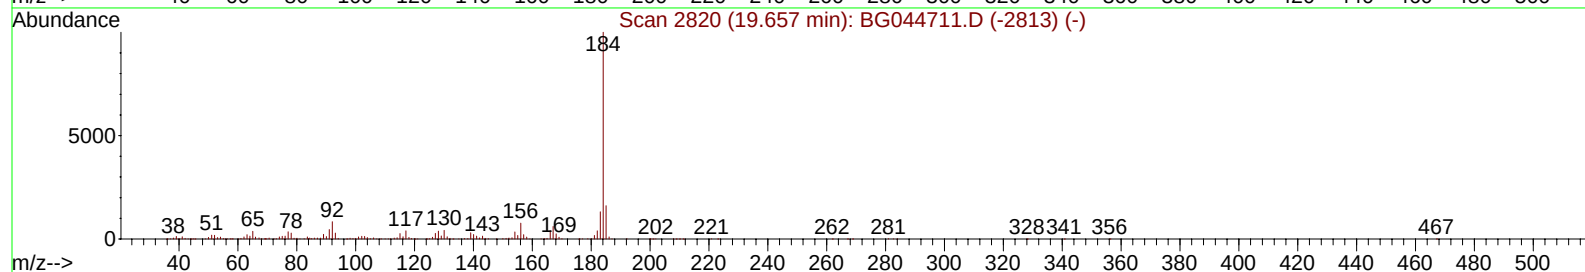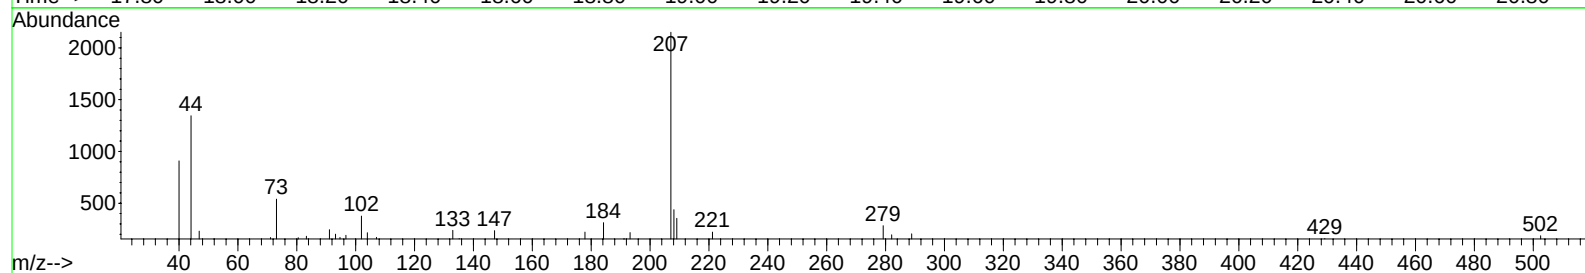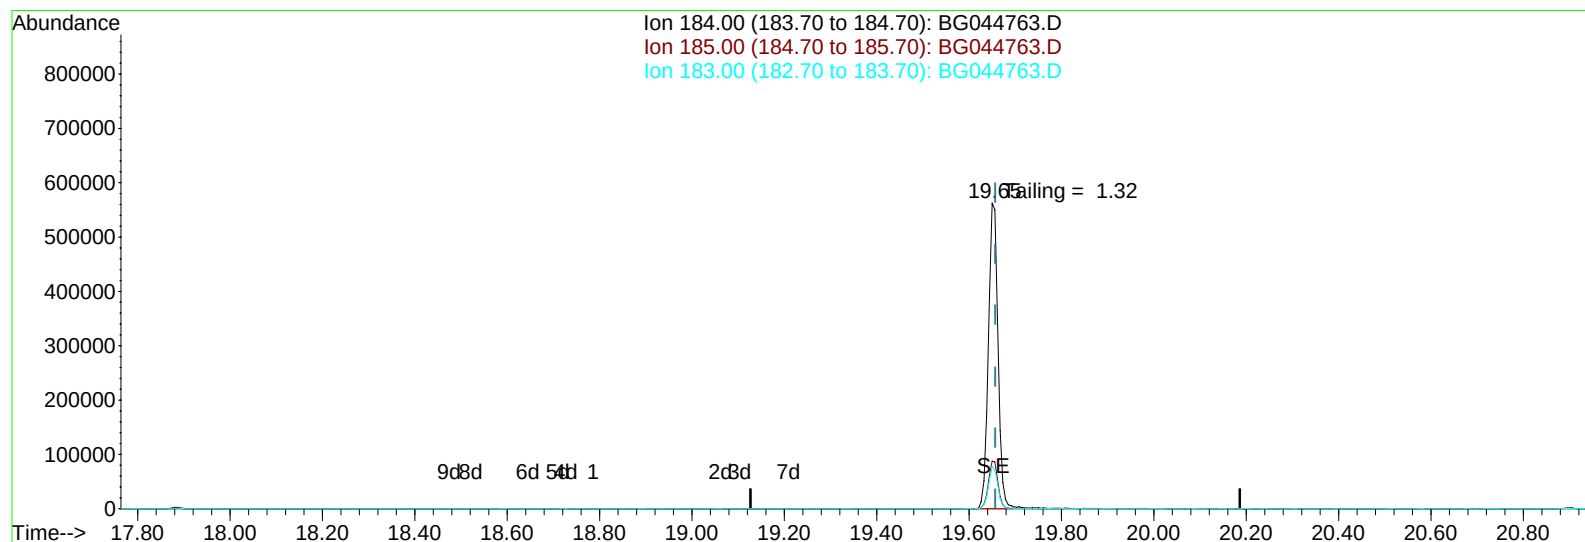

TIC: BG044763.D

(77) Benzidine

18.786min (-0.871) 0.84ng

response 164

Ion	Exp%	Act%
184.00	100	100
185.00	16.10	0.00#
183.00	13.20	0.00#
0.00	0.00	0.00