
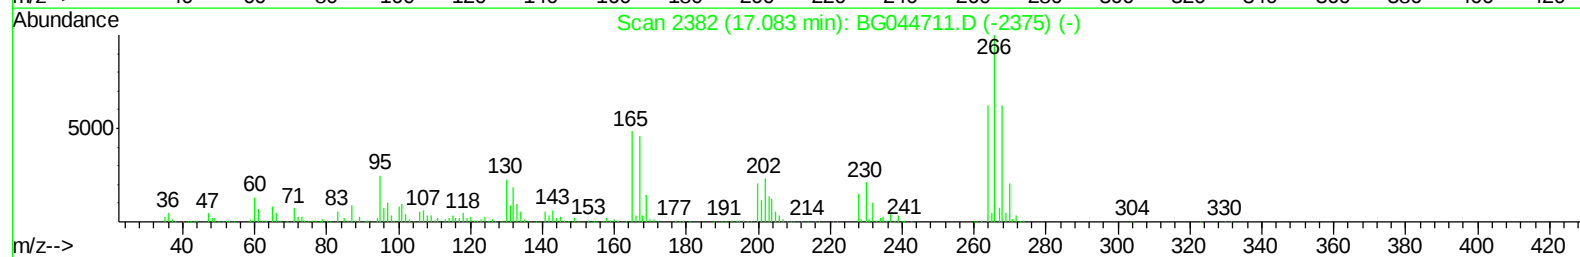
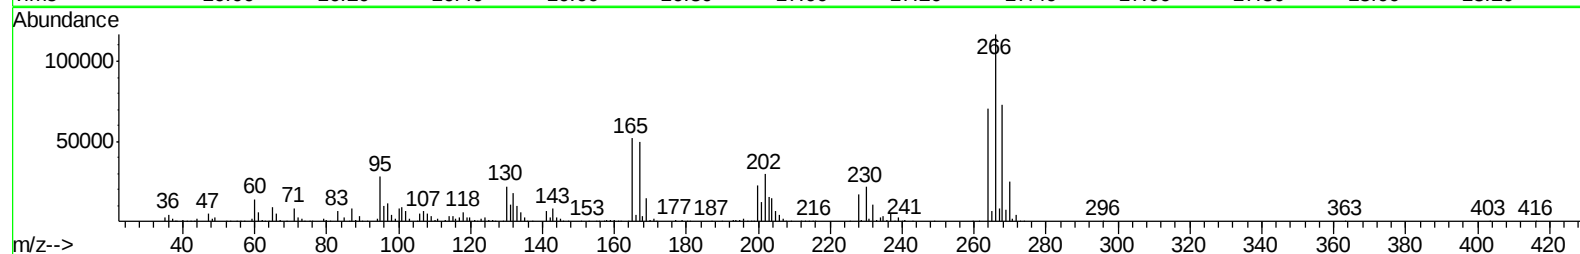


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG031320\
 Data File : BG044781.D
 Acq On : 14 Mar 2020 2:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 16 08:58:46 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 10 16:27:39 2020
 Response via : Initial Calibration

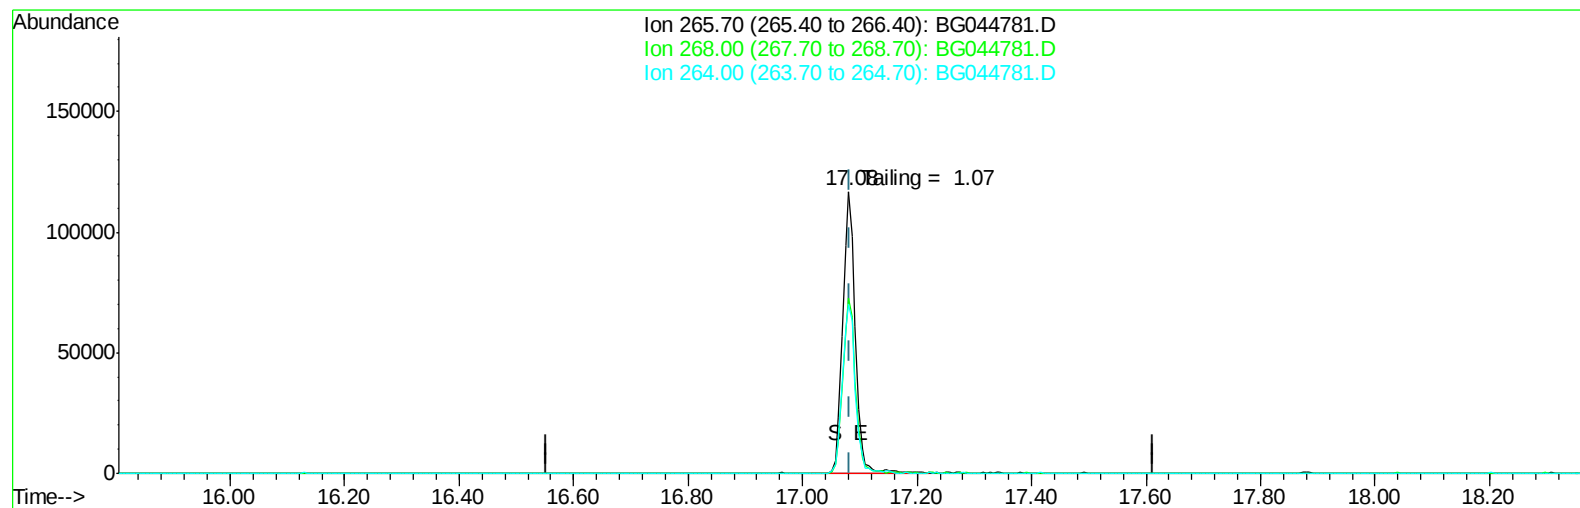

TIC: BG044781.D

(70) Pentachlorophenol (C)




17.081min (-0.003) 261890.70ng

response 177844

Ion	Exp%	Act%
265.70	100	100
268.00	62.40	62.35
264.00	62.40	60.02
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG031320\
 Data File : BG044781.D
 Acq On : 14 Mar 2020 2:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 16 08:58:46 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 10 16:27:39 2020
 Response via : Initial Calibration

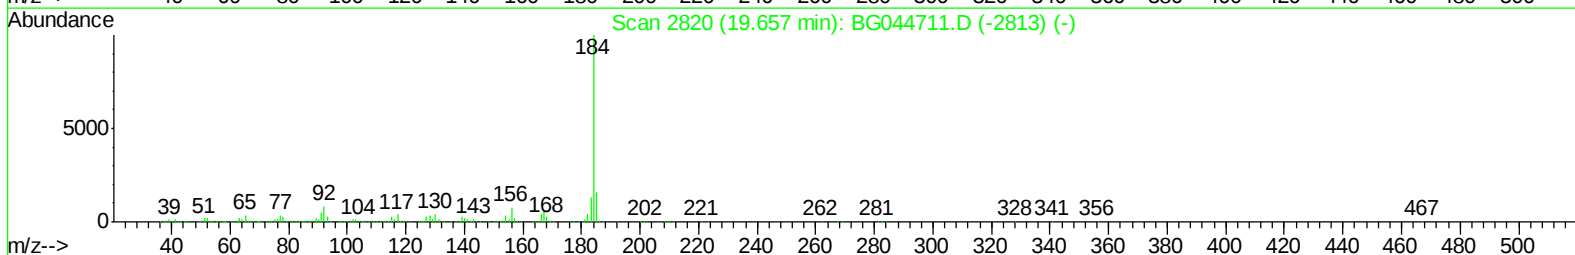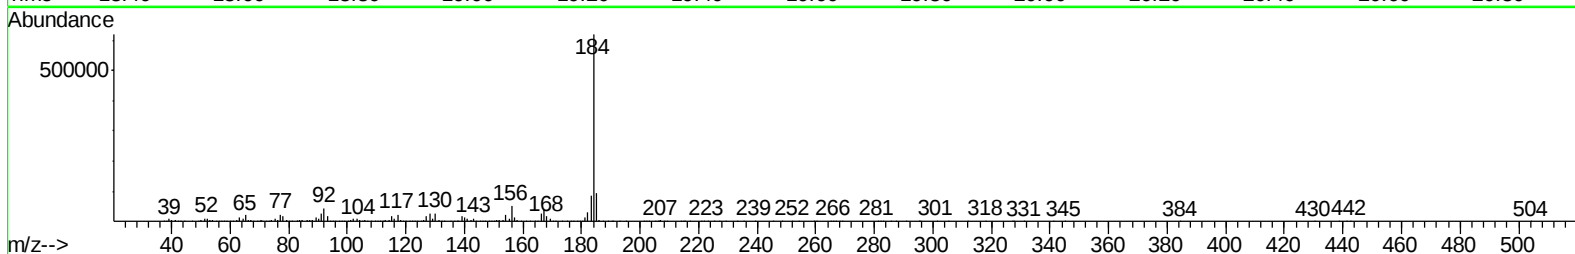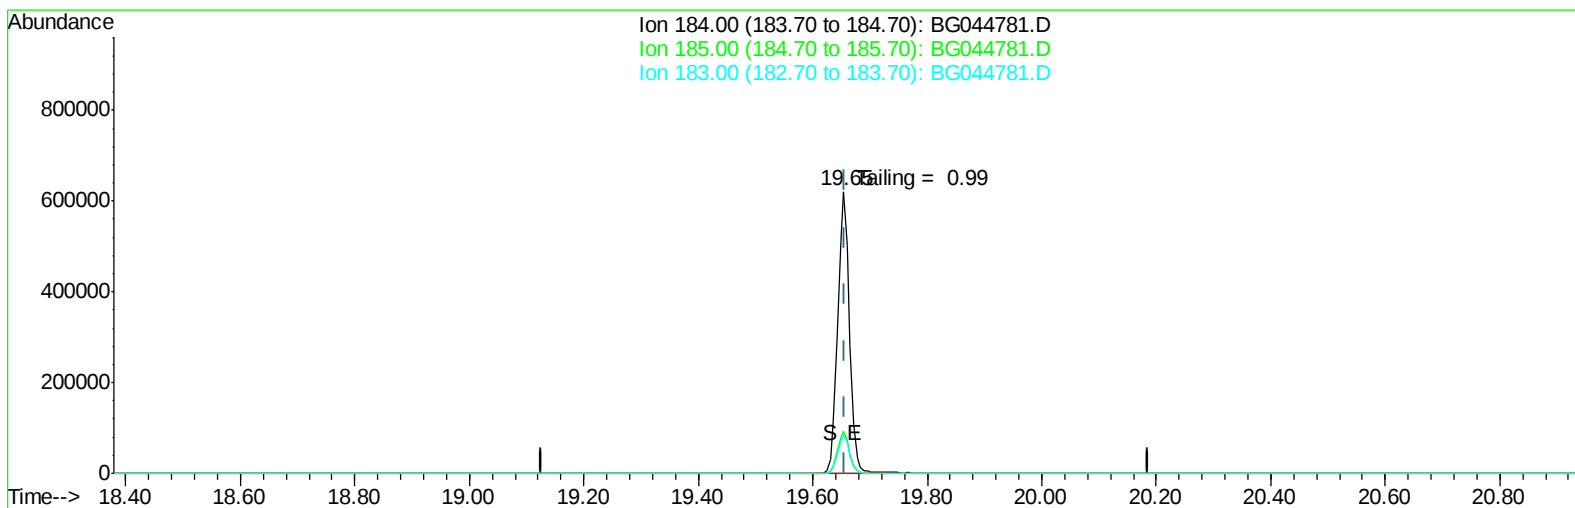

TIC: BG044781.D

(77) Benzidine

19.654min (-0.003) 323075.70ng

response 901995

Ion	Exp%	Act%
184.00	100	100
185.00	16.10	15.23
183.00	13.20	13.82
0.00	0.00	0.00