
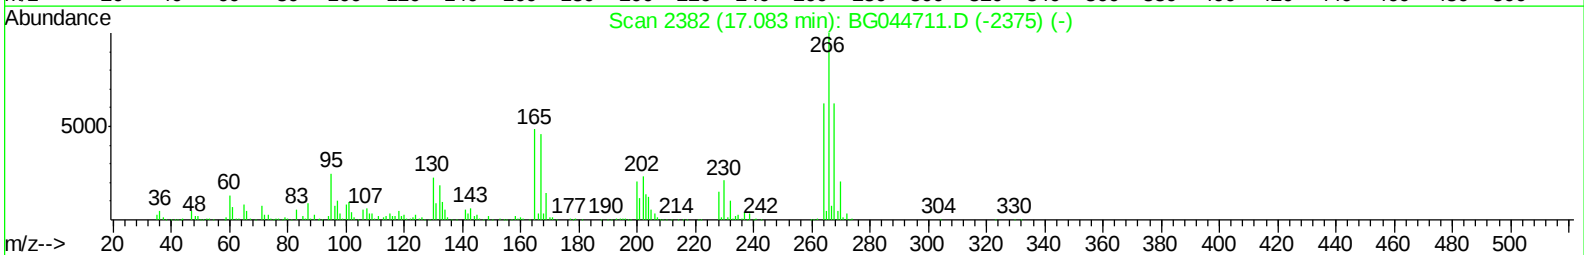
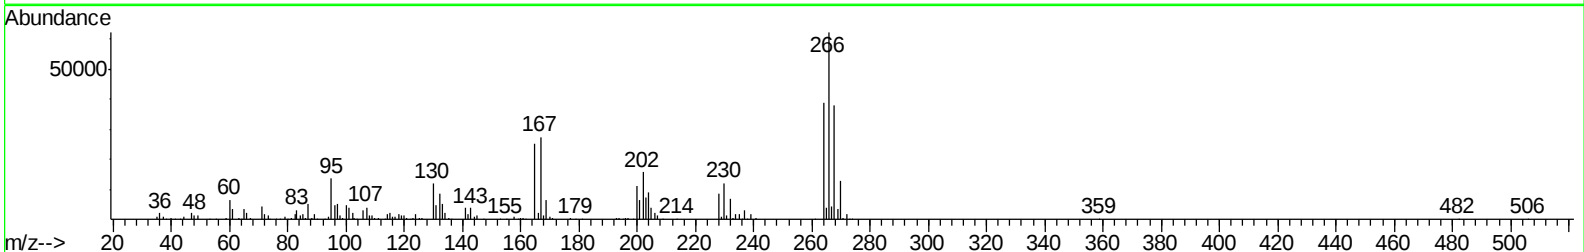


```
Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG031320\  
Data File : BG044799.D  
Acq On    : 14 Mar 2020  17:03  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Mar 16 09:14:03 2020
Quant Method : Z:\SV0ASRV\HPCHEM1\BNA_G\METHODS\8270-BG031020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 10 16:27:39 2020
Response via : Initial Calibration



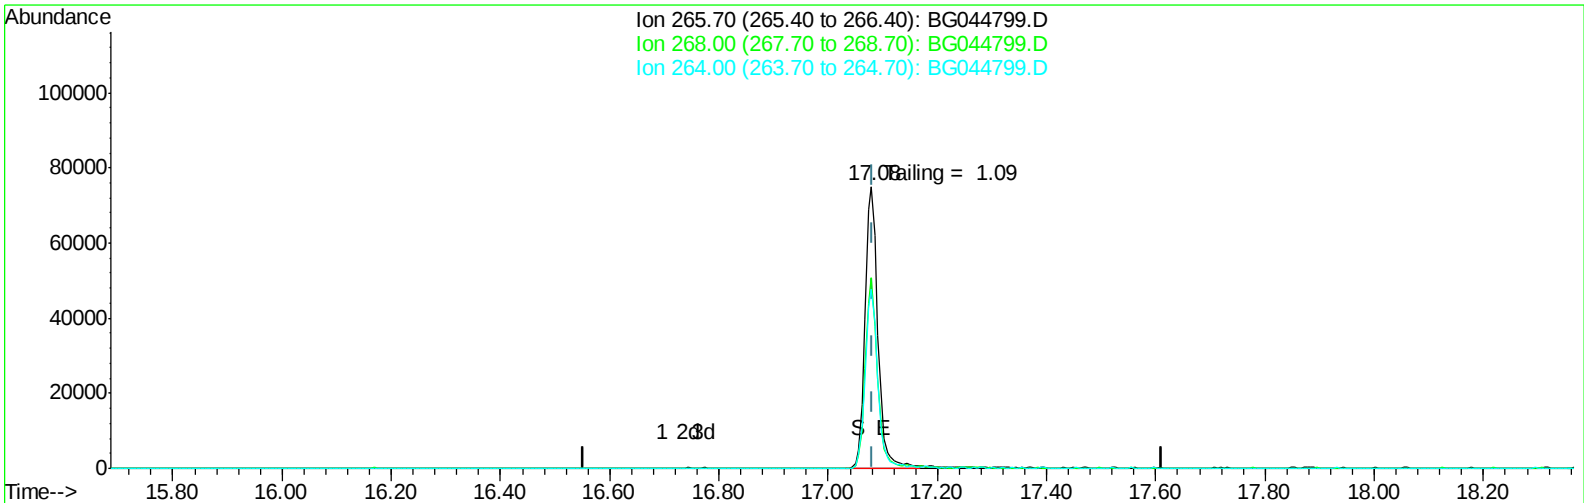


TIC: BG044799.D

Ion	Exp%	Act%
265.70	100	100
268.00	62.40	0.00#
264.00	62.40	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG031320\
Data File : BG044799.D
Acq On : 14 Mar 2020 17:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 16 09:14:03 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 10 16:27:39 2020
Response via : Initial Calibration

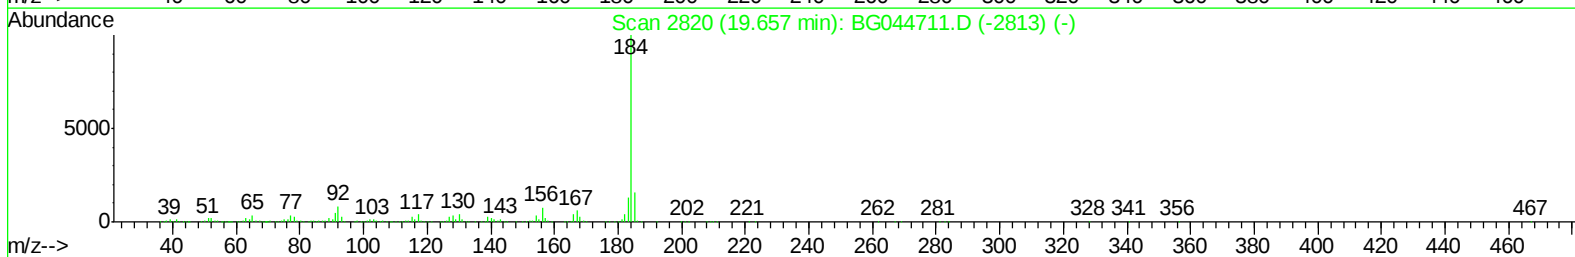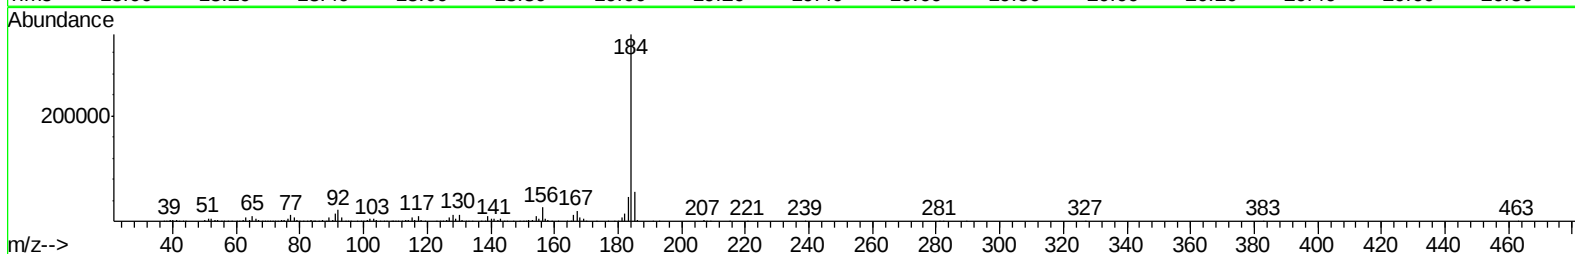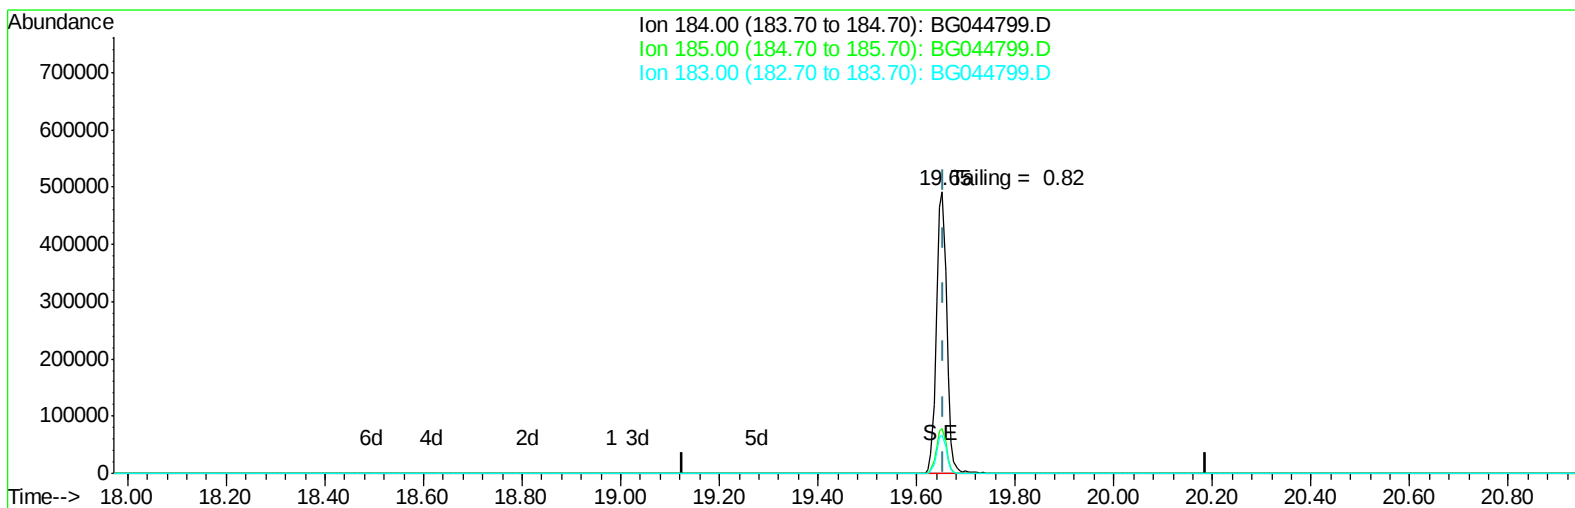

TIC: BG044799.D

(77) Benzidine

18.983min (-0.674) 2.37ng

response 53

Ion	Exp%	Act%
184.00	100	100
185.00	16.10	0.00#
183.00	13.20	0.00#
0.00	0.00	0.00