


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG031320\
 Data File : BG044763.D
 Acq On : 13 Mar 2020 12:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 10 16:27:39 2020

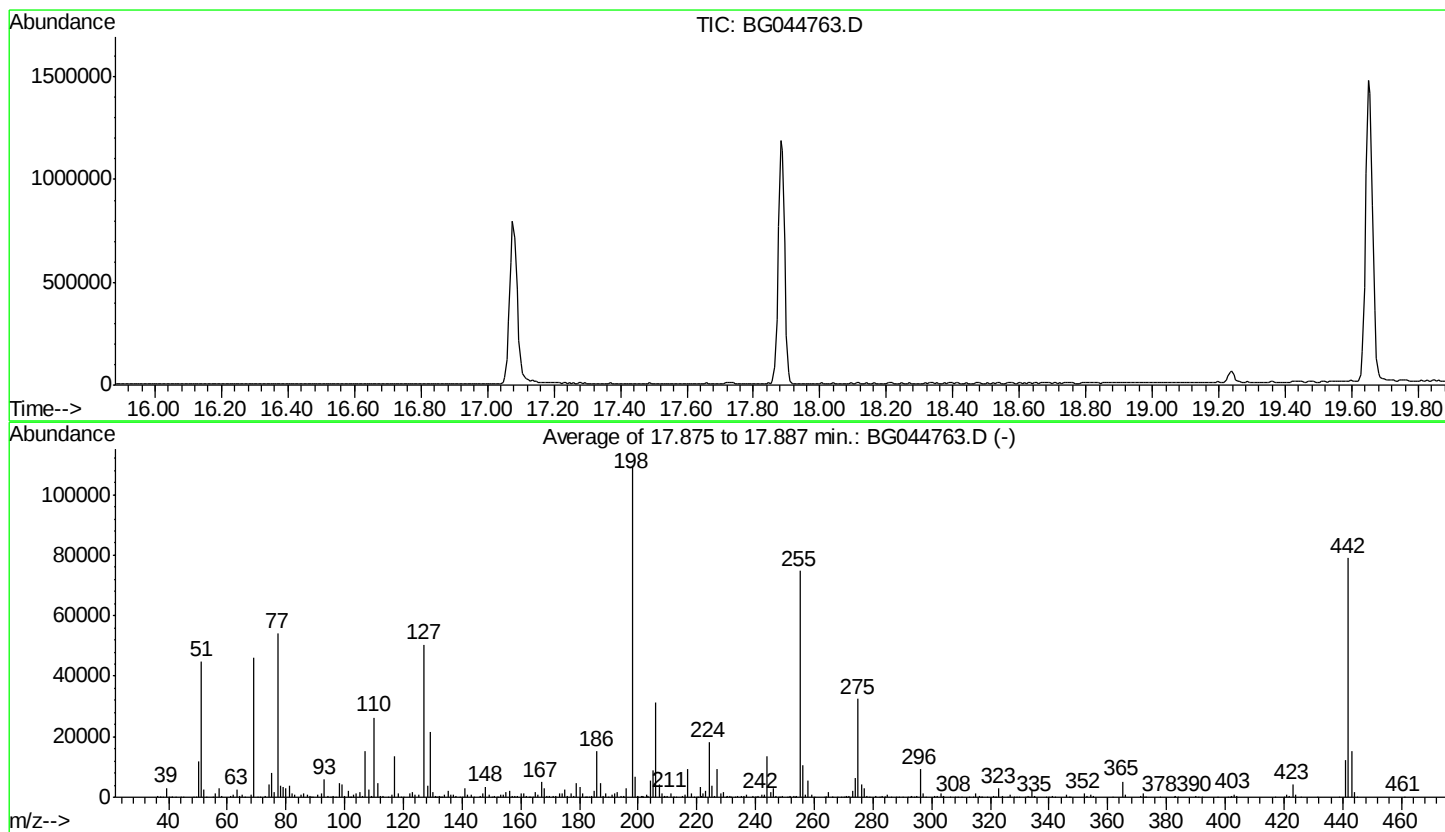

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.8	44722	PASS
68	69	0.00	2	1.9	866	PASS
69	198	0.00	100	42.0	46082	PASS
70	69	0.00	2	0.5	221	PASS
127	198	10	80	46.1	50565	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	109602	PASS
199	198	5	9	6.2	6829	PASS
275	198	10	60	29.6	32458	PASS
365	198	1	100	4.8	5279	PASS
441	198	0.01	100	11.2	12292	PASS
442	198	50	100	72.1	78989	PASS
443	442	15	24	19.5	15368	PASS