


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG031320\
 Data File : BG044781.D
 Acq On : 14 Mar 2020 2:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 10 16:27:39 2020

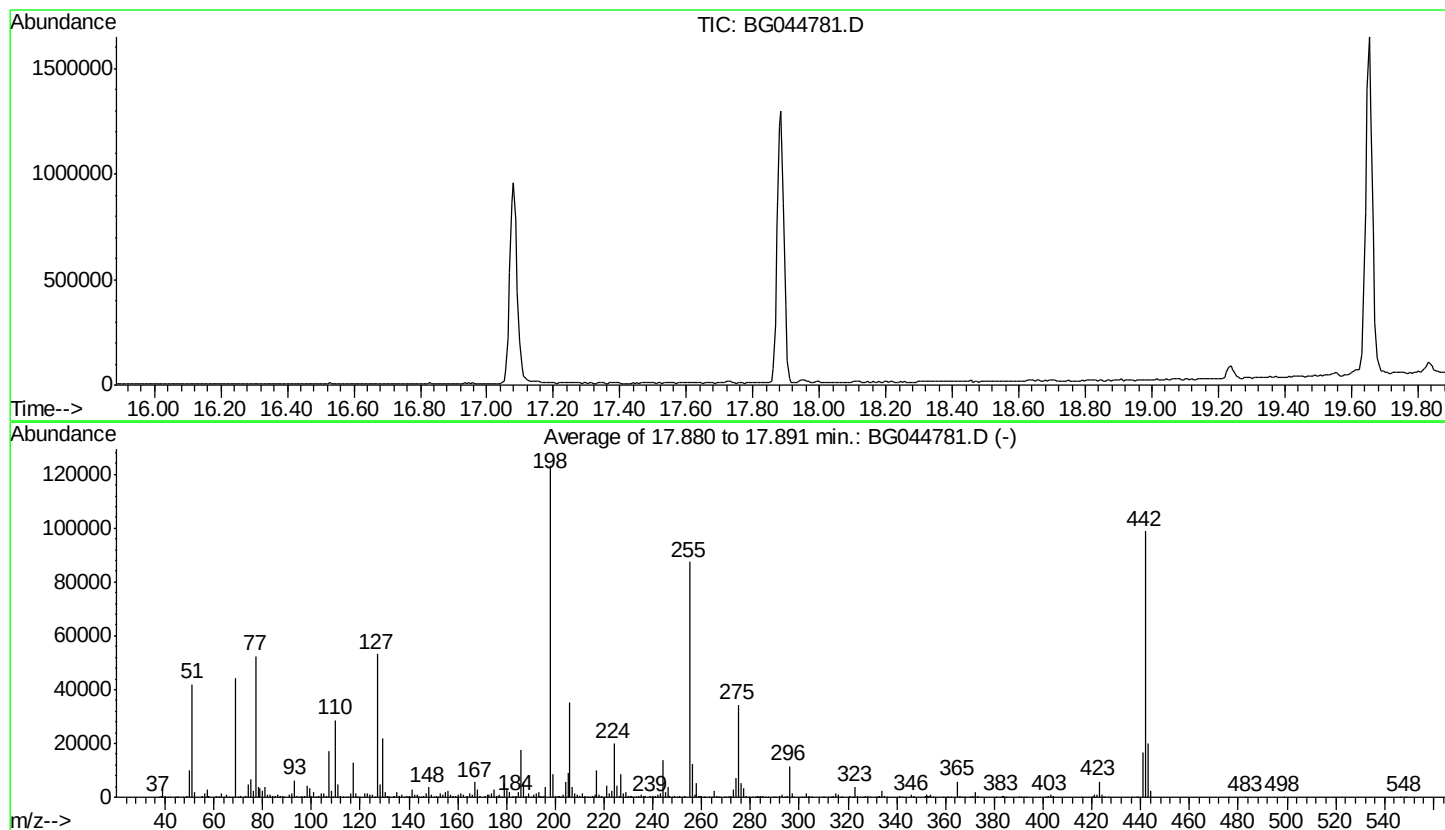

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2509

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	42061	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.8	44143	PASS
70	69	0.00	2	0.3	133	PASS
127	198	10	80	43.1	53114	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	123226	PASS
199	198	5	9	6.8	8372	PASS
275	198	10	60	27.8	34309	PASS
365	198	1	100	4.8	5952	PASS
441	198	0.01	100	13.4	16487	PASS
442	198	50	100	80.1	98765	PASS
443	442	15	24	20.2	19962	PASS