


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG031320\
Data File : BG044799.D
Acq On : 14 Mar 2020 17:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031020.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Mar 10 16:27:39 2020

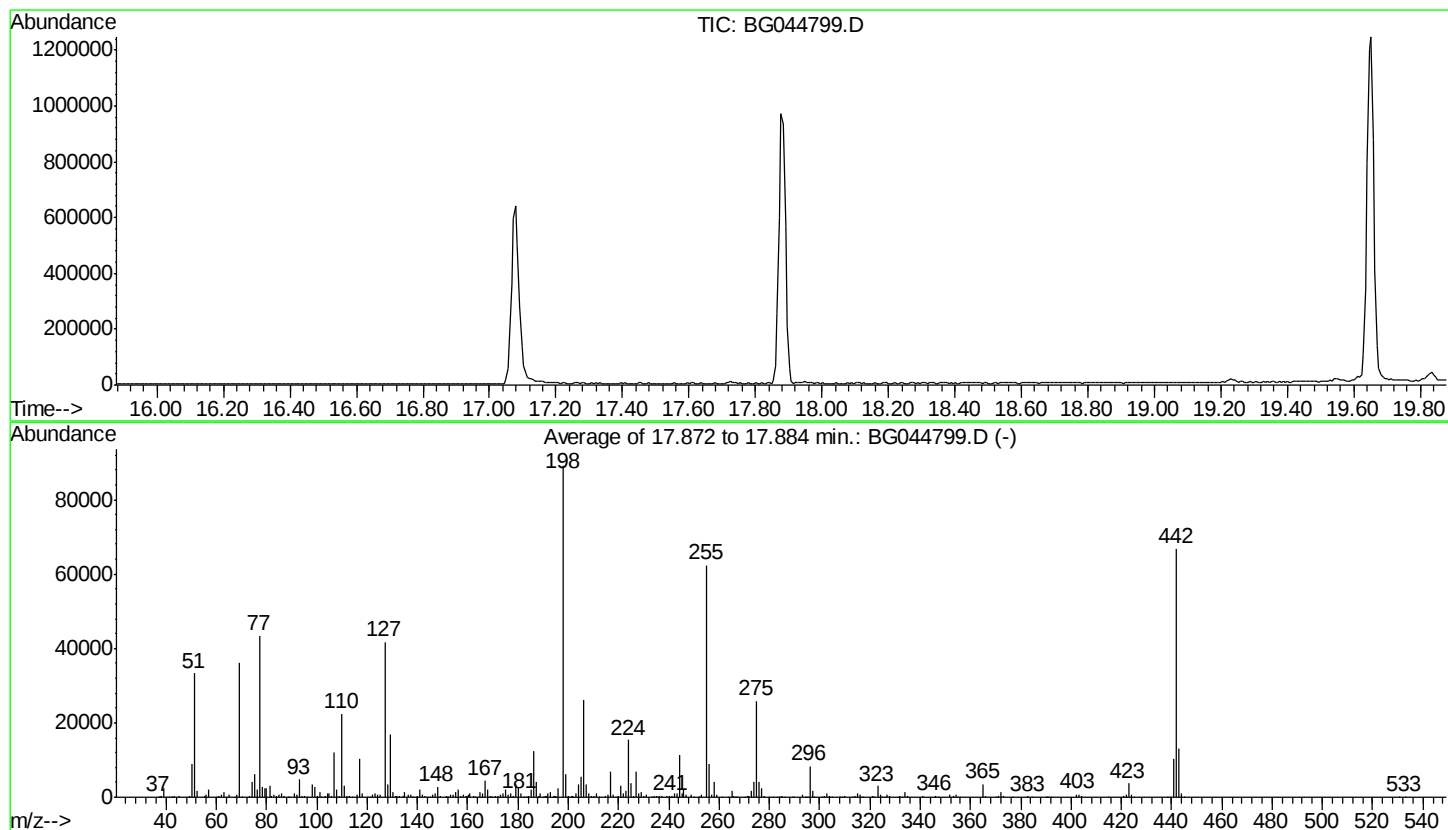

AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	33285	PASS
68	69	0.00	2	1.6	595	PASS
69	198	0.00	100	40.6	36209	PASS
70	69	0.00	2	0.4	144	PASS
127	198	10	80	46.8	41746	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	89157	PASS
199	198	5	9	6.8	6070	PASS
275	198	10	60	29.0	25886	PASS
365	198	1	100	3.9	3517	PASS
441	198	0.01	100	11.6	10384	PASS
442	198	50	100	74.9	66781	PASS
443	442	15	24	19.4	12978	PASS