
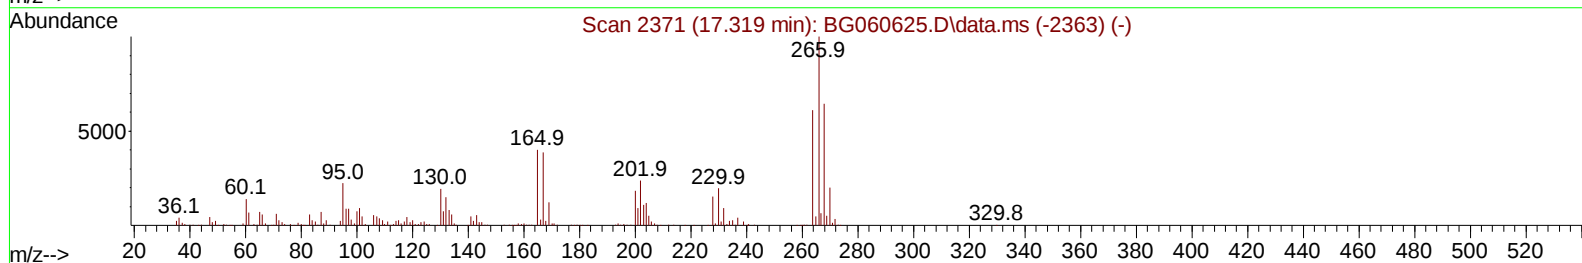
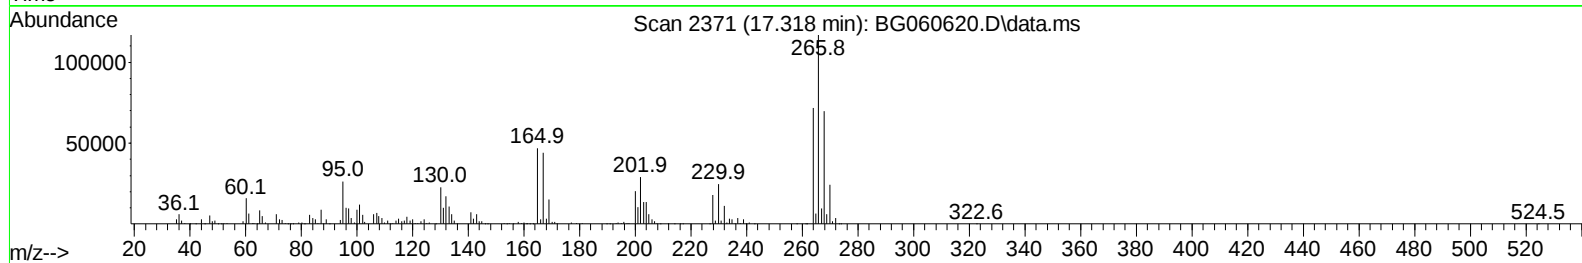


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031324\
Data File : BG060620.D
Acq On : 13 Mar 2024 10:02
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 14 00:52:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 00:45:22 2024
Response via : Initial Calibration

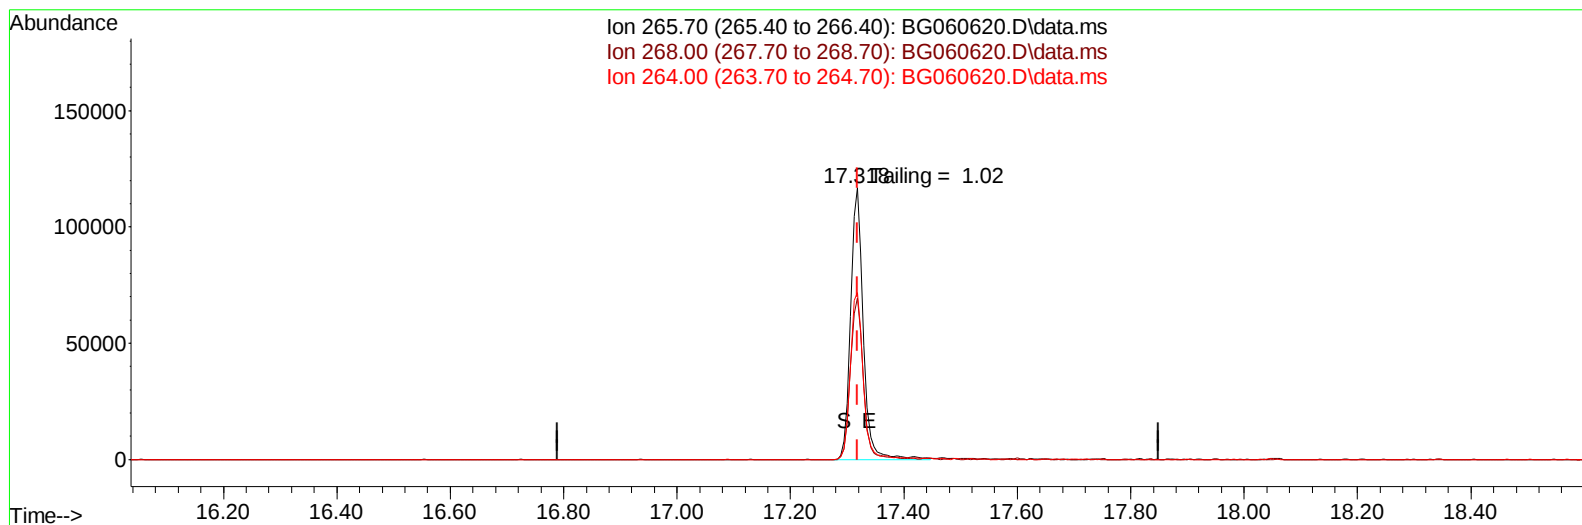

TIC: BG060620.D\data.ms




(70) Pentachlorophenol (C)

17.318min (-0.001) 405314.76 ng

response 179139

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	59.60
264.00	61.10	61.40
0.00	0.00	0.00

Quant Time: Mar 14 00:52:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 00:45:22 2024
Response via : Initial Calibration

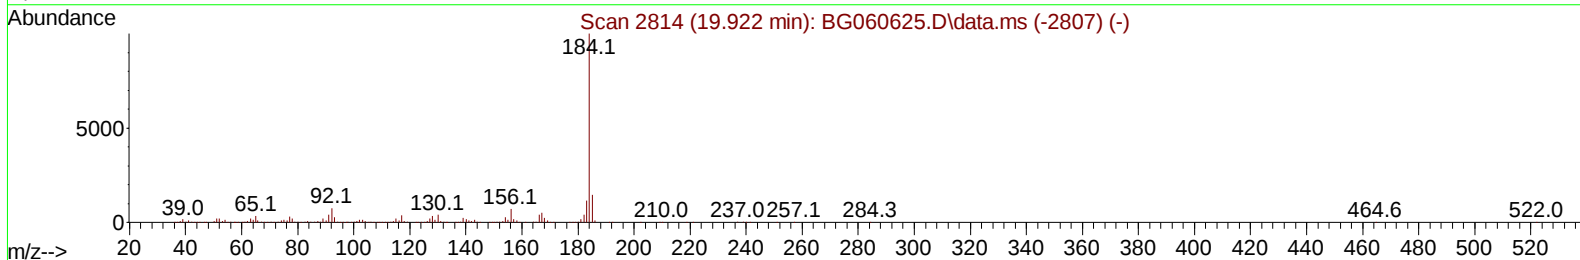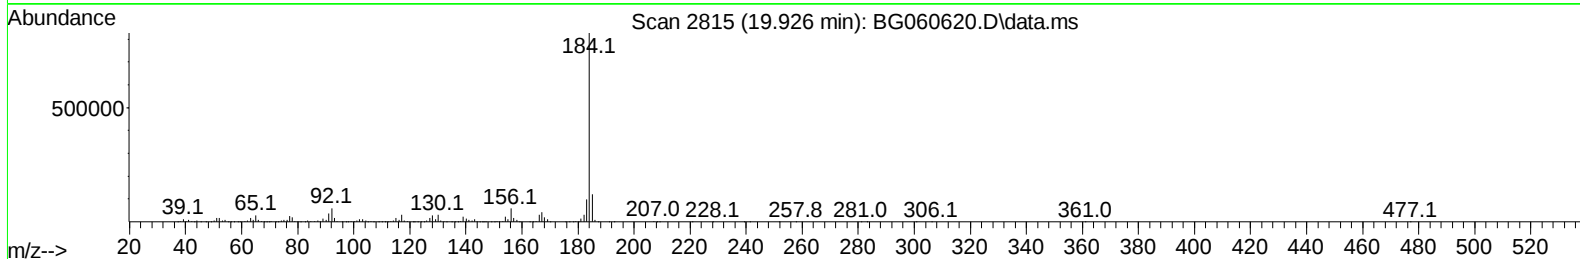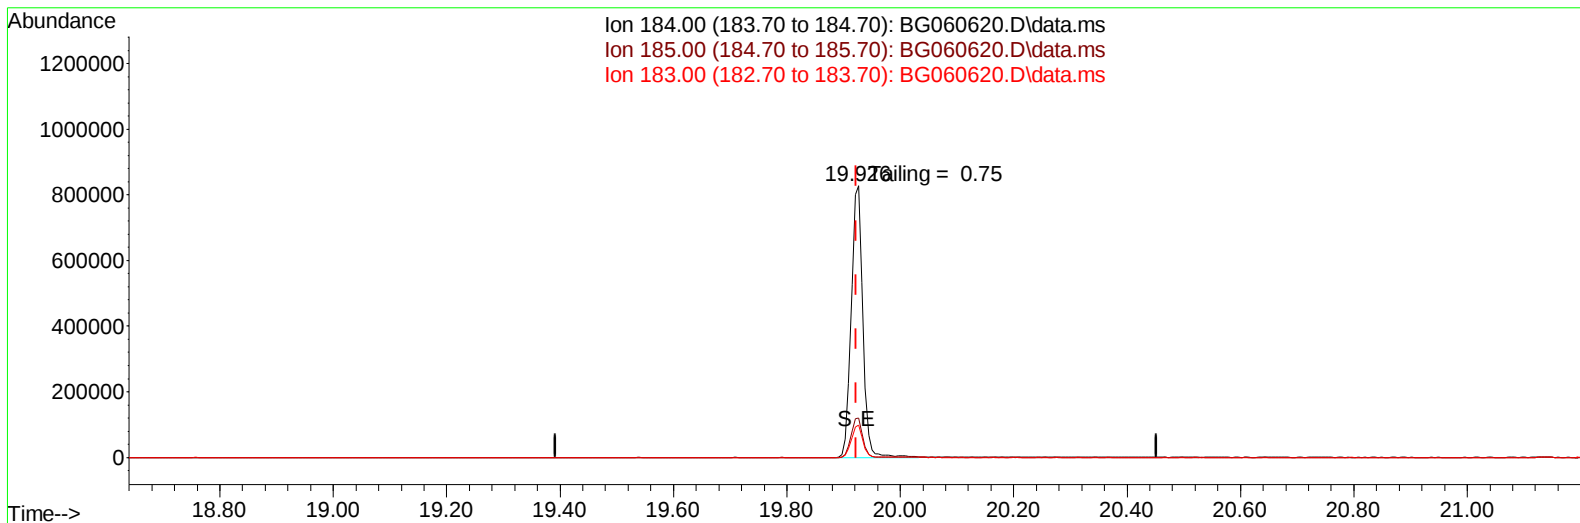

TIC: BG060620.D\data.ms

(77) Benzidine

19.926min (+ 0.004) 5804.20 ng

response **1176934**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.62
183.00	11.50	11.86
0.00	0.00	0.00