
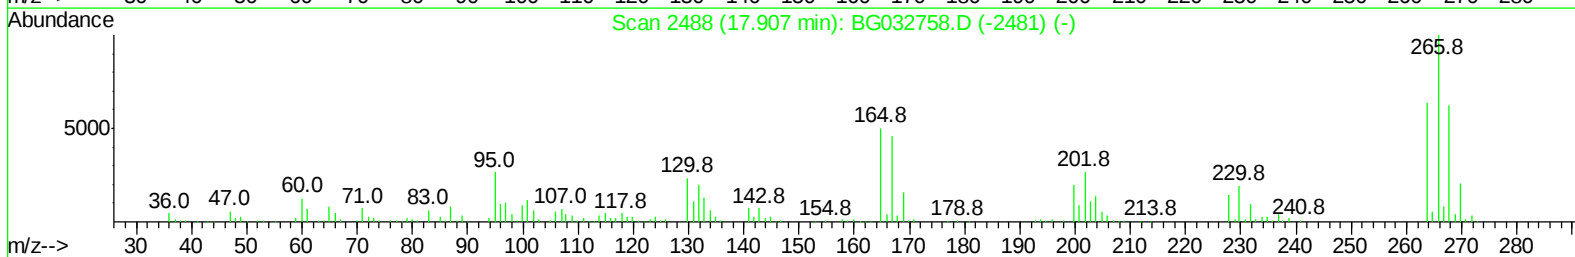
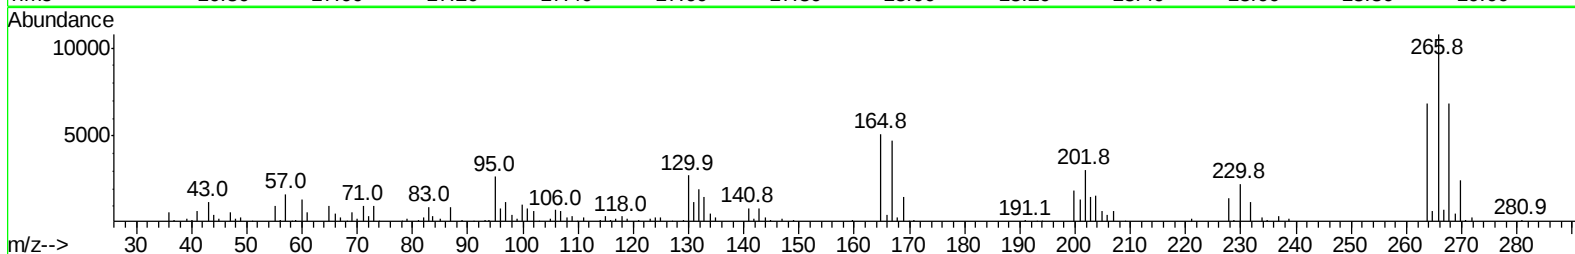


Data Path : Z:\HPCHEM1\BNA G\DATA\BG031418\  
Data File : BG033142.D  
Acq On : 14 Mar 2018 11:19  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 05:28:06 2018  
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Mar 14 13:59:34 2018  
Response via : Initial Calibration

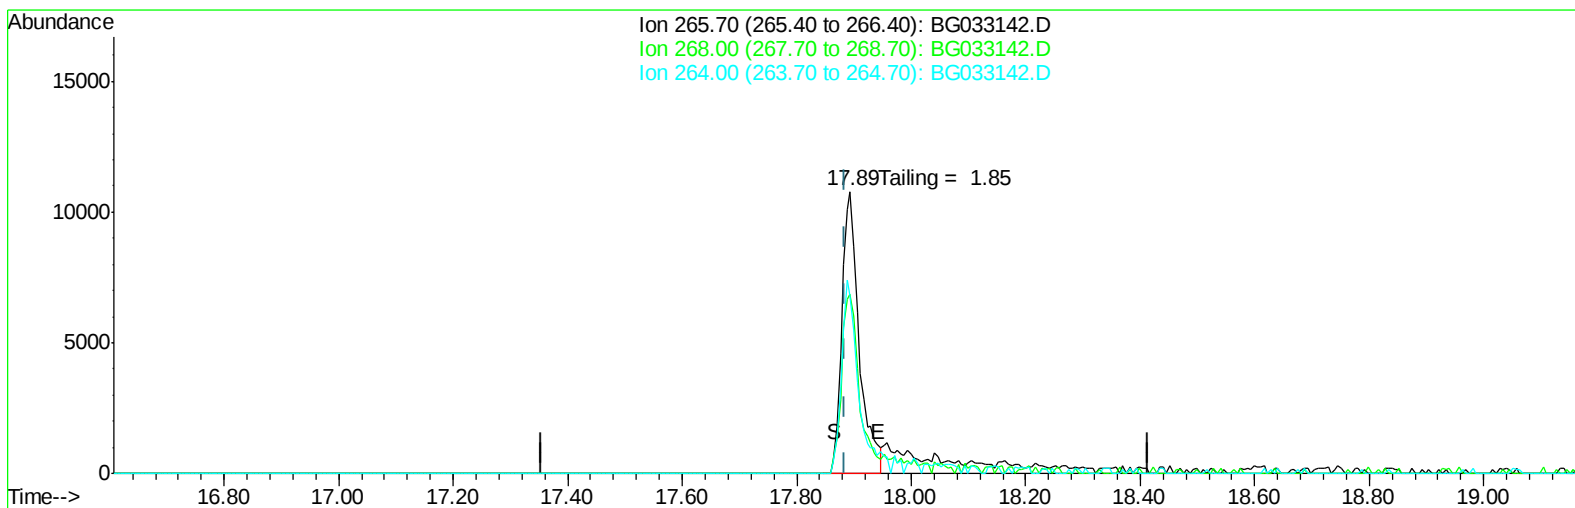

TIC: BG033142.D

(69) Pentachlorophenol (C)




17.894min (+0.008) 48418.30ng

response 22652

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 63.64 |
| 264.00 | 62.00 | 63.27 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA G\DATA\BG031418\  
Data File : BG033142.D  
Acq On : 14 Mar 2018 11:19  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 05:28:06 2018  
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Mar 14 13:59:34 2018  
Response via : Initial Calibration

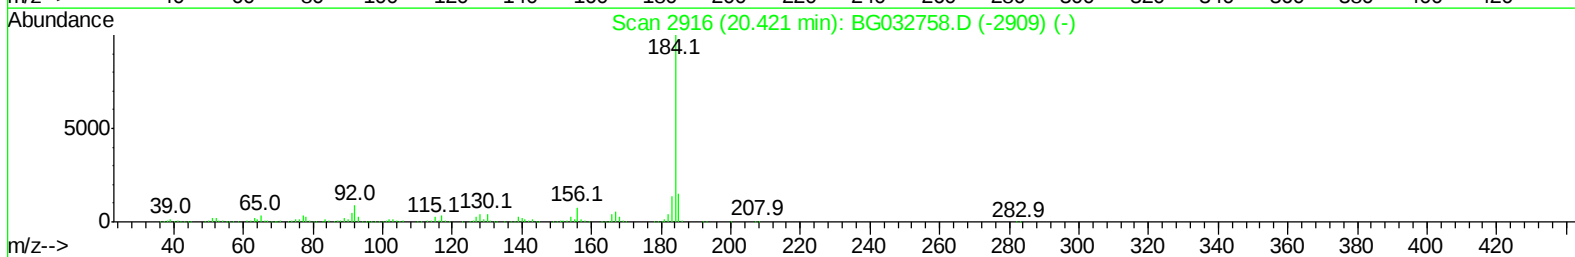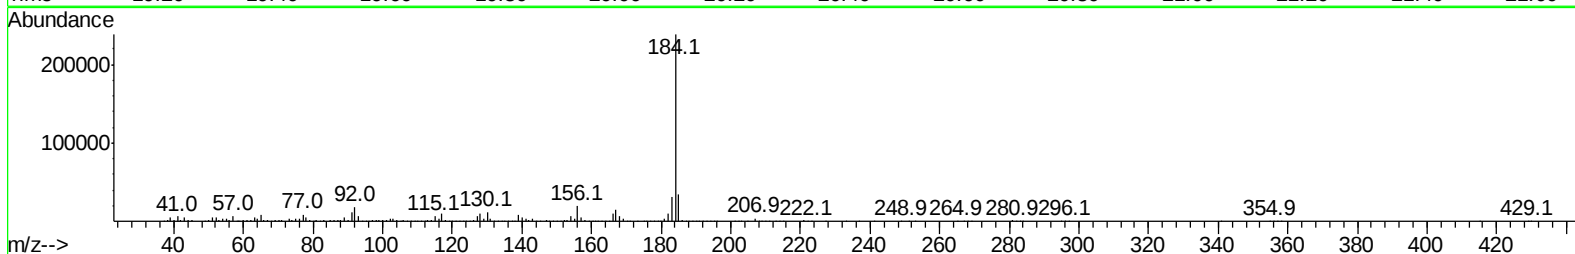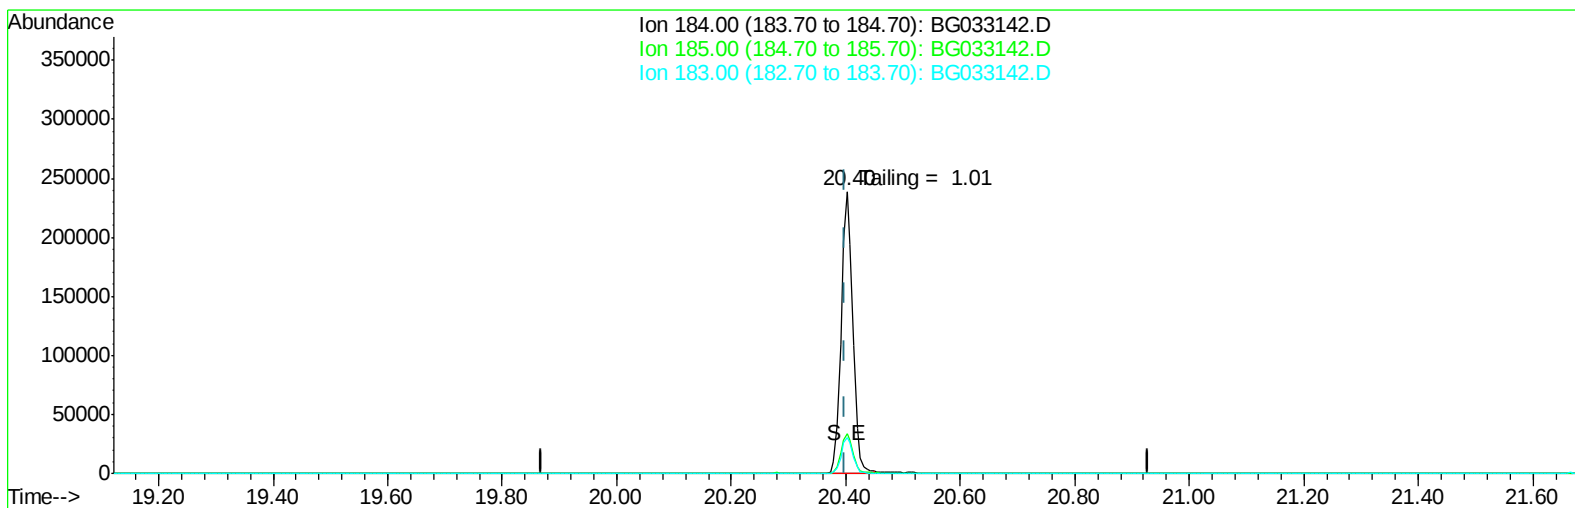

TIC: BG033142.D

(76) Benzidine

20.402min (+0.003) 14323.84ng

response 342265

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 13.90 | 14.25 |
| 183.00 | 13.30 | 12.76 |
| 0.00   | 0.00  | 0.00  |