
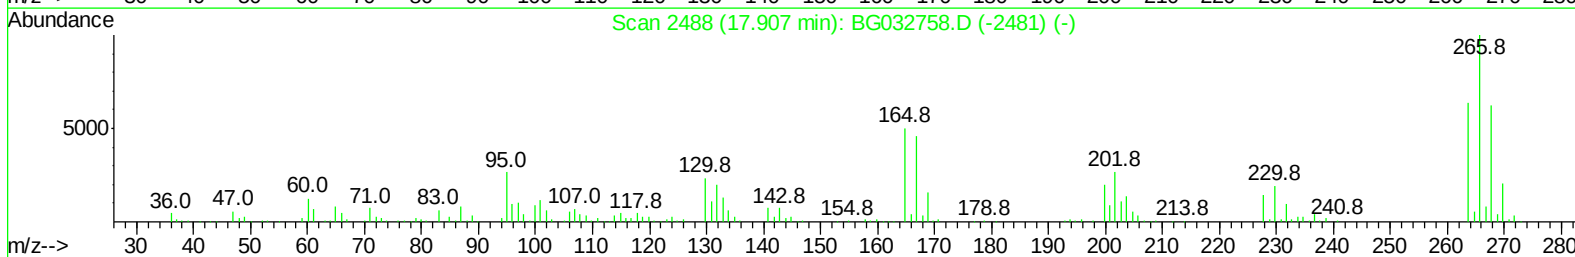
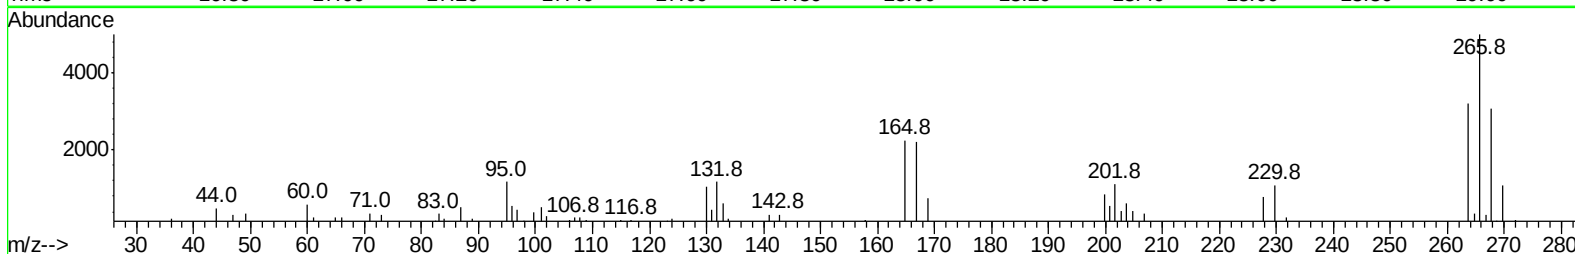


Data Path : Z:\HPCHEM1\BNA G\DATA\BG031418\
Data File : BG033160.D
Acq On : 15 Mar 2018 1:19
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 05:29:32 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 14 13:59:34 2018
Response via : Initial Calibration

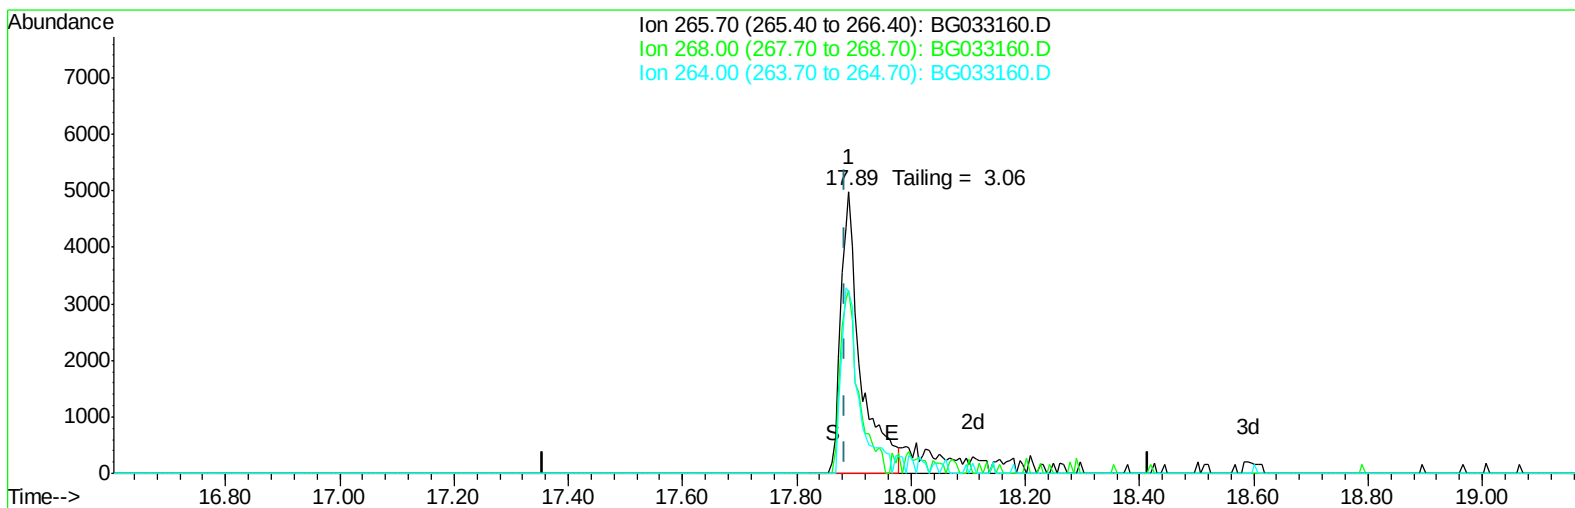

TIC: BG033160.D

(69) Pentachlorophenol (C)




17.891min (+0.005) 8537.19ng

response 12105

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.15
264.00	62.00	64.49
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG031418\
Data File : BG033160.D
Acq On : 15 Mar 2018 1:19
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 05:29:32 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 14 13:59:34 2018
Response via : Initial Calibration

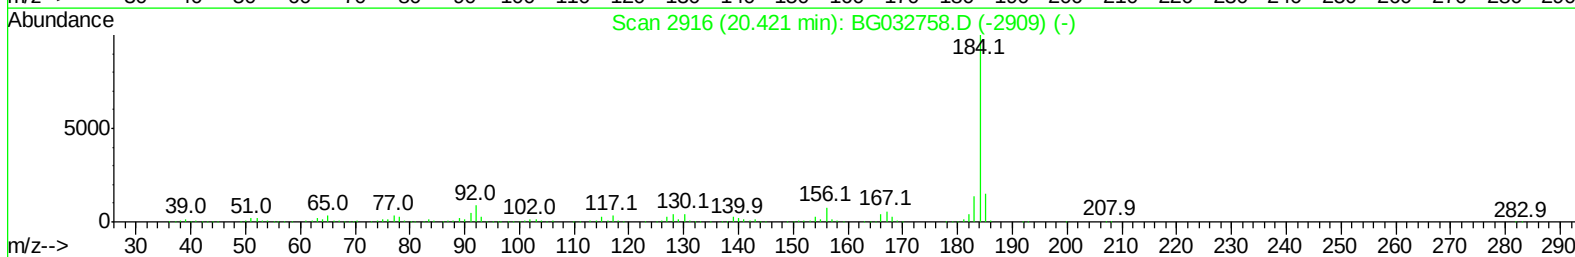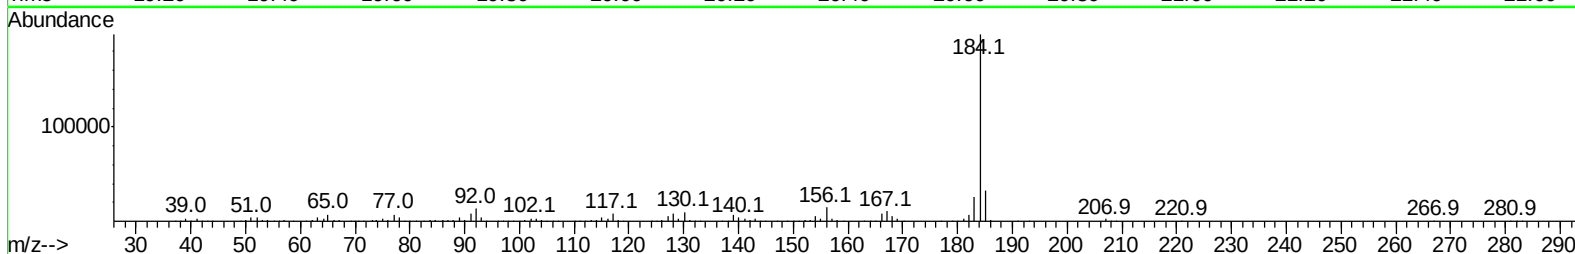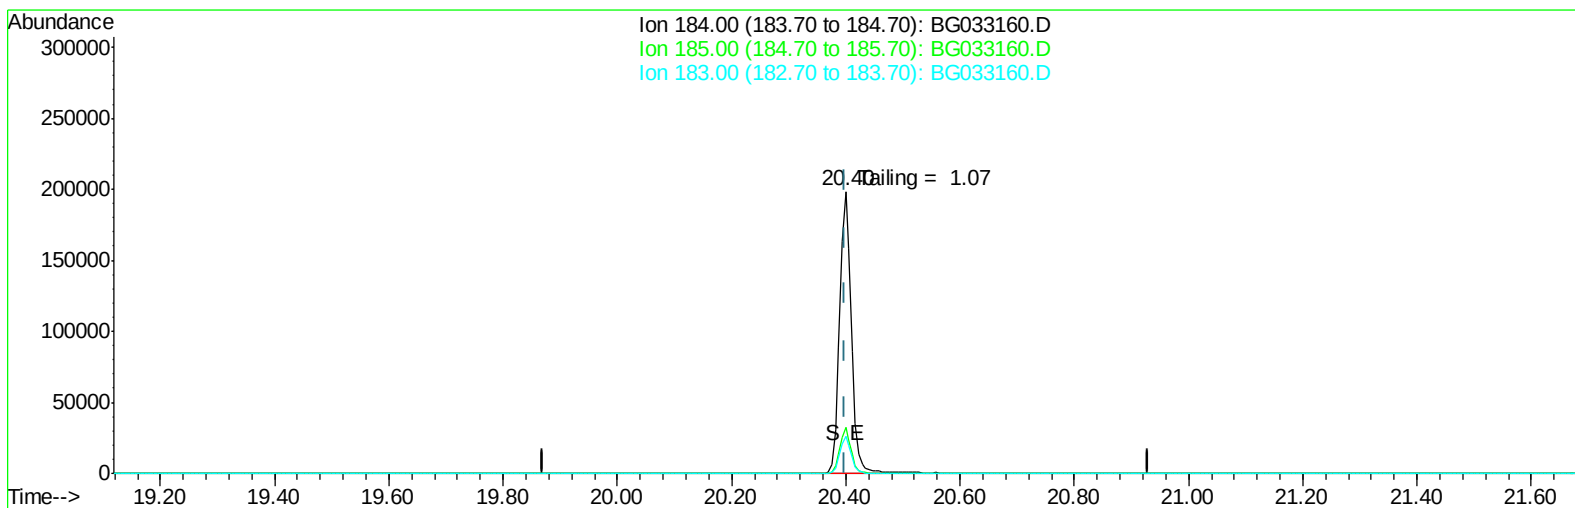

TIC: BG033160.D

(76) Benzidine

20.399min (-0.000) 0.00ng

response 286326

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	16.35
183.00	13.30	13.29
0.00	0.00	0.00