


Data Path : Z:\HPCHEM1\BNA G\DATA\BG031418\
 Data File : BG033142.D
 Acq On : 14 Mar 2018 11:19
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 14 13:59:34 2018

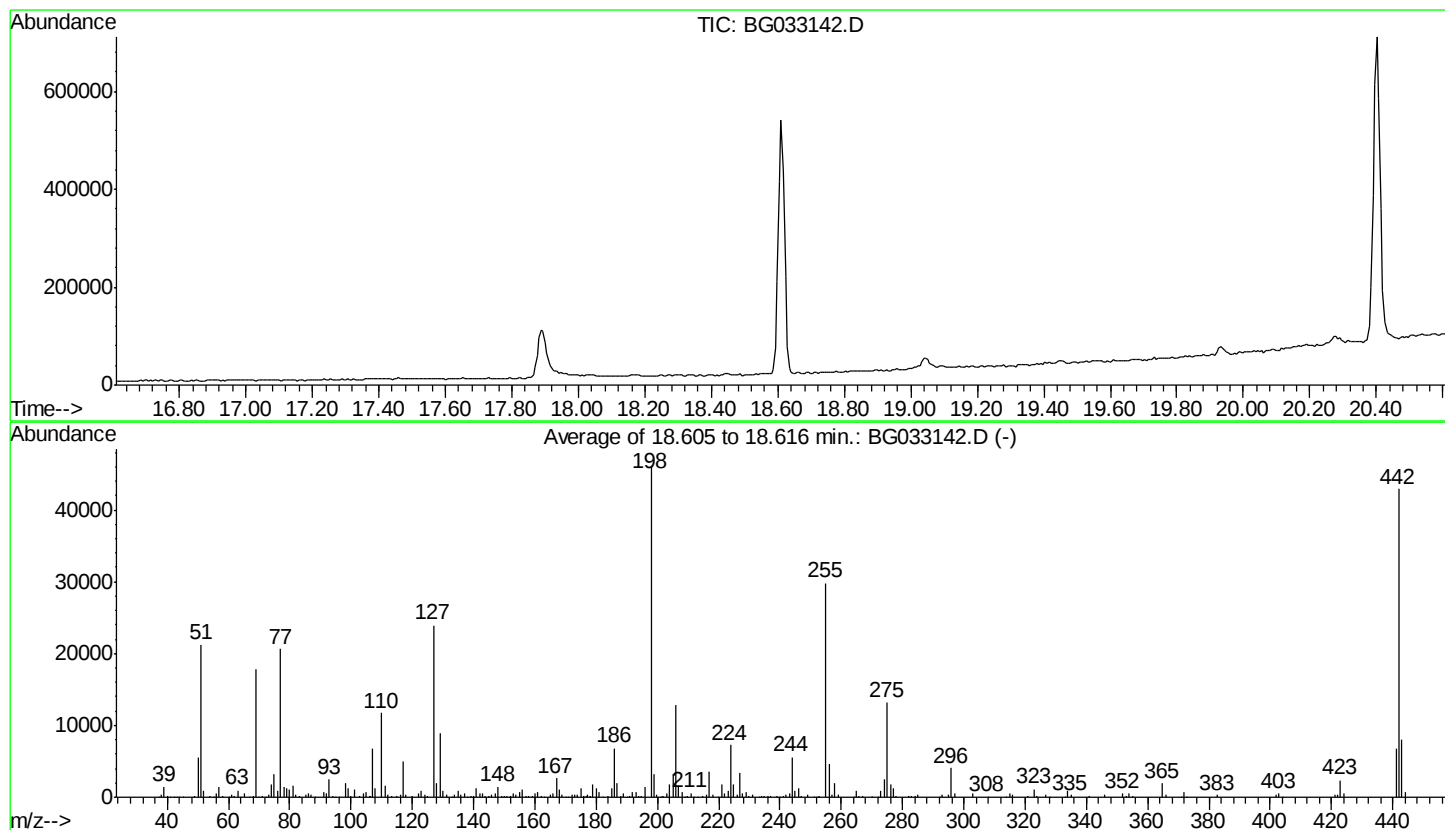

AutoFind: Scans 2607, 2608, 2609; Background Corrected with Scan 2601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.1	21292	PASS
68	69	0.00	2	0.8	136	PASS
69	198	0.00	100	38.5	17772	PASS
70	69	0.00	2	0.2	42	PASS
127	198	10	80	51.8	23936	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	46170	PASS
199	198	5	9	7.1	3263	PASS
275	198	10	60	28.4	13131	PASS
365	198	1	100	4.1	1900	PASS
441	442	0.01	24	15.8	6767	PASS
442	198	50	100	92.9	42896	PASS
443	442	15	24	18.7	8034	PASS