


Data Path : Z:\HPCHEM1\BNA G\DATA\BG031418\
 Data File : BG033160.D
 Acq On : 15 Mar 2018 1:19
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 14 13:59:34 2018

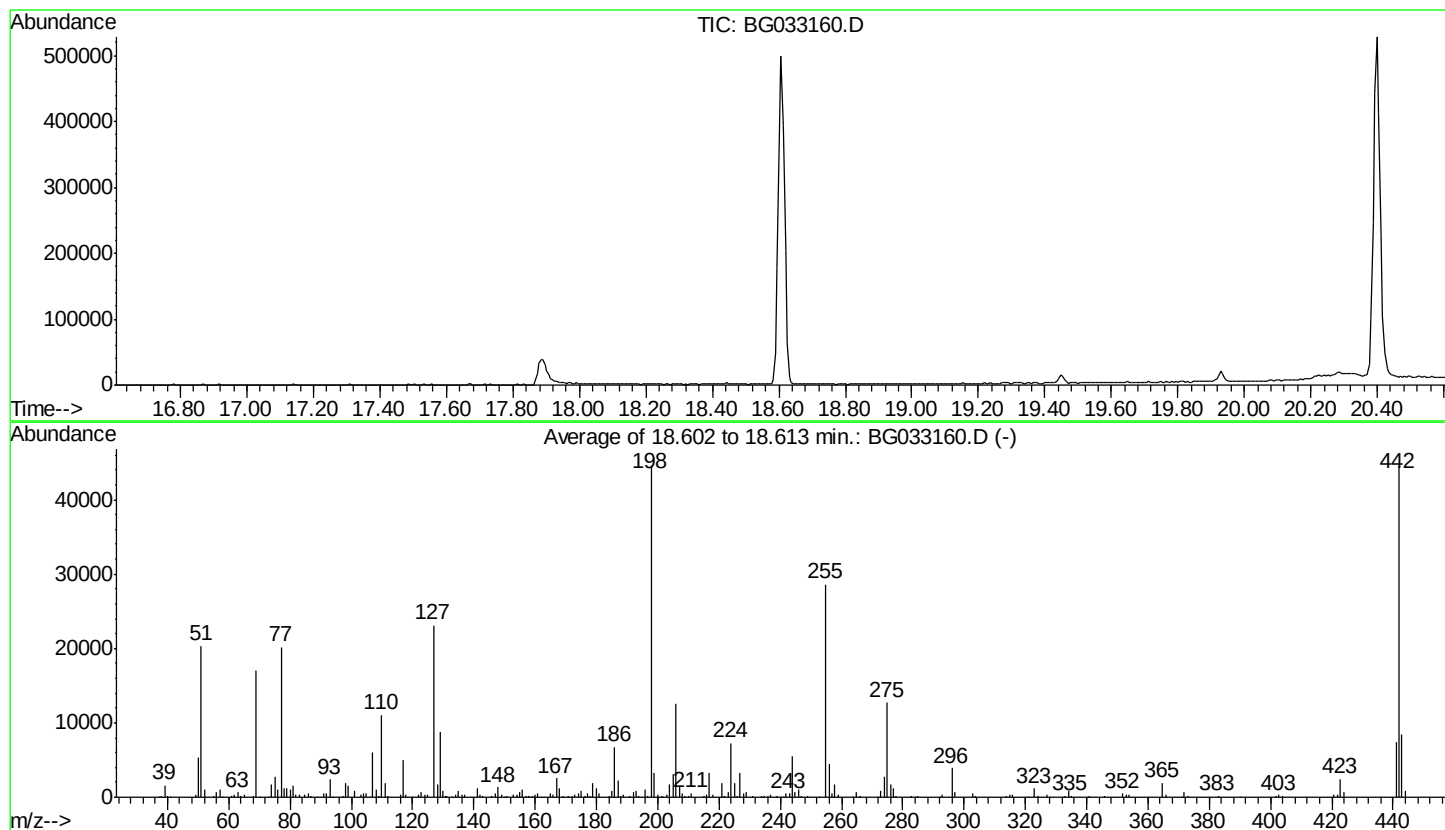

AutoFind: Scans 2607, 2608, 2609; Background Corrected with Scan 2600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.7	20378	PASS
68	69	0.00	2	0.6	103	PASS
69	198	0.00	100	38.1	16978	PASS
70	69	0.00	2	0.3	59	PASS
127	198	10	80	51.9	23152	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	44586	PASS
199	198	5	9	7.4	3310	PASS
275	198	10	60	28.4	12658	PASS
365	198	1	100	4.3	1930	PASS
441	442	0.01	24	16.5	7361	PASS
442	198	50	100	100.0	44581	PASS
443	442	15	24	19.1	8517	PASS