

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG031419\
 Data File : BG039930.D
 Acq On : 14 Mar 2019 18:21
 Operator : JU/SJ
 Sample : K1894-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 RFK-RMAB-MW06-GW

Quant Time: Mar 15 08:10:08 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG030419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 04 14:38:15 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.15	152	42707	20.00	ng	-0.02
21) Naphthalene-d8	10.97	136	179367	20.00	ng	-0.02
39) Acenaphthene-d10	14.77	164	124253	20.00	ng	-0.02
64) Phenanthrene-d10	17.52	188	310055	20.00	ng	-0.02
76) Chrysene-d12	21.80	240	328042	20.00	ng	-0.02
87) Perylene-d12	25.16	264	337225	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.69	112	171940	68.68	ng	-0.02
7) Phenol-d6	7.29	99	161981	43.40	ng	-0.02
23) Nitrobenzene-d5	9.33	82	320784	96.73	ng	-0.02
42) 2,4,6-Tribromophenol	16.26	330	209921	144.95	ng	-0.02
45) 2-Fluorobiphenyl	13.40	172	786617	90.14	ng	-0.02
79) Terphenyl-d14	20.11	244	1295273	86.94	ng	-0.01
Target Compounds						
15) Benzyl Alcohol	8.47	79	6160	2.080	ng	# 49
18) Hexachloroethane	9.24	117	24239	19.308	ng	# 1
19) n-Nitroso-di-n-propylamine	9.33	70	43213	16.084	ng	# 72
24) Nitrobenzene	9.33	77	7723	2.220	ng	# 8
31) Naphthalene	11.02	128	212391	22.365	ng	99
32) Benzoic acid	10.44	122	406	6.794	ng	# 32
33) 4-Chloroaniline	11.02	127	29259	7.266	ng	# 32
37) 2-Methylnaphthalene	12.83	142	62682	8.828	ng	94
38) 1-Methylnaphthalene	12.83	142	62682	9.085	ng	# 93
49) Acenaphthylene	14.84	152	84623	6.705	ng	# 1
52) Acenaphthene	14.84	154	167400	22.037	ng	99
55) Dibenzofuran	15.17	168	143723	11.532	ng	99
56) 4-Nitrophenol	15.17	139	53080	26.799	ng	# 1
58) Fluorene	15.82	166	87378	8.918	ng	96
67) 4-Bromophenyl-phenylether	16.26	248	16363	4.715	ng	# 1
72) Anthracene	17.65	178	57293	3.443	ng	99
73) Carbazole	17.92	167	110233	7.347	ng	95
75) Fluoranthene	19.56	202	72404	3.587	ng	97
77) Benzidine	20.11	184	24052	2.311	ng	96
78) Pvrene	19.92	202	55035	2.582	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG031419\
Data File : BG039930.D
Acq On : 14 Mar 2019 18:21
Operator : JU/SJ
Sample : K1894-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
RFK-RMAB-MW06-GW

Quant Time: Mar 15 08:10:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG030419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 04 14:38:15 2019
Response via : Initial Calibration

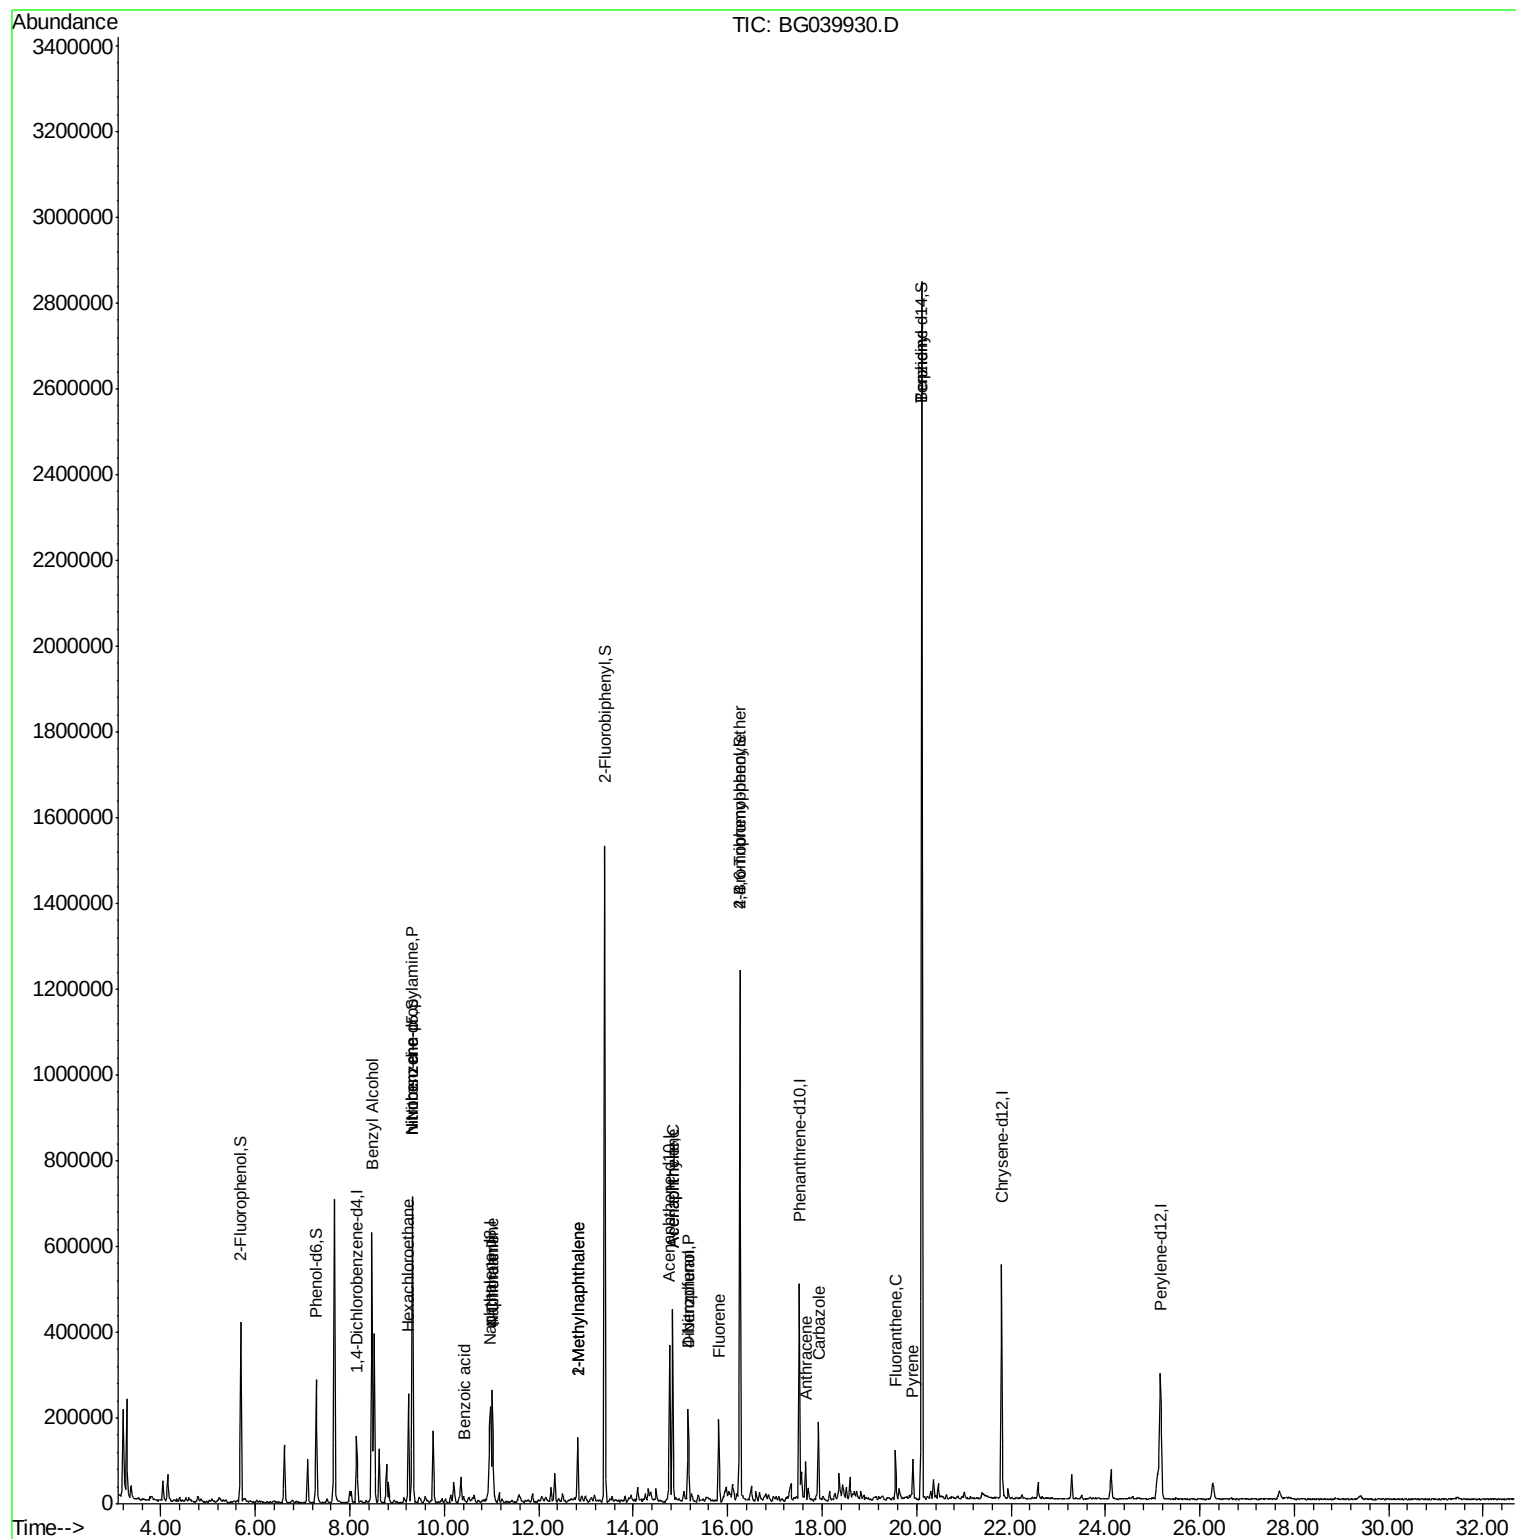




#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.15 min Scan# 861
Delta R.T. -0.02 min
Lab File: BG039930.D
Acq: 14 Mar 2019 18:21

Instrument :
BNA_G
ClientSampleId :
RFK-RMAB-MW06-GW

Tot Ion	Ratio	Lower	Upper
152	100		
150	158.1	123.7	185.5
115	57.5	45.9	68.9






Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

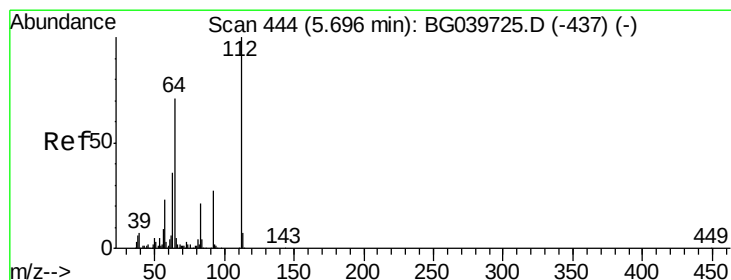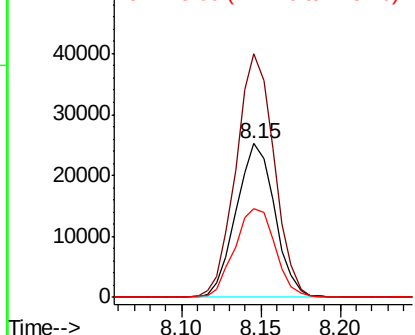

#5

2-Fluorophenol
Concen: 68.685 ng
RT: 5.69 min Scan# 443
Delta R.T. -0.02 min
Lab File: BG039930.D
Acq: 14 Mar 2019 18:21

Tgt Ion	Ratio	Lower	Upper
112	100		
64	71.0	57.8	86.8
63	37.1	29.8	44.6






Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG

Ion 63.00 (62.70 to 63.70): BG

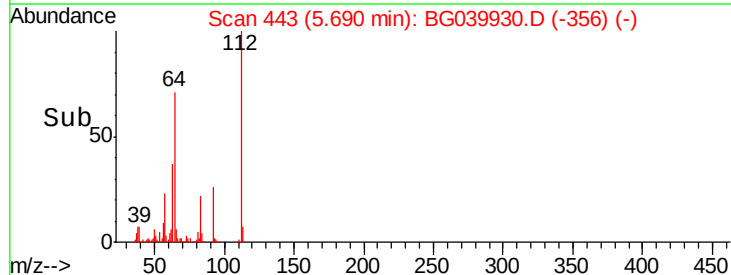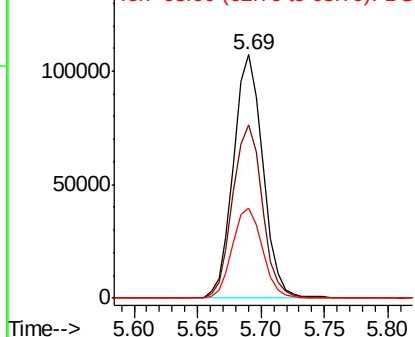



#7

Phenol-d6

Concen: 43.396 ng

RT: 7.29 min Scan# 715

Delta R.T. -0.02 min

Lab File: BG039930.D

Acq: 14 Mar 2019 18:21

Instrument :

BNA_G

ClientSampleId :

RFK-RMAB-MW06-GW


Tot Ion: 99 Resp: 161981

Ion Ratio Lower Upper




99 100

42 21.6 18.2 27.2

71 36.8 28.0 42.0

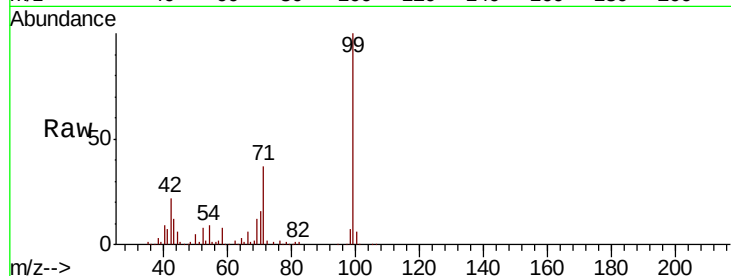

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

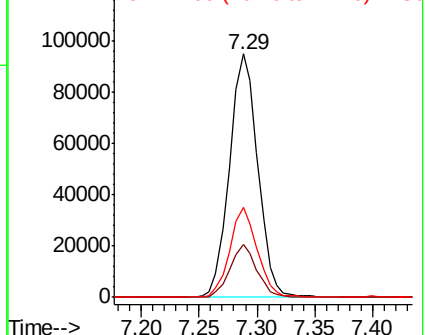

#15

Benzyl Alcohol

Concen: 2.080 ng

RT: 8.47 min Scan# 916

Delta R.T. 0.06 min

Lab File: BG039930.D

Acq: 14 Mar 2019 18:21


Tgt Ion: 79 Resp: 6160

Ion Ratio Lower Upper



79 100


108 34.1 57.8 86.6#

77 108.0 51.1 76.7#



Abundance Ion 79.00 (78.70 to 79.70): BGC
Ion 108.00 (107.70 to 108.70): BGC
Ion 77.00 (76.70 to 77.70): BGC

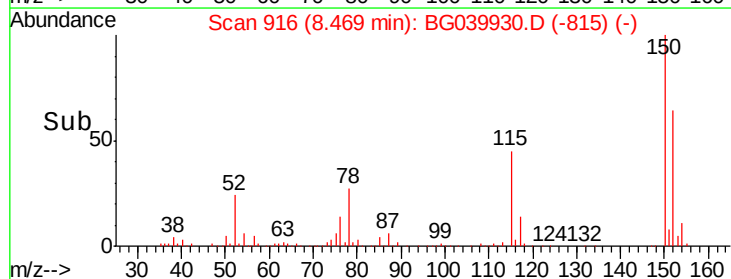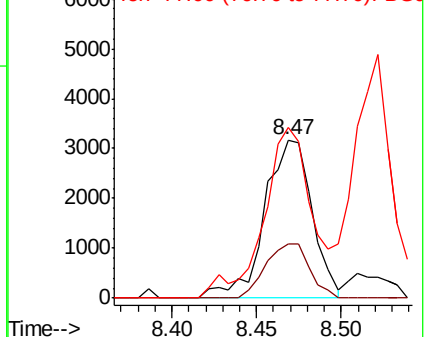

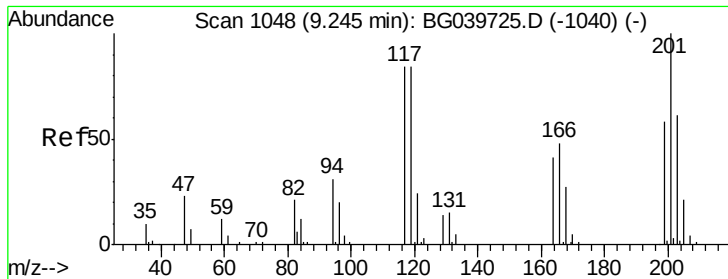

#18

Hexachloroethane

Concen: 19.308 ng

RT: 9.24 min Scan# 1048

Delta R.T. -0.01 min

Lab File: BG039930.D

Acq: 14 Mar 2019 18:21

Instrument :

BNA_G

ClientSampleId :

RFK-RMAB-MW06-GW


Tot Ion:117 Resp: 24239

Ion Ratio Lower Upper

117 100

119 638.1 76.3 114.5#

201 0.0 91.1 136.7#



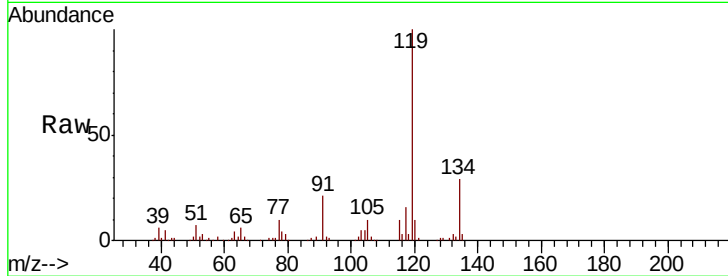


Abundance

Ion 117.00 (116.70 to 117.70): E

Ion 119.00 (118.70 to 119.70): E

Ion 201.00 (200.70 to 201.70): E

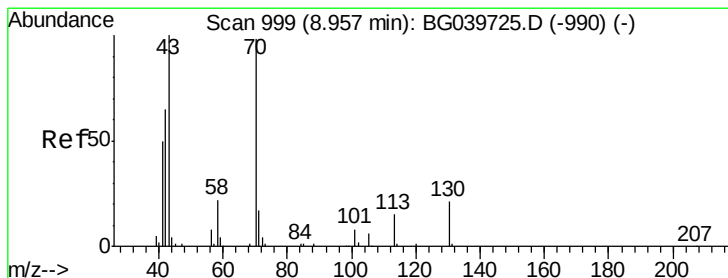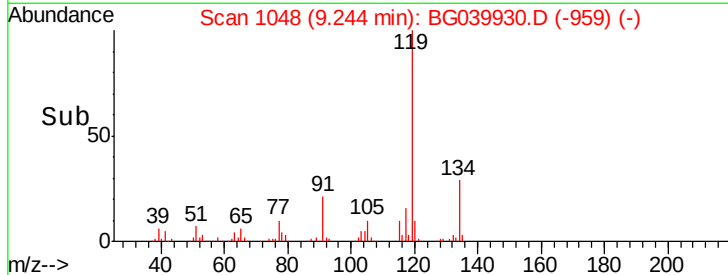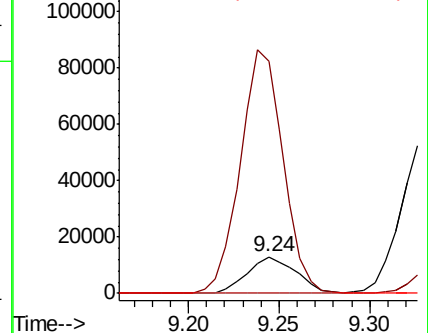

#19

n-Nitroso-di-n-propylamine

Concen: 16.084 ng

RT: 9.33 min Scan# 1062

Delta R.T. 0.36 min

Lab File: BG039930.D

Acq: 14 Mar 2019 18:21

Tgt Ion: 70 Resp: 43213


Ion Ratio Lower Upper

70 100

42 52.0 60.4 90.6#

101 1.9 7.5 11.3#

130 4.7 16.9 25.3#

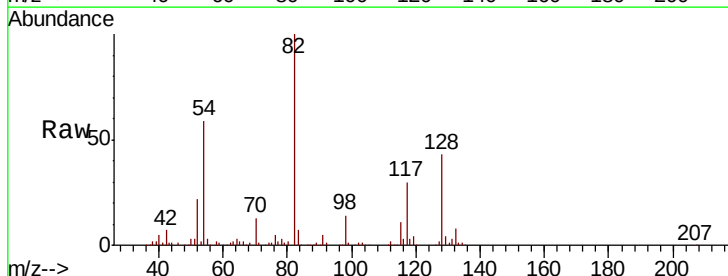



Abundance


Ion 70.00 (69.70 to 70.70): BGC

Ion 42.00 (41.70 to 42.70): BGC

Ion 101.00 (100.70 to 101.70): BGC

Ion 130.00 (129.70 to 130.70): BGC

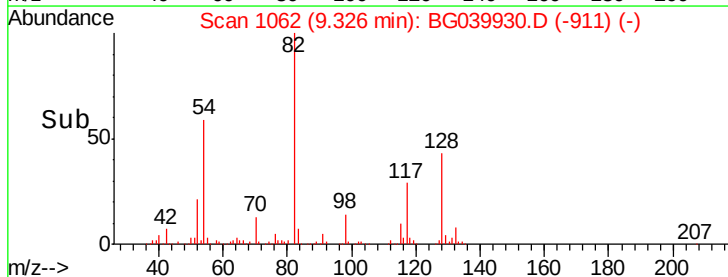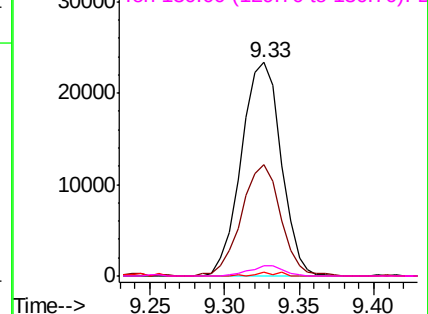


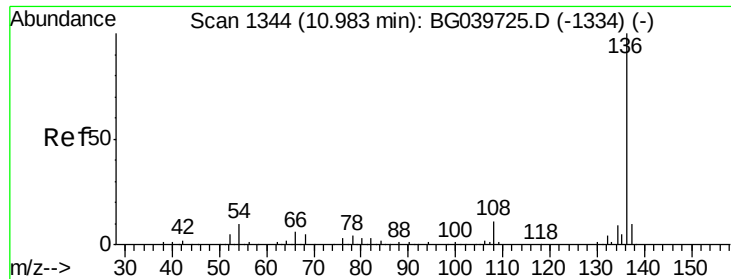




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.97 min Scan# 1341
Delta R.T. -0.02 min
Lab File: BG039930.D
Acq: 14 Mar 2019 18:21

Instrument :
BNA_G
ClientSampleId :
RFK-RMAB-MW06-GW

Tot Ion:136	Resp:	179367
Ion Ratio	Lower	Upper
136	100	
137	11.7	9.1 13.7
54	10.5	9.4 14.2
68	6.0	4.2 6.4

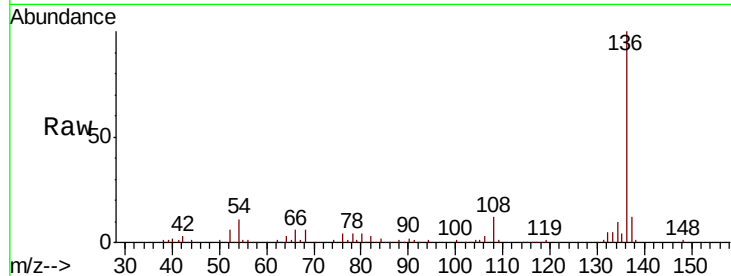


Abundance Ion 136.00 (135.70 to 136.70): E
150000
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC


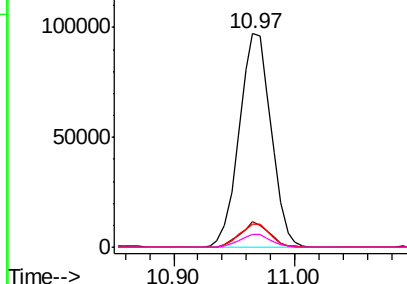



#23
Nitrobenzene-d5
Concen: 96.725 ng
RT: 9.33 min Scan# 1062
Delta R.T. -0.02 min
Lab File: BG039930.D
Acq: 14 Mar 2019 18:21

Tgt Ion: 82	Resp:	320784
Ion Ratio	Lower	Upper
82	100	
128	43.4	31.3 46.9
54	59.4	50.9 76.3



Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC

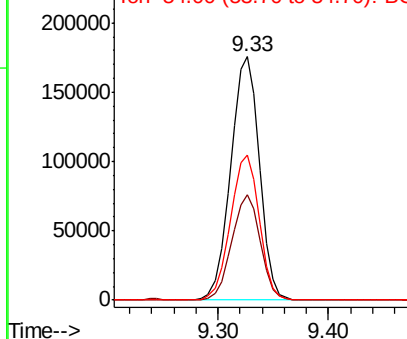



#24

Nitrobenzene

Concen: 2.220 ng

RT: 9.33 min Scan# 1063

Delta R.T. -0.05 min

Lab File: BG039930.D

Acq: 14 Mar 2019 18:21

Instrument :

BNA_G

ClientSampleId :

RFK-RMAB-MW06-GW


Tot Ion: 77 Resp: 7723

Ion Ratio Lower Upper




77 100

123 0.0 34.1 51.1#

65 82.7 12.3 18.5#



Abundance Ion 77.00 (76.70 to 77.70): BGC
Ion 123.00 (122.70 to 123.70): BGC
Ion 65.00 (64.70 to 65.70): BGC

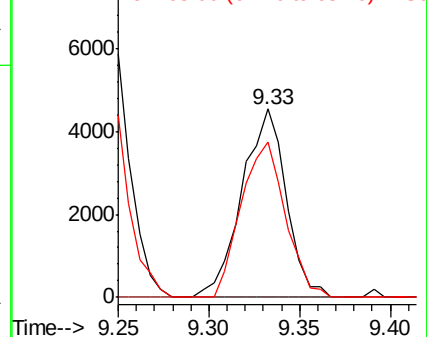

#31

Naphthalene

Concen: 22.365 ng

RT: 11.02 min Scan# 1350

Delta R.T. -0.02 min

Lab File: BG039930.D

Acq: 14 Mar 2019 18:21


Tgt Ion: 128 Resp: 212391

Ion Ratio Lower Upper



128 100


129 11.7 8.7 13.1

127 13.8 10.8 16.2



Abundance Ion 128.00 (127.70 to 128.70): BGC
Ion 129.00 (128.70 to 129.70): BGC
Ion 127.00 (126.70 to 127.70): BGC




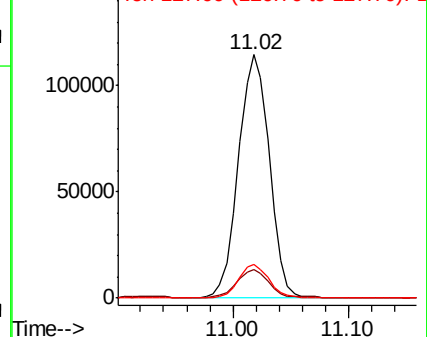


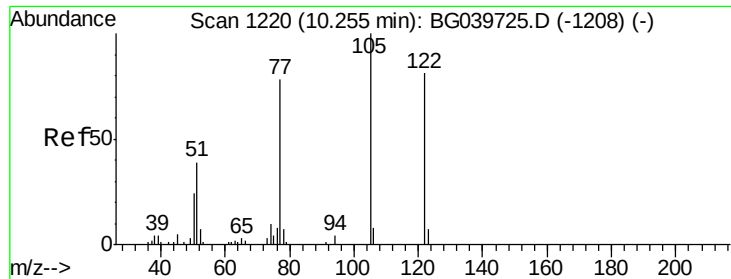

#32
Benzoic acid
Concen: 6.794 ng
RT: 10.44 min Scan# 1251
Delta R.T. 0.18 min
Lab File: BG039930.D
Acq: 14 Mar 2019 18:21




Instrument :
BNA_G
ClientSampleId :
RFK-RMAB-MW06-GW


Tot Ion	Ratio	Lower	Upper
122	100		
105	0.0	101.8	141.8#
77	81.2	76.3	116.3

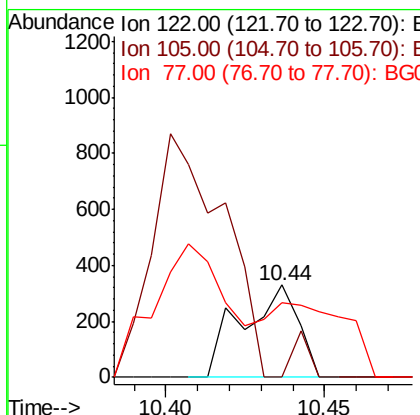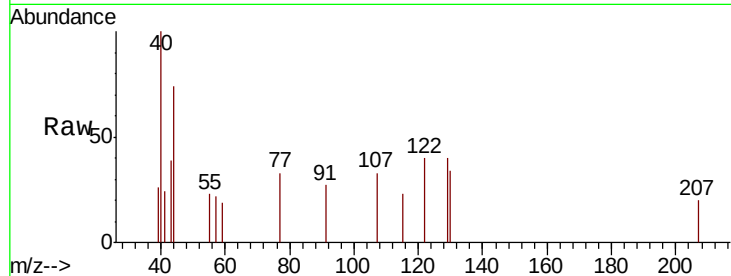

#33
4-Chloroaniline
Concen: 7.266 ng
RT: 11.02 min Scan# 1350
Delta R.T. -0.13 min
Lab File: BG039930.D
Acq: 14 Mar 2019 18:21

Tgt Ion	Ratio	Lower	Upper
127	100		
129	85.3	27.0	40.4#
65	0.0	28.8	43.2#
92	0.0	16.6	25.0#


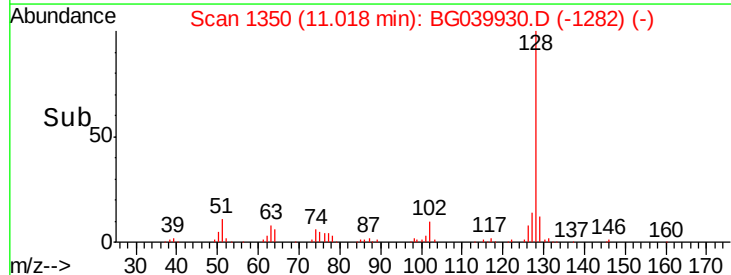
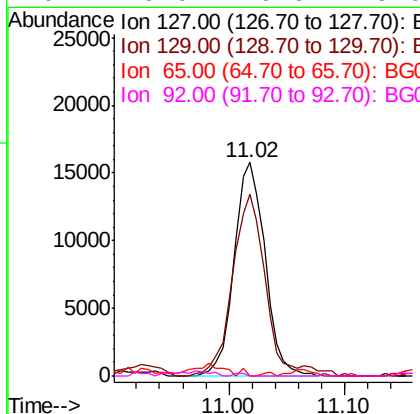



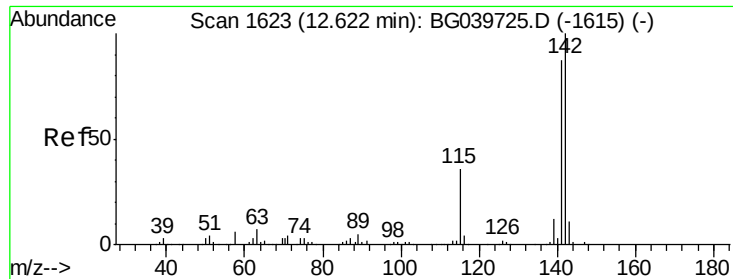

#37
2-Methylnaphthalene
Concen: 8.828 ng
RT: 12.83 min Scan# 1658
Delta R.T. 0.20 min
Lab File: BG039930.D
Acq: 14 Mar 2019 18:21




Instrument :
BNA_G
ClientSampleId :
RFK-RMAB-MW06-GW


Tot Ion:142 Resp: 62682
Ion Ratio Lower Upper
142 100
141 99.5 73.5 110.3
115 39.8 30.8 46.2

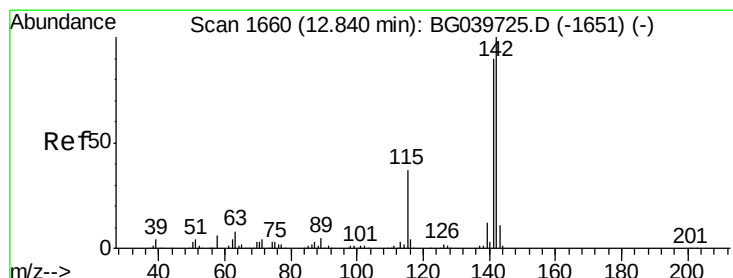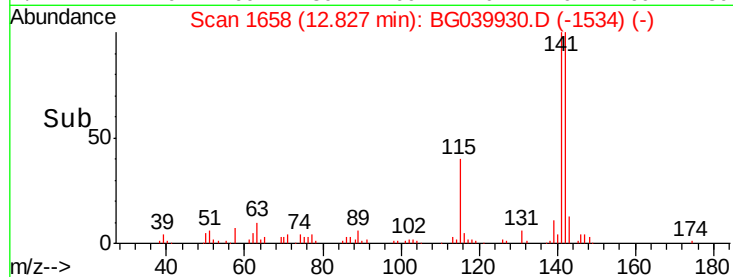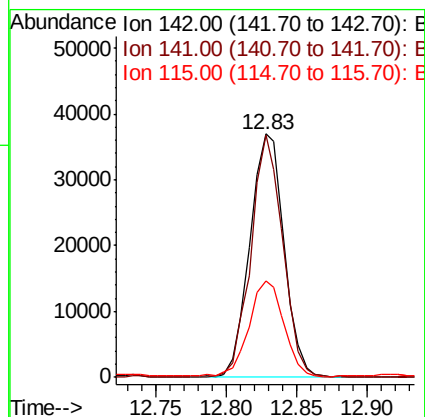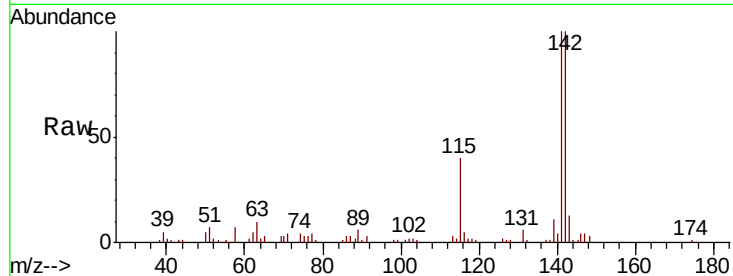

#38
1-Methylnaphthalene
Concen: 9.085 ng
RT: 12.83 min Scan# 1658
Delta R.T. -0.02 min
Lab File: BG039930.D
Acq: 14 Mar 2019 18:21

Tgt Ion:142 Resp: 62682
Ion Ratio Lower Upper
142 100
141 99.5 74.2 111.4
116 5.1 3.0 4.6#

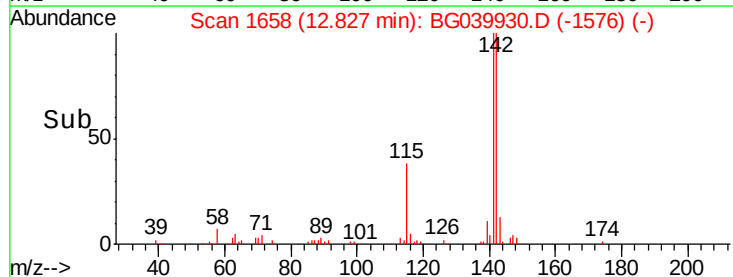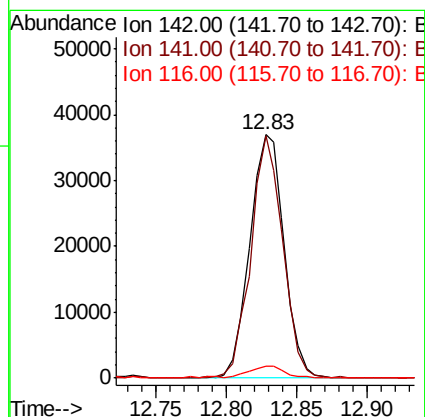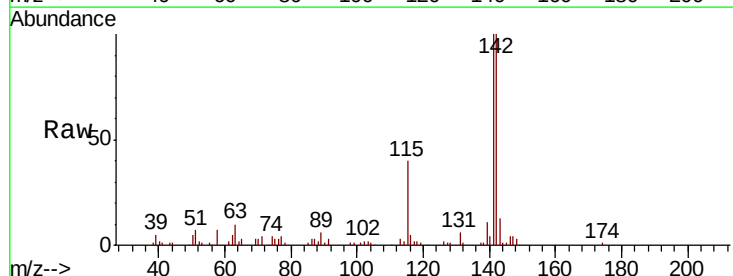



#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.77 min Scan# 1989

Delta R.T. -0.02 min

Lab File: BG039930.D

Acq: 14 Mar 2019 18:21

Instrument :

BNA_G

ClientSampleId :

RFK-RMAB-MW06-GW


Tot Ion:164 Resp: 124253

Ion Ratio Lower Upper

164 100

162 101.5 81.6 122.4




160 43.1 34.2 51.2



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

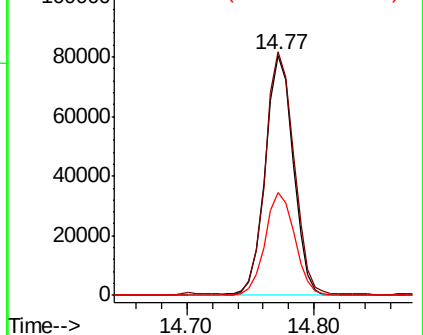

#42

2,4,6-Tribromophenol

Concen: 144.947 ng

RT: 16.26 min Scan# 2242

Delta R.T. -0.02 min

Lab File: BG039930.D

Acq: 14 Mar 2019 18:21


Tgt Ion:330 Resp: 209921

Ion Ratio Lower Upper

330 100

332 97.6 75.7 113.5



141 42.5 35.6 53.4




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E




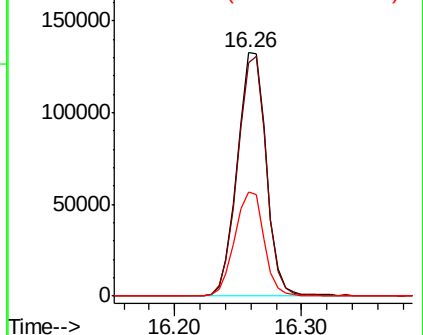


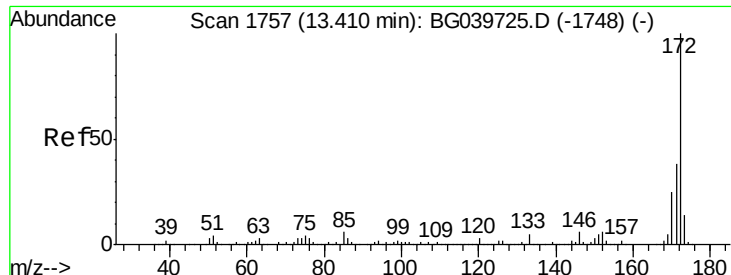

#45
2-Fluorobiphenyl
Concen: 90.139 ng
RT: 13.40 min Scan# 1755
Delta R.T. -0.02 min
Lab File: BG039930.D
Acq: 14 Mar 2019 18:21




Instrument :
BNA_G
ClientSampleId :
RFK-RMAB-MW06-GW


Tot Ion	Ratio	Lower	Upper
172	100		
171	37.6	30.8	46.2
170	25.1	20.2	30.4

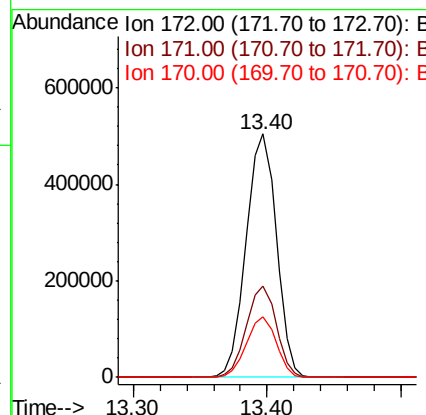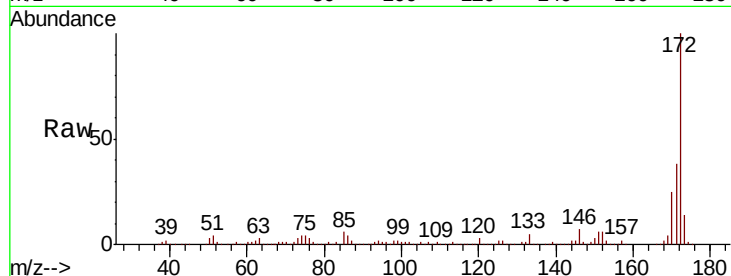

#49
Acenaphthylene
Concen: 6.705 ng
RT: 14.84 min Scan# 2000
Delta R.T. 0.32 min
Lab File: BG039930.D
Acq: 14 Mar 2019 18:21

Tgt Ion	Ratio	Lower	Upper
152	100		
151	37.2	16.8	25.2#
153	222.8	11.7	17.5#

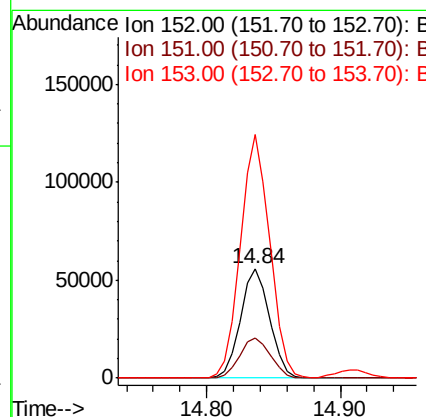

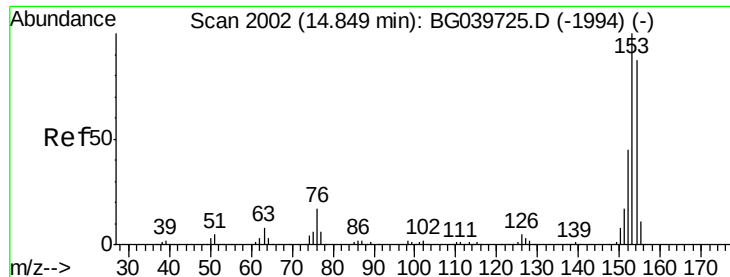

#52

Acenaphthene

Concen: 22.037 ng

RT: 14.84 min Scan# 2000

Delta R.T. -0.02 min

Lab File: BG039930.D

Acq: 14 Mar 2019 18:21

Instrument :

BNA_G

ClientSampleId :

RFK-RMAB-MW06-GW


Tot Ion:154 Resp: 167400

Ion Ratio Lower Upper

154 100

153 114.2 90.1 135.1




152 51.3 40.9 61.3

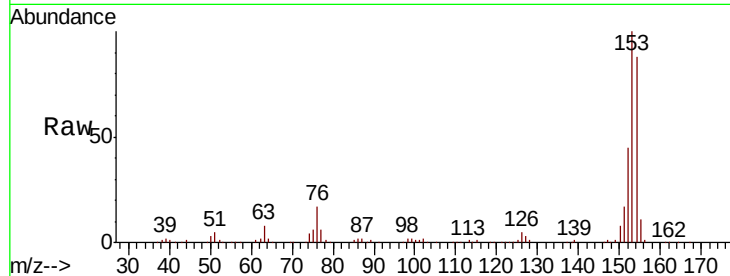

Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

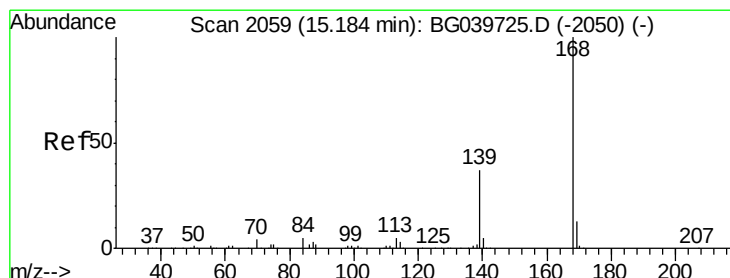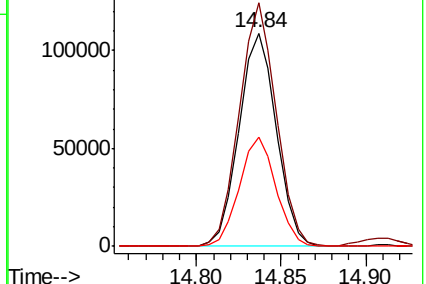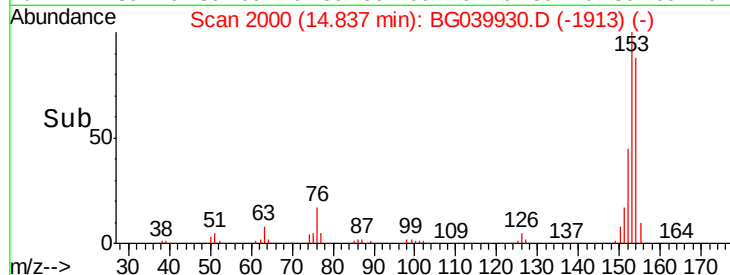

#55

Dibenzofuran

Concen: 11.532 ng

RT: 15.17 min Scan# 2056

Delta R.T. -0.02 min

Lab File: BG039930.D

Acq: 14 Mar 2019 18:21


Tgt Ion:168 Resp: 143723

Ion Ratio Lower Upper

168 100

139 37.2 30.1 45.1



169 13.0 10.6 16.0

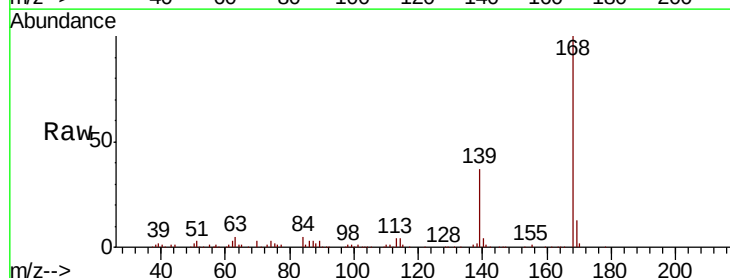


Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 169.00 (168.70 to 169.70): E

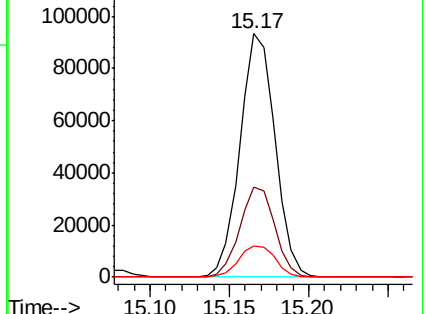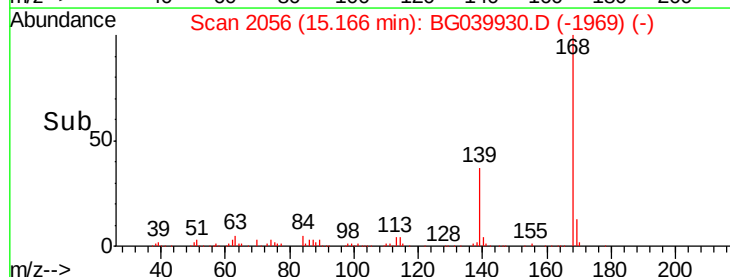







#56
4-Nitrophenol
Concen: 26.799 ng
RT: 15.17 min Scan# 2056
Delta R.T. 0.18 min
Lab File: BG039930.D
Acq: 14 Mar 2019 18:21

Instrument :
BNA_G
ClientSampleId :
RFK-RMAB-MW06-GW

Tot Ion:139 Resp: 53080
Ion Ratio Lower Upper
139 100
109 1.1 61.9 101.9#
65 2.0 99.1 139.1#




Abundance Ion 139.00 (138.70 to 139.70): E
Ion 109.00 (108.70 to 109.70): E
Ion 65.00 (64.70 to 65.70): BGC


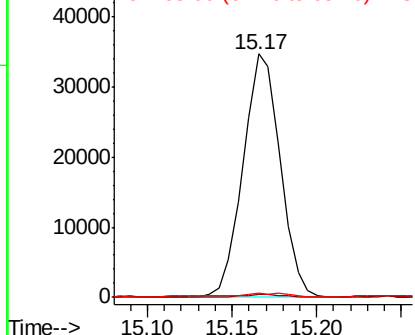



#58
Fluorene
Concen: 8.918 ng
RT: 15.82 min Scan# 2167
Delta R.T. -0.02 min
Lab File: BG039930.D
Acq: 14 Mar 2019 18:21

Tgt Ion:166 Resp: 87378
Ion Ratio Lower Upper
166 100
165 93.0 77.9 116.9
167 13.7 10.8 16.2



Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E




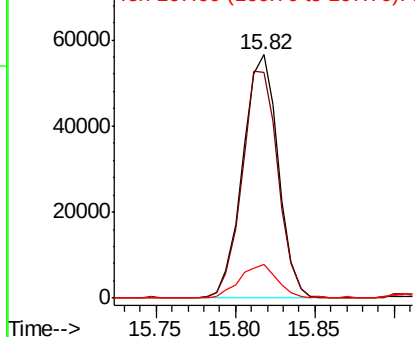




#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.52 min Scan# 2456
 Delta R.T. -0.02 min
 Lab File: BG039930.D
 Acq: 14 Mar 2019 18:21




Instrument :
 BNA_G
 ClientSampleId :
 RFK-RMAB-MW06-GW


Tot Ion:188 Resp: 310055
 Ion Ratio Lower Upper
 188 100
 94 8.4 6.9 10.3
 80 9.3 8.1 12.1

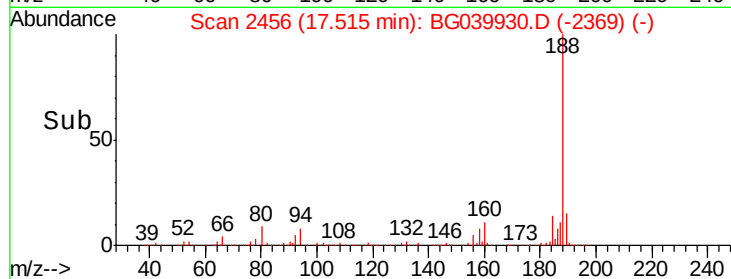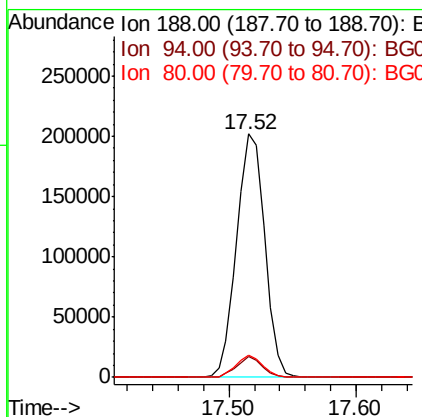

#67
 4-Bromophenyl-phenylether
 Concen: 4.715 ng
 RT: 16.26 min Scan# 2243
 Delta R.T. -0.45 min
 Lab File: BG039930.D
 Acq: 14 Mar 2019 18:21

Tgt Ion:248 Resp: 16363
 Ion Ratio Lower Upper
 248 100
 250 186.1 77.6 116.4#
 141 517.2 63.9 95.9#

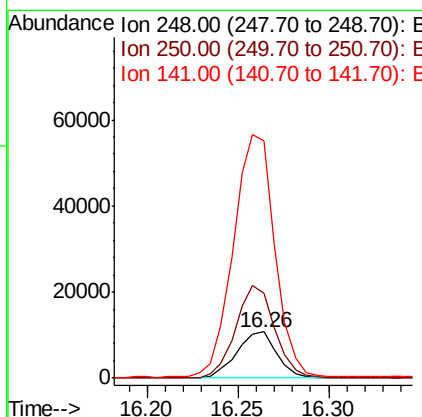

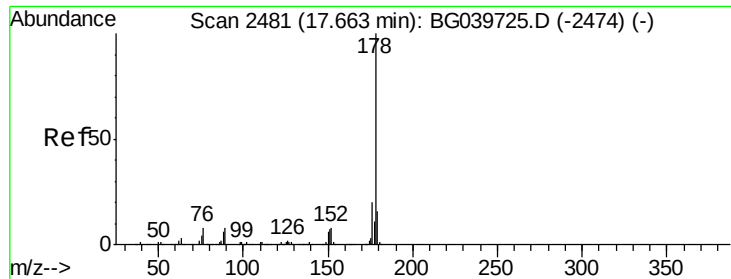

#72

Anthracene

Concen: 3.443 ng

RT: 17.65 min Scan# 2479

Delta R.T. -0.02 min

Lab File: BG039930.D

Acq: 14 Mar 2019 18:21

Instrument :

BNA_G

ClientSampleId :

RFK-RMAB-MW06-GW


Tot Ion:178 Resp: 57293

Ion Ratio Lower Upper

178 100

176 19.7 15.8 23.6




179 16.2 12.5 18.7

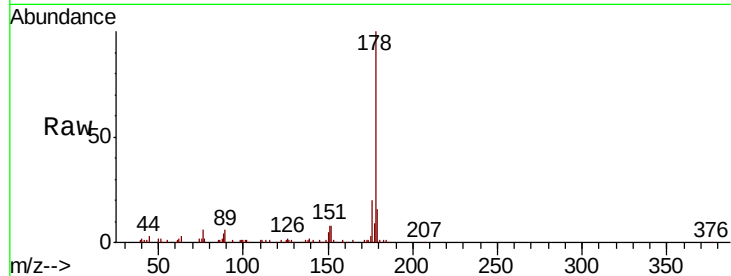

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

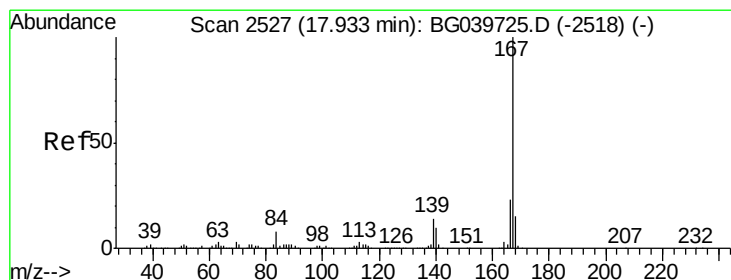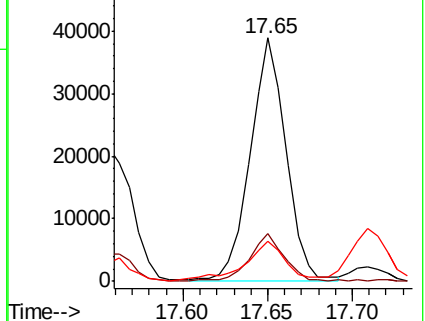

#73

Carbazole

Concen: 7.347 ng

RT: 17.92 min Scan# 2525

Delta R.T. -0.02 min

Lab File: BG039930.D

Acq: 14 Mar 2019 18:21


Tgt Ion:167 Resp: 110233

Ion Ratio Lower Upper

167 100

166 21.0 19.4 29.2



139 14.0 10.8 16.2




Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

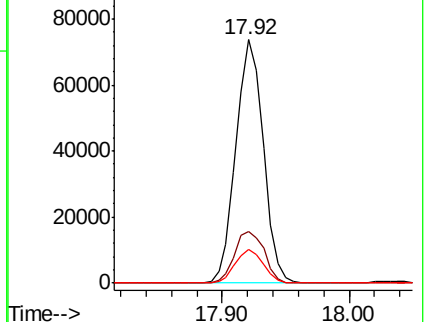



#75

Fluoranthene

Concen: 3.587 ng

RT: 19.56 min Scan# 2804

Delta R.T. -0.02 min

Lab File: BG039930.D

Acq: 14 Mar 2019 18:21

Instrument :

BNA_G

ClientSampleId :

RFK-RMAB-MW06-GW


Tot Ion:202 Resp: 72404

Ion Ratio Lower Upper

202 100

101 7.7 0.0 30.0




203 18.0 0.0 38.9

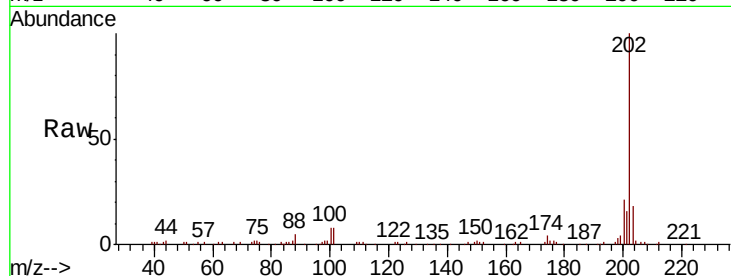

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

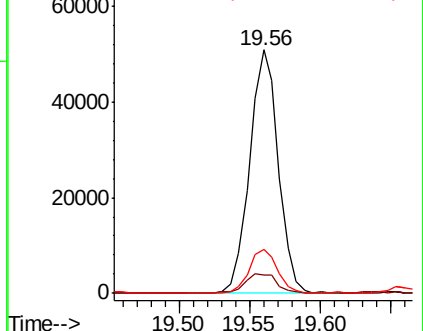

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.80 min Scan# 3186

Delta R.T. -0.02 min

Lab File: BG039930.D

Acq: 14 Mar 2019 18:21


Tgt Ion:240 Resp: 328042

Ion Ratio Lower Upper

240 100

120 7.9 7.0 10.6



236 27.3 21.0 31.4




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

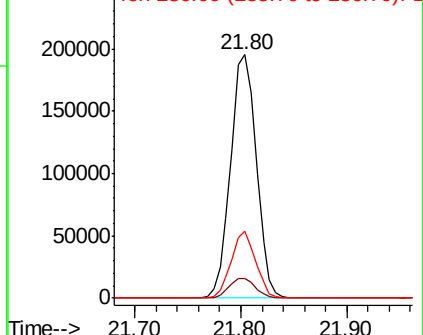



#77

Benzidine

Concen: 2.311 ng

RT: 20.11 min Scan# 2898

Delta R.T. 0.36 min

Lab File: BG039930.D

Acq: 14 Mar 2019 18:21

Instrument :

BNA_G

ClientSampleId :

RFK-RMAB-MW06-GW


Tot Ion:184 Resp: 24052

Ion Ratio Lower Upper

184 100

185 14.3 12.2 18.2

183 11.0 10.6 15.8



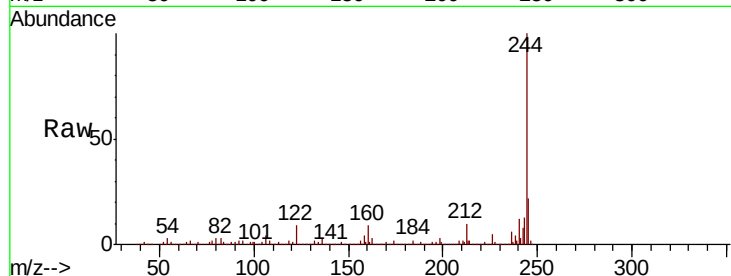


Abundance

Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

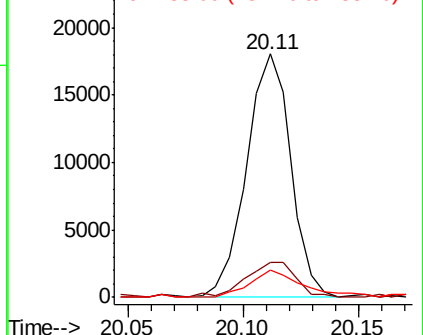

#78

Pyrene

Concen: 2.582 ng

RT: 19.92 min Scan# 2866

Delta R.T. -0.02 min

Lab File: BG039930.D

Acq: 14 Mar 2019 18:21


Tgt Ion:202 Resp: 55035

Ion Ratio Lower Upper

202 100

200 23.1 17.8 26.8

203 17.7 15.3 22.9






Abundance

Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

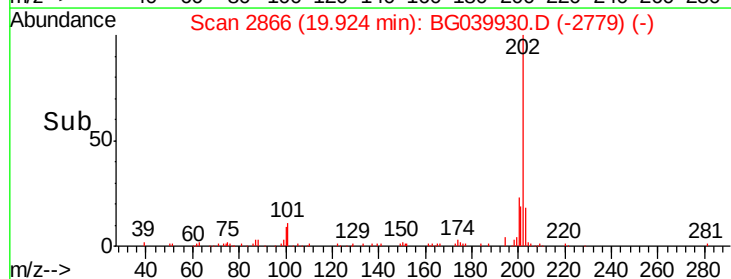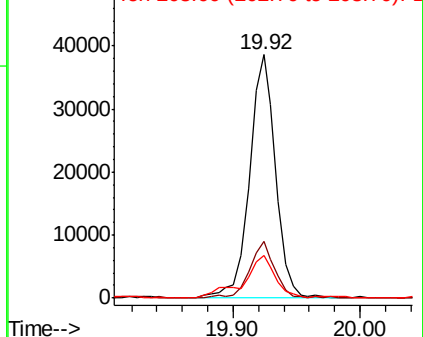



#79

Terphenyl-d14

Concen: 86.938 ng

RT: 20.11 min Scan# 2898

Delta R.T. -0.01 min

Lab File: BG039930.D

Acq: 14 Mar 2019 18:21

Instrument :

BNA_G

ClientSampleId :

RFK-RMAB-MW06-GW


Tot Ion:244 Resp: 1295273

Ion Ratio Lower Upper




244 100

212 9.6 7.3 10.9

122 9.5 8.4 12.6



Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

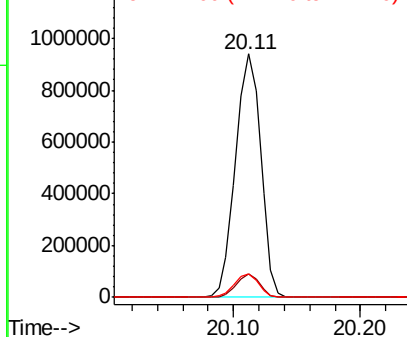

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.16 min Scan# 3758

Delta R.T. -0.04 min

Lab File: BG039930.D

Acq: 14 Mar 2019 18:21


Tgt Ion:264 Resp: 337225

Ion Ratio Lower Upper

264 100

260 23.9 18.2 27.4

265 23.1 18.5 27.7



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

