
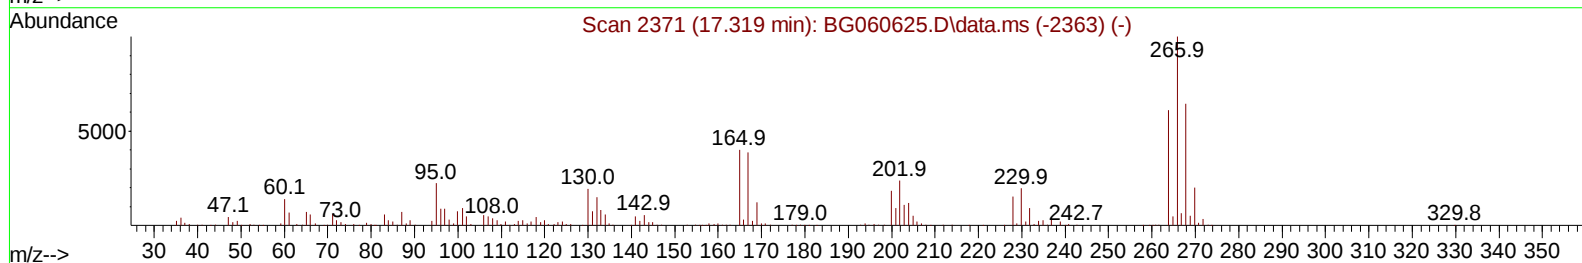
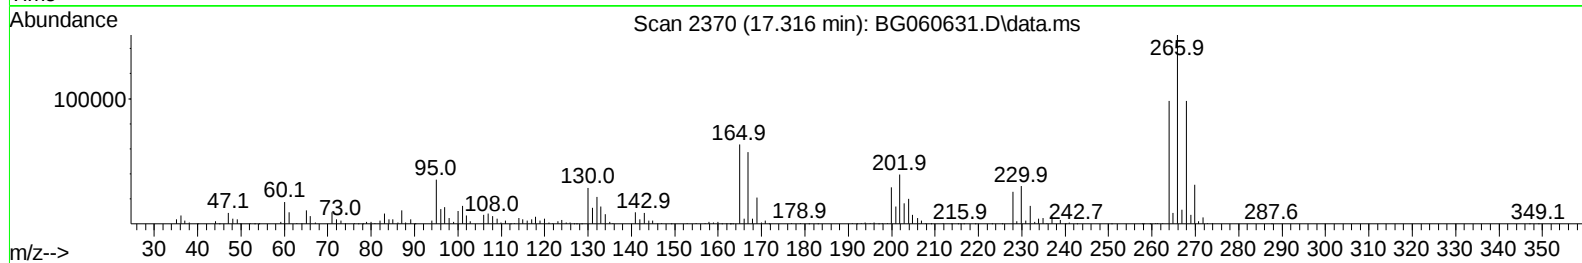


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031424\
Data File : BG060631.D
Acq On : 14 Mar 2024 9:44
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 14 12:23:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 00:45:22 2024
Response via : Initial Calibration

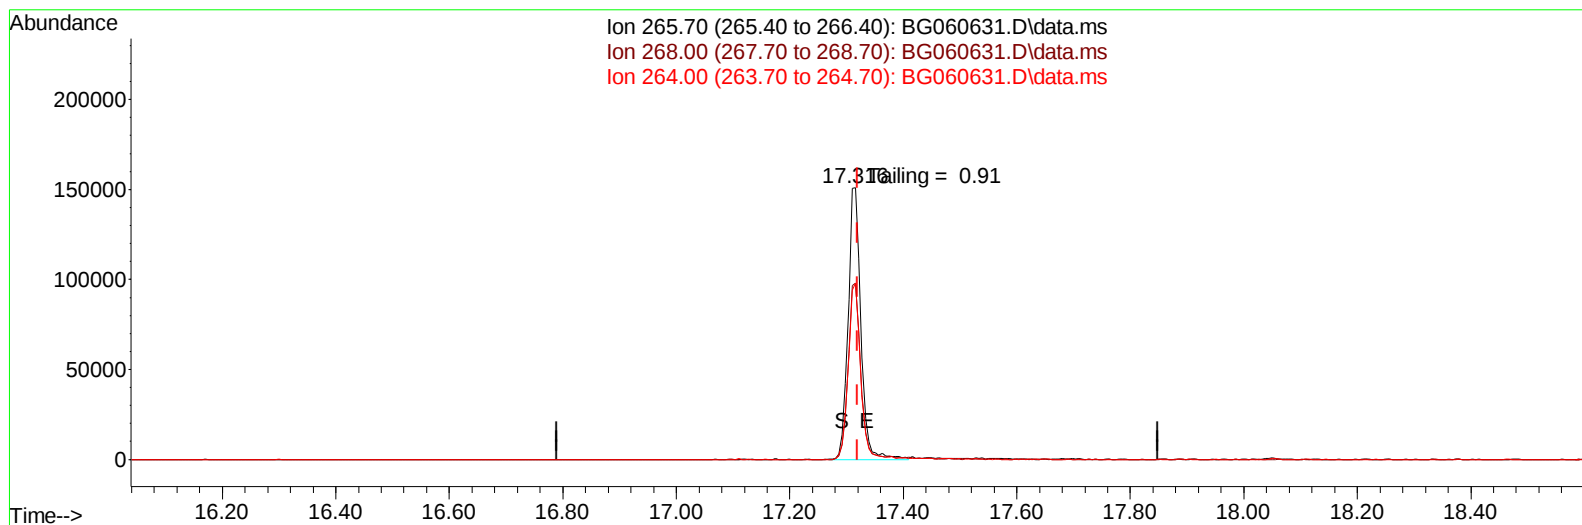

TIC: BG060631.D\data.ms

(70) Pentachlorophenol (C)




17.316min (-0.003) 241234.25 ng

response 238440

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	65.08
264.00	61.10	65.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031424\
Data File : BG060631.D
Acq On : 14 Mar 2024 9:44
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 14 12:23:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 00:45:22 2024
Response via : Initial Calibration

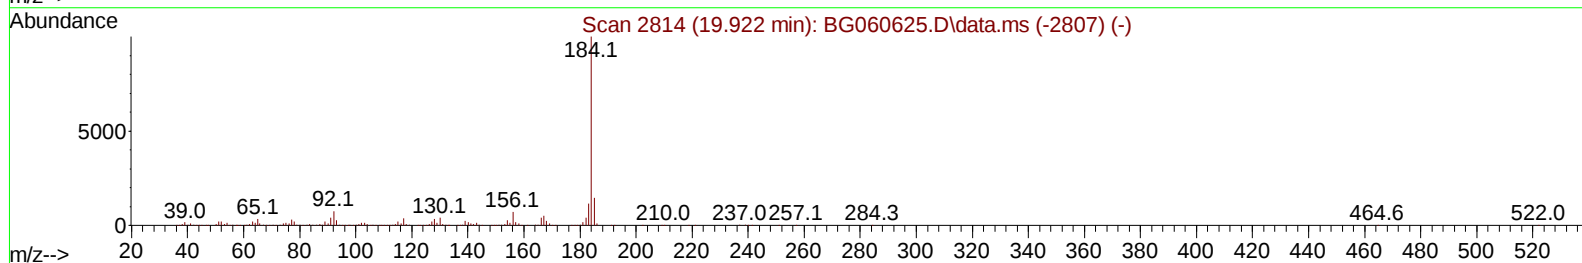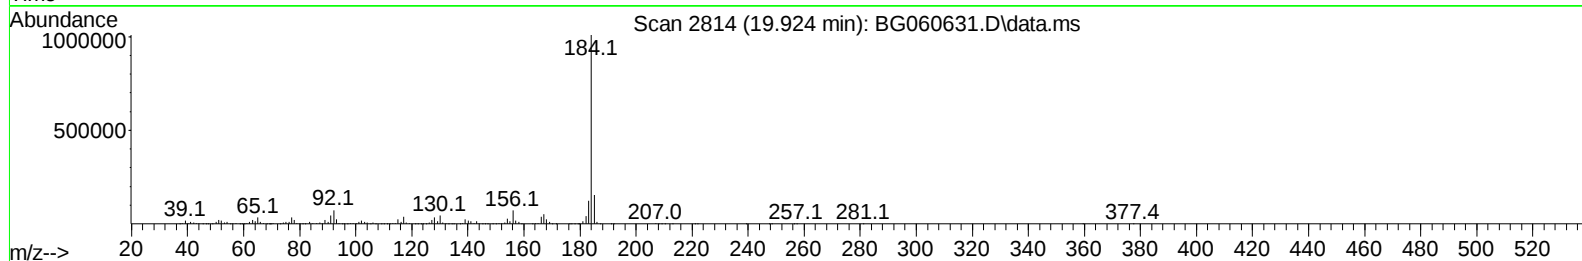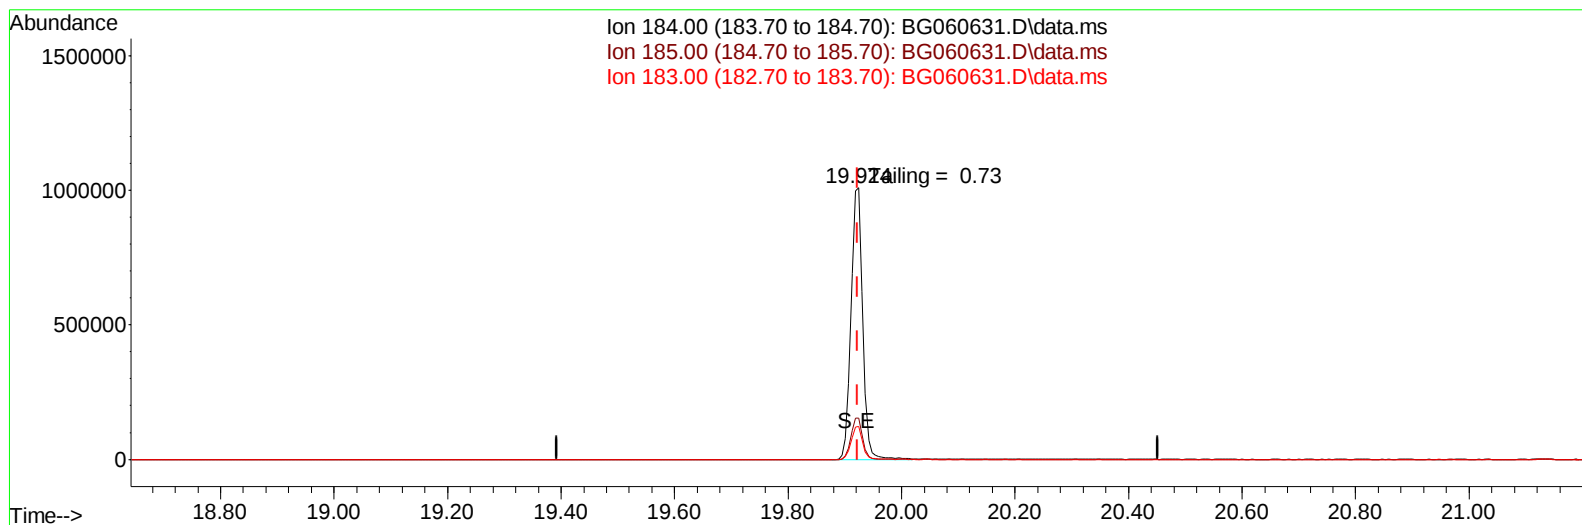

TIC: BG060631.D\data.ms

(77) Benzidine**19.924min (+ 0.002) 5207.67 ng****response 1443715**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	15.11
183.00	11.50	12.20
0.00	0.00	0.00