
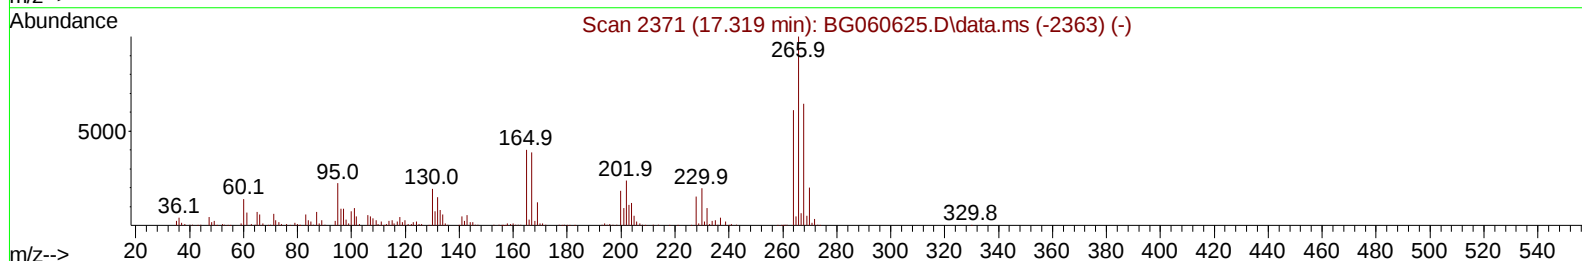
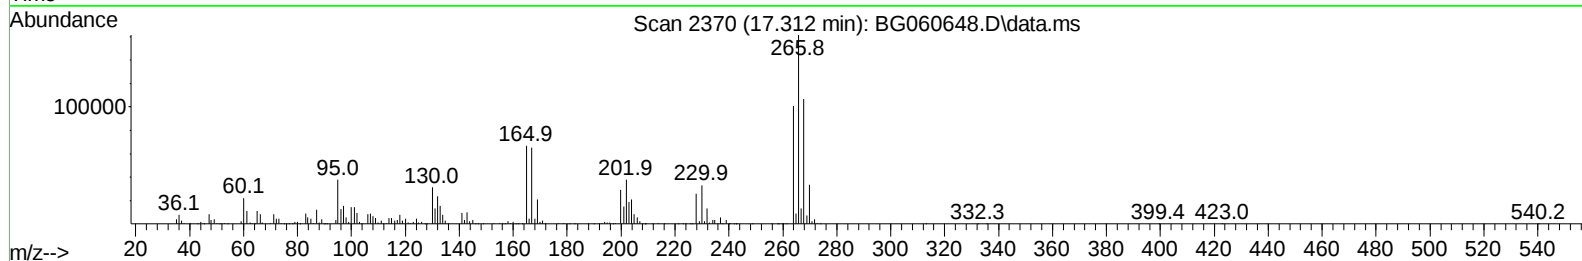


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031424\
Data File : BG060648.D
Acq On : 14 Mar 2024 21:59
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 02:26:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 00:45:22 2024
Response via : Initial Calibration

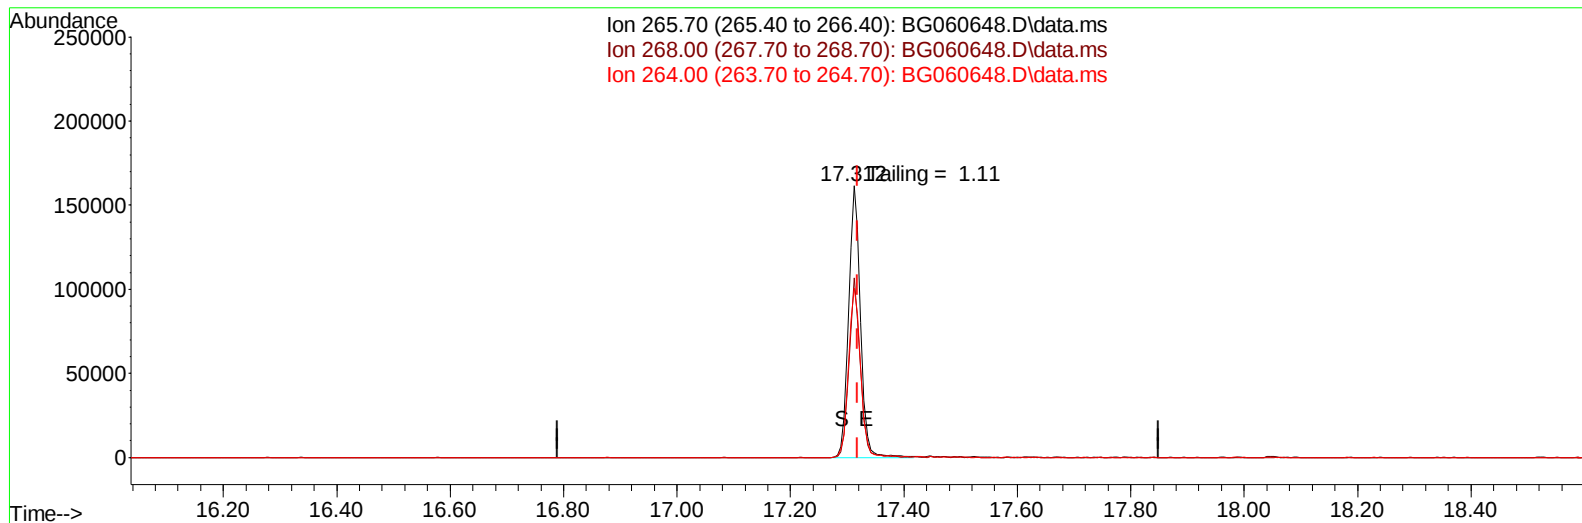

TIC: BG060648.D\data.ms

(70) Pentachlorophenol (C)




17.312min (-0.007) 359159.45 ng

response 233780

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	66.07
264.00	61.10	62.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031424\
Data File : BG060648.D
Acq On : 14 Mar 2024 21:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 02:26:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 00:45:22 2024
Response via : Initial Calibration

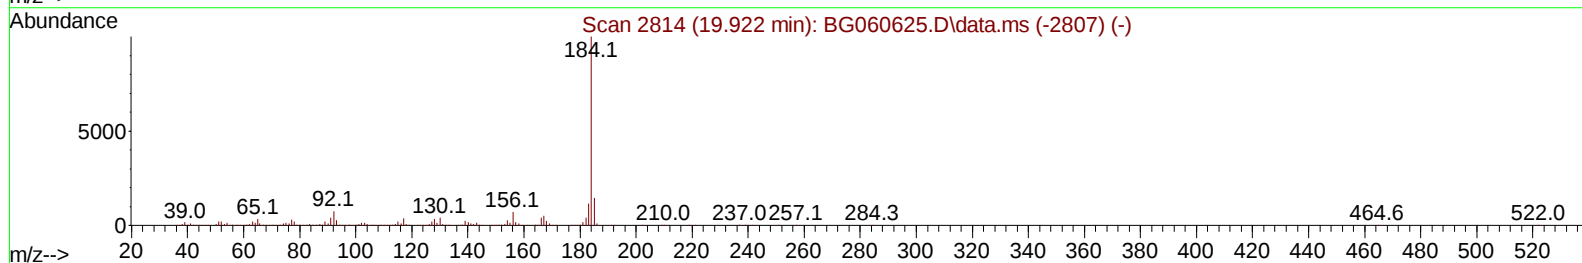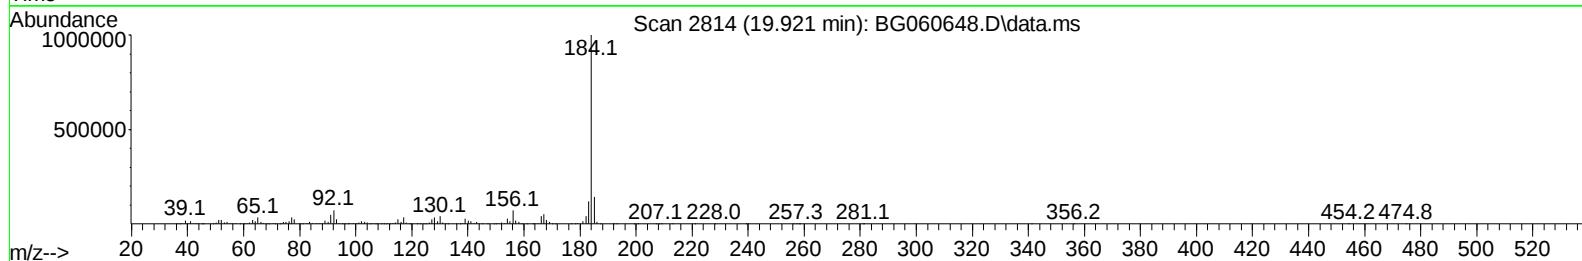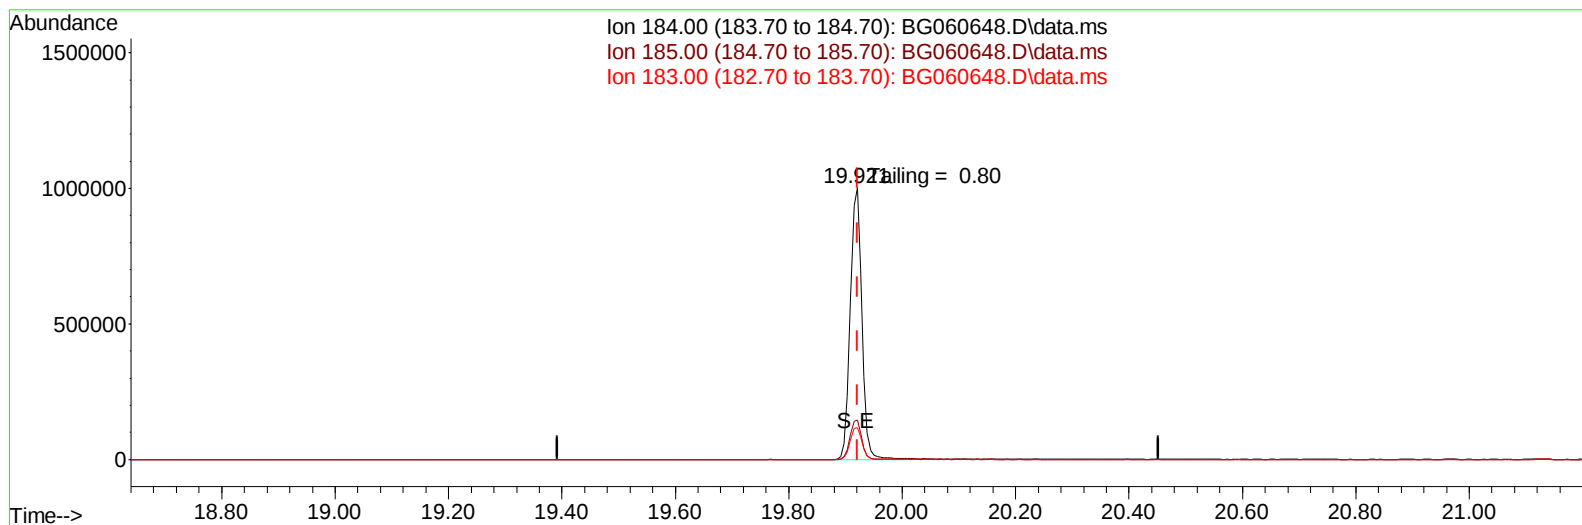

TIC: BG060648.D\data.ms

(77) Benzydine**19.921min (-0.001) 735570.01 ng****response 1421367**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.43
183.00	11.50	11.76
0.00	0.00	0.00