

Data Path : Z:\HPCHEM1\BNA G\DATA\BG031517\
 Data File : BG026258.D
 Acq On : 16 Mar 2017 6:49
 Operator : SJ/MA
 Sample : I2236-17
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DABJ3

Quant Time: Mar 16 07:37:58 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.3-EPA-BG021617MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 16 04:25:12 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	81659	20.00	ng/ul	0.00
2) Naphthalene-d8	10.86	136	429981	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.66	164	236481	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.39	188	509978	20.00	ng/ul	0.00
17) Chrysene-d12	21.64	240	535926	20.00	ng/ul	0.00
22) Perylene-d12	24.83	264	520636	20.00	ng/ul	0.01
System Monitoring Compounds						
7) Acenaphthylene-d8	14.36	160	400535	20.45	ng/ul	0.00
10) Fluorene-d10	15.64	176	293059	19.49	ng/ul	0.00
14) Anthracene-d10	17.49	188	428025	18.56	ng/ul	0.00
18) Pyrene-d10	19.76	212	466961	18.08	ng/ul	0.00
25) Benzo(a)pyrene-d12	24.60	264	435806	18.91	ng/ul	0.00
Target Compounds				Ovalue		
13) Phenanthrene	17.43	178	103481	3.80	ng/ul	99
16) Fluoranthene	19.43	202	209056	6.99	ng/ul	98
19) Pyrene	19.79	202	177700	5.48	ng/ul#	95
20) Benzo(a)anthracene	21.62	228	101885	3.38	ng/ul	94
21) Chrysene	21.68	228	103754	3.60	ng/ul	98
23) Benzo(b)fluoranthene	23.81	252	154243	5.13	ng/ul#	92
24) Benzo(k)fluoranthene	23.87	252	51489	1.77	ng/ul#	91
26) Benzo(a)pyrene	24.67	252	98282	3.38	ng/ul#	93
27) Indeno(1,2,3-cd)pyrene	28.45	276	42946	1.26	ng/ul#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG031517\
Data File : BG026258.D
Acq On : 16 Mar 2017 6:49
Operator : SJ/MA
Sample : I2236-17
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DABJ3

Quant Time: Mar 16 07:37:58 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.3-EPA-BG021617MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 16 04:25:12 2017
Response via : Initial Calibration

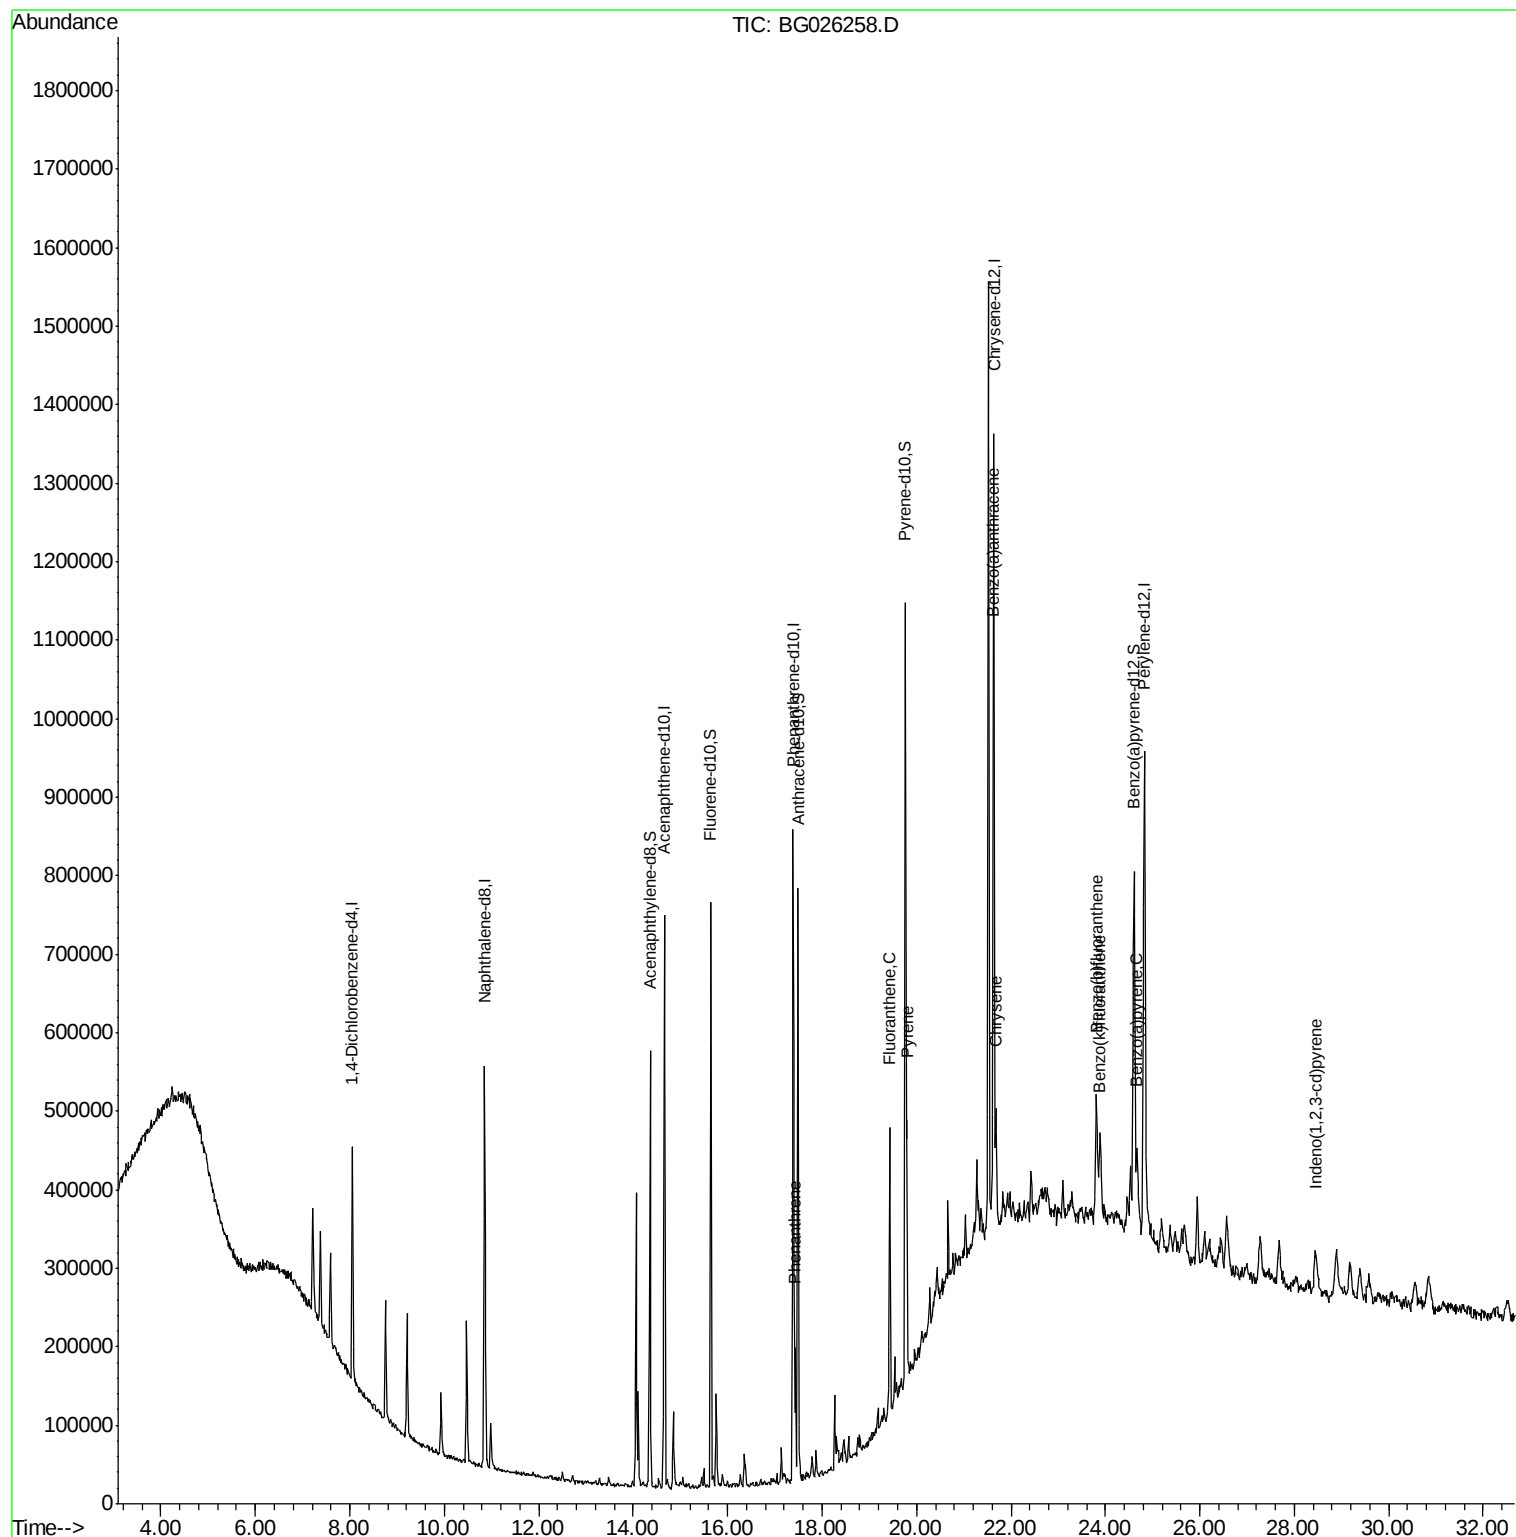

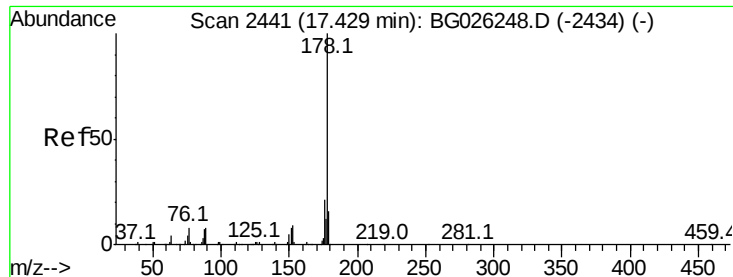

#13

Phenanthrene

Concen: 3.80 ng/ul

RT: 17.43 min Scan# 2441

Delta R.T. 0.00 min

Lab File: BG026258.D

Acq: 16 Mar 2017 6:49

Instrument :


BNA_G

ClientSampleId :

DABJ3

Tot Ion:178 Resp: 103481




Ion	Ratio	Lower	Upper
178	100		
179	14.7	12.3	18.5
176	18.3	15.1	22.7

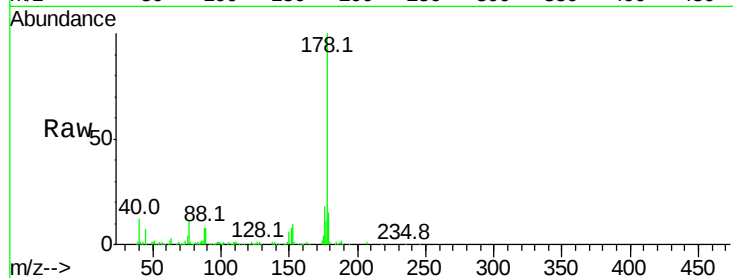

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

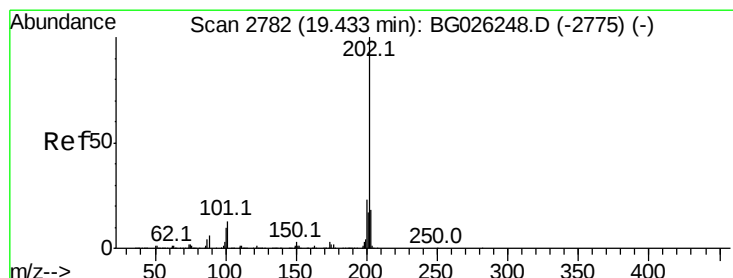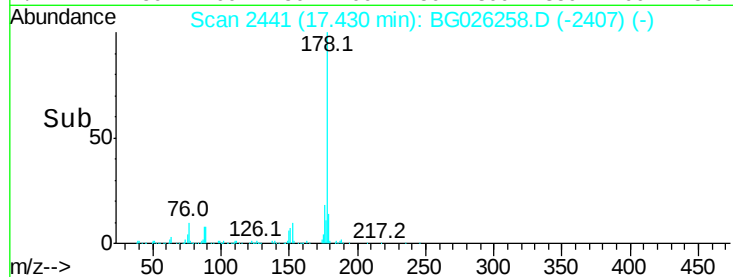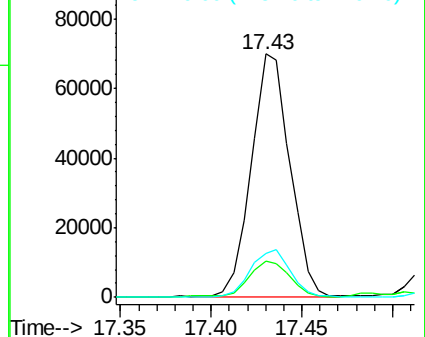

#16

Fluoranthene

Concen: 6.99 ng/ul

RT: 19.43 min Scan# 2782


Delta R.T. 0.00 min

Lab File: BG026258.D

Acq: 16 Mar 2017 6:49

Tgt Ion:202 Resp: 209056



Ion	Ratio	Lower	Upper
202	100		
101	12.8	9.9	14.9
100	10.6	7.4	11.0

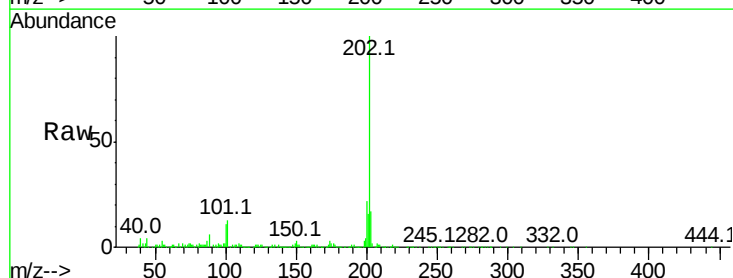


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

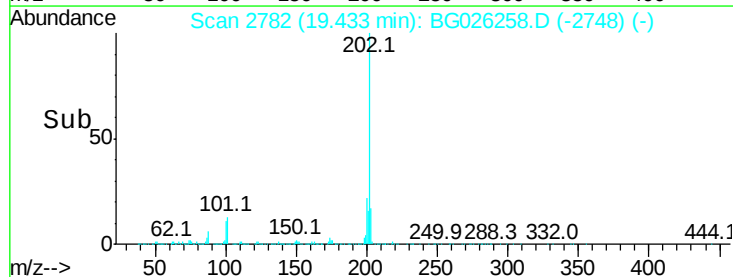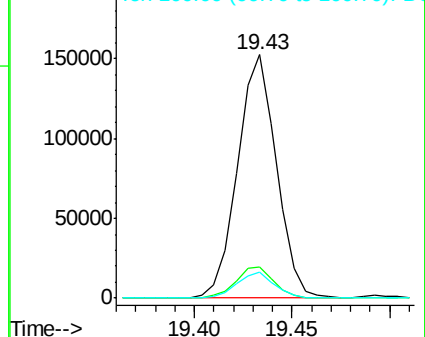

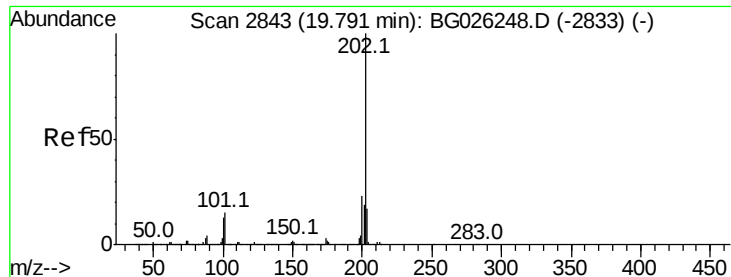

#19

Pvrene

Concen: 5.48 ng/ul

RT: 19.79 min Scan# 2843

Delta R.T. 0.00 min

Lab File: BG026258.D

Acq: 16 Mar 2017 6:49

Instrument :

BNA_G

ClientSampleId :

DABJ3


Tot Ion:202 Resp: 177700

Ion Ratio Lower Upper

202 100

101 14.3 11.0 16.4




100 13.9 8.1 12.1#

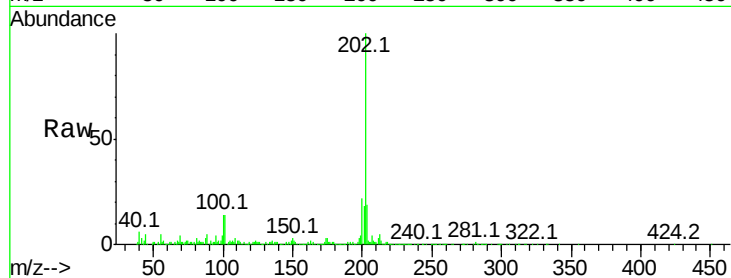

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

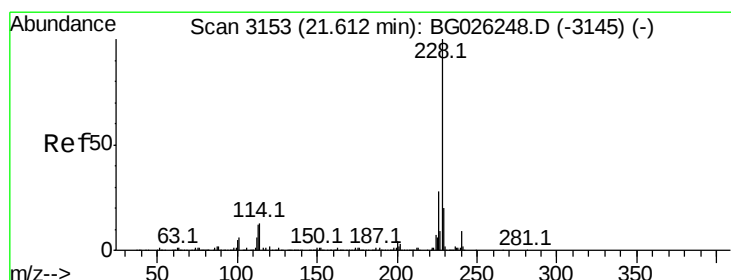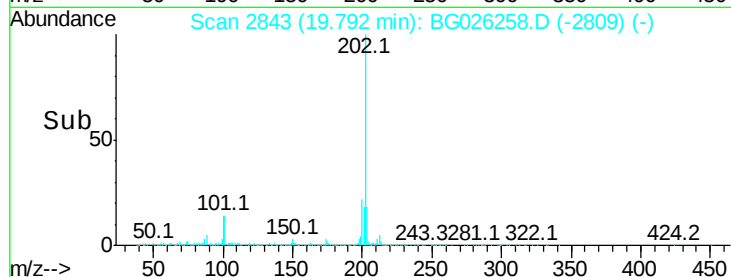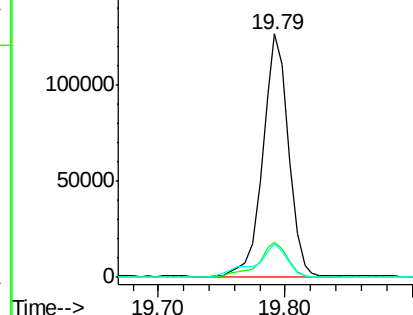

#20

Benzo(a)anthracene

Concen: 3.38 ng/ul

RT: 21.62 min Scan# 3154

Delta R.T. 0.01 min

Lab File: BG026258.D

Acq: 16 Mar 2017 6:49


Tgt Ion:228 Resp: 101885

Ion Ratio Lower Upper

228 100

229 22.3 15.7 23.5



226 29.5 21.1 31.7

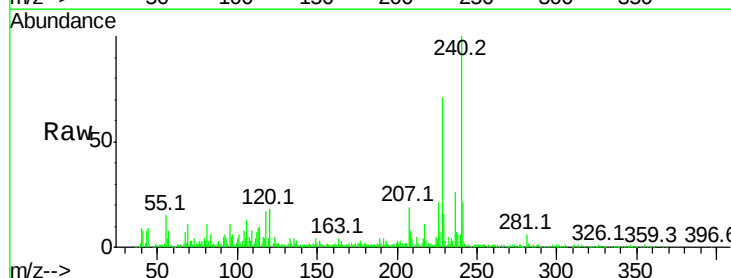


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

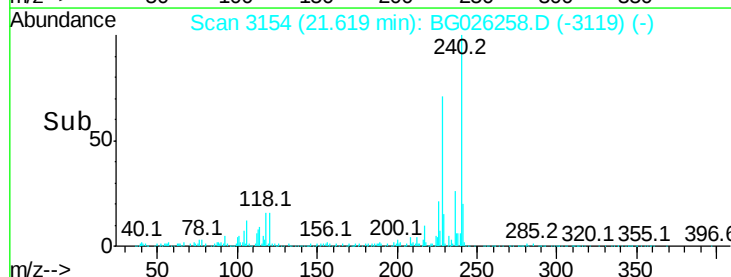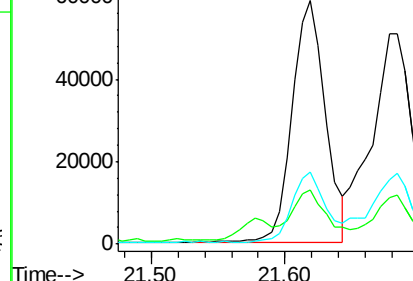

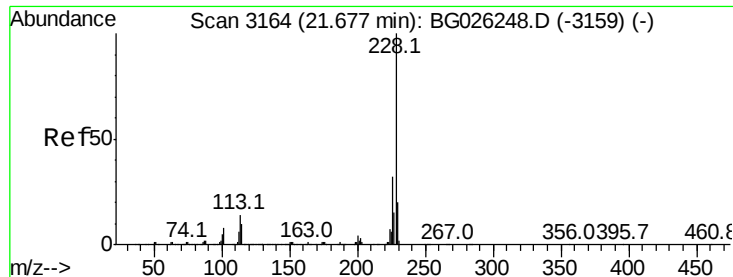

#21

Chrysene

Concen: 3.60 ng/ul

RT: 21.68 min Scan# 3164

Delta R.T. 0.00 min

Lab File: BG026258.D

Acq: 16 Mar 2017 6:49

Instrument :






BNA_G

ClientSampleId :

DABJ3

Tot Ion:228 Resp: 103754

Ion	Ratio	Lower	Upper
228	100		
226	30.7	24.5	36.7
229	22.4	15.8	23.8

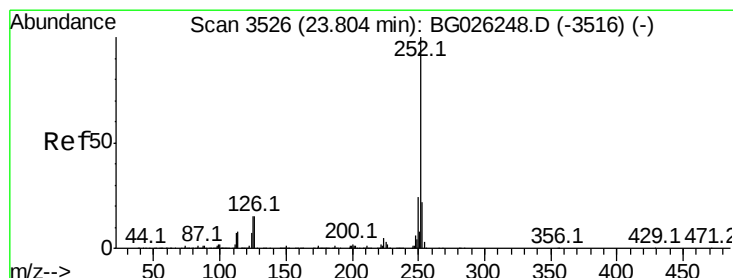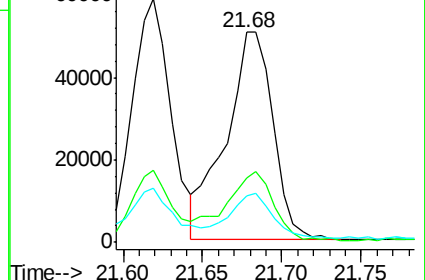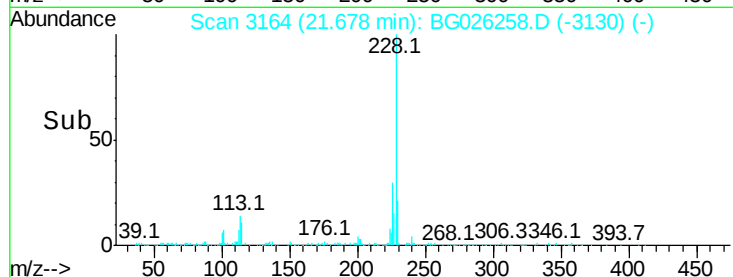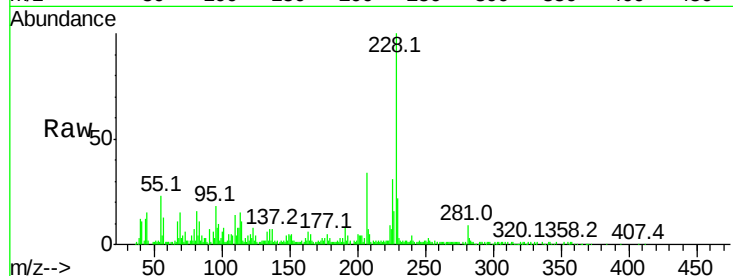

#23

Benzo(b)fluoranthene

Concen: 5.13 ng/ul

RT: 23.81 min Scan# 3527





Delta R.T. 0.01 min


Lab File: BG026258.D

Acq: 16 Mar 2017 6:49

Tgt Ion:252 Resp: 154243

Ion	Ratio	Lower	Upper
252	100		
253	23.7	18.0	27.0
125	17.1	8.0	12.0

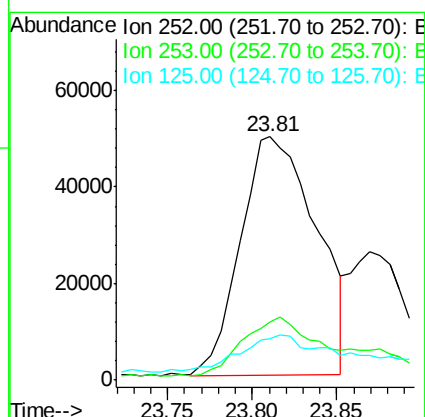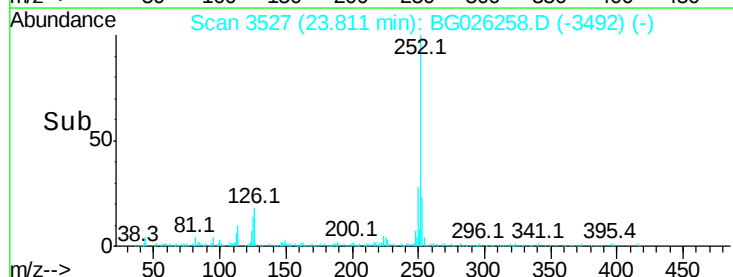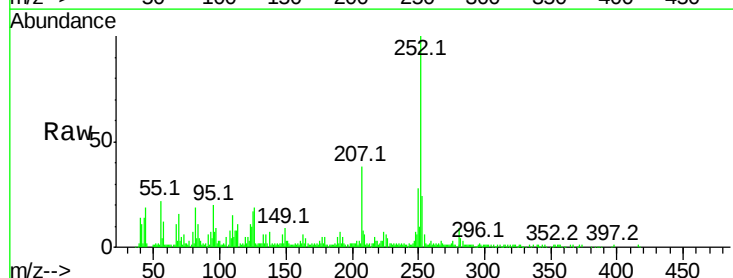

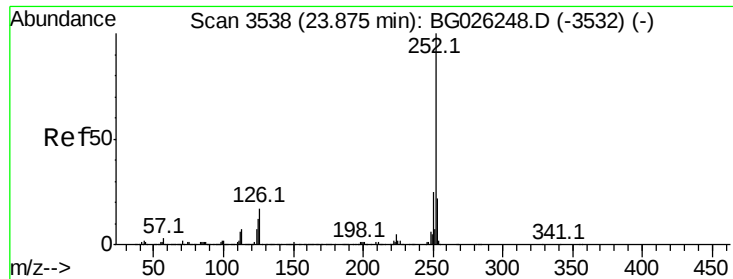

#24

Benzo(k)fluoranthene

Concen: 1.77 ng/ul

RT: 23.87 min Scan# 3537

Delta R.T. -0.01 min

Lab File: BG026258.D

Acq: 16 Mar 2017 6:49

Instrument :

BNA_G

ClientSampleId :

DABJ3





Tot Ion:252 Resp: 51489

Ion Ratio Lower Upper

252 100

253 23.2 18.0 27.0

125 19.3 8.1 12.1#

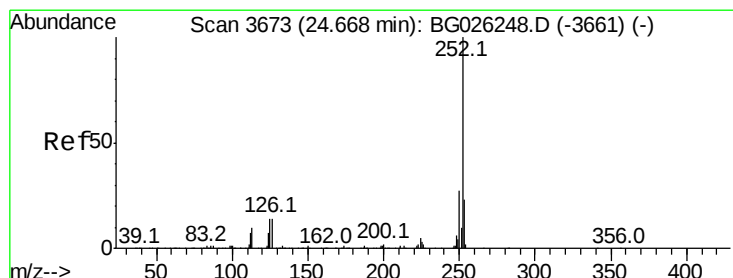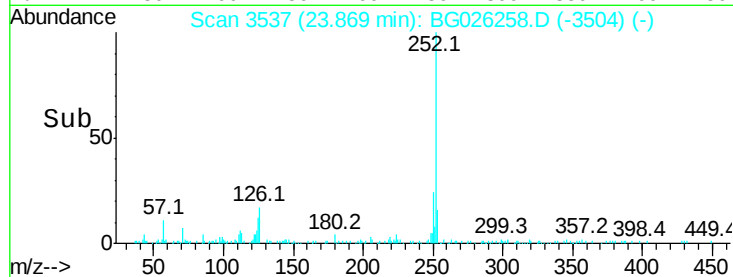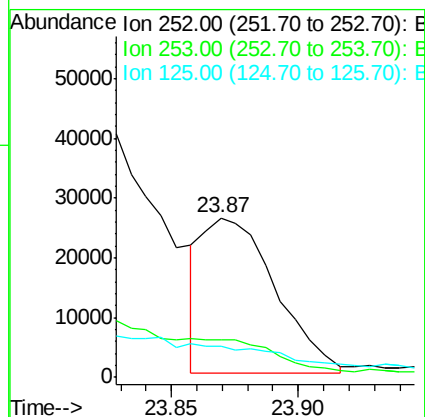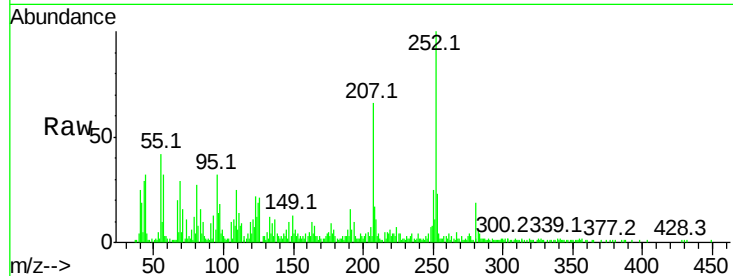

#26

Benzo(a)pyrene

Concen: 3.38 ng/ul

RT: 24.67 min Scan# 3673

Delta R.T. 0.00 min

Lab File: BG026258.D

Acq: 16 Mar 2017 6:49




Tgt Ion:252 Resp: 98282




Ion Ratio Lower Upper

252 100

253 21.6 17.2 25.8

125 18.0 8.2 12.4#

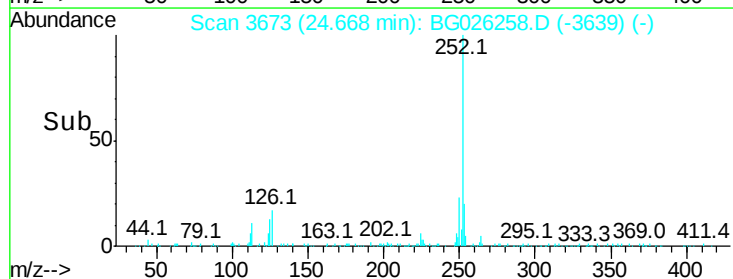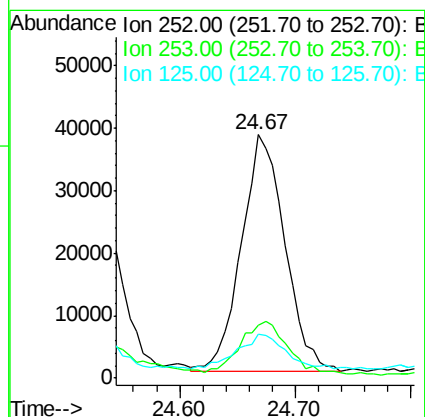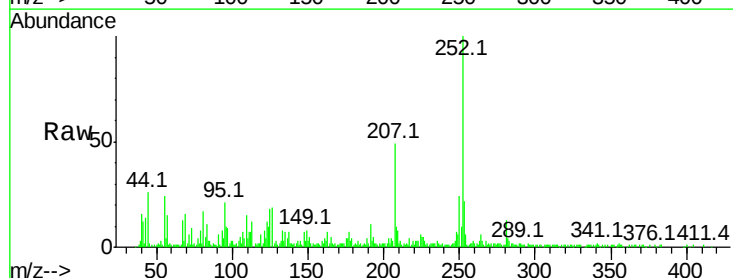

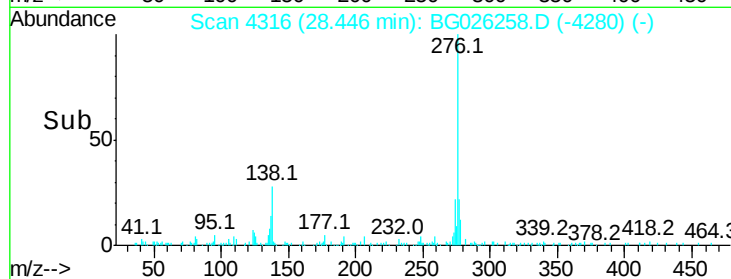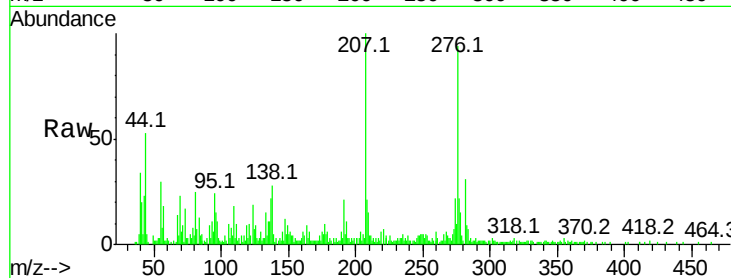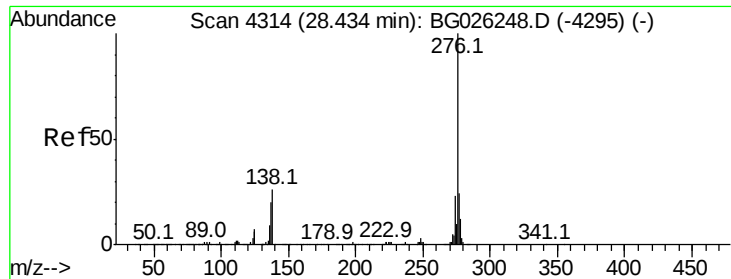

#27

Indeno(1,2,3-cd)pvrene

Concen: 1.26 ng/ul

RT: 28.45 min Scan# 4316

Delta R.T. 0.01 min

Lab File: BG026258.D

Acq: 16 Mar 2017 6:49

Instrument :

BNA_G

ClientSampleId :

DABJ3

Tot Ion:276 Resp: 42946

Ion Ratio Lower Upper

276 100

138 29.7 14.4 21.6#

277 23.8 18.0 27.0

